


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV033120\
 Data File : VV015302.D
 Acq On : 31 Mar 2020 09:17
 Operator : SY/MD
 Sample : BFB75
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB75

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM033020WMA.M
 Title : VOC Analysis
 Last Update : Mon Mar 09 14:00:26 2020

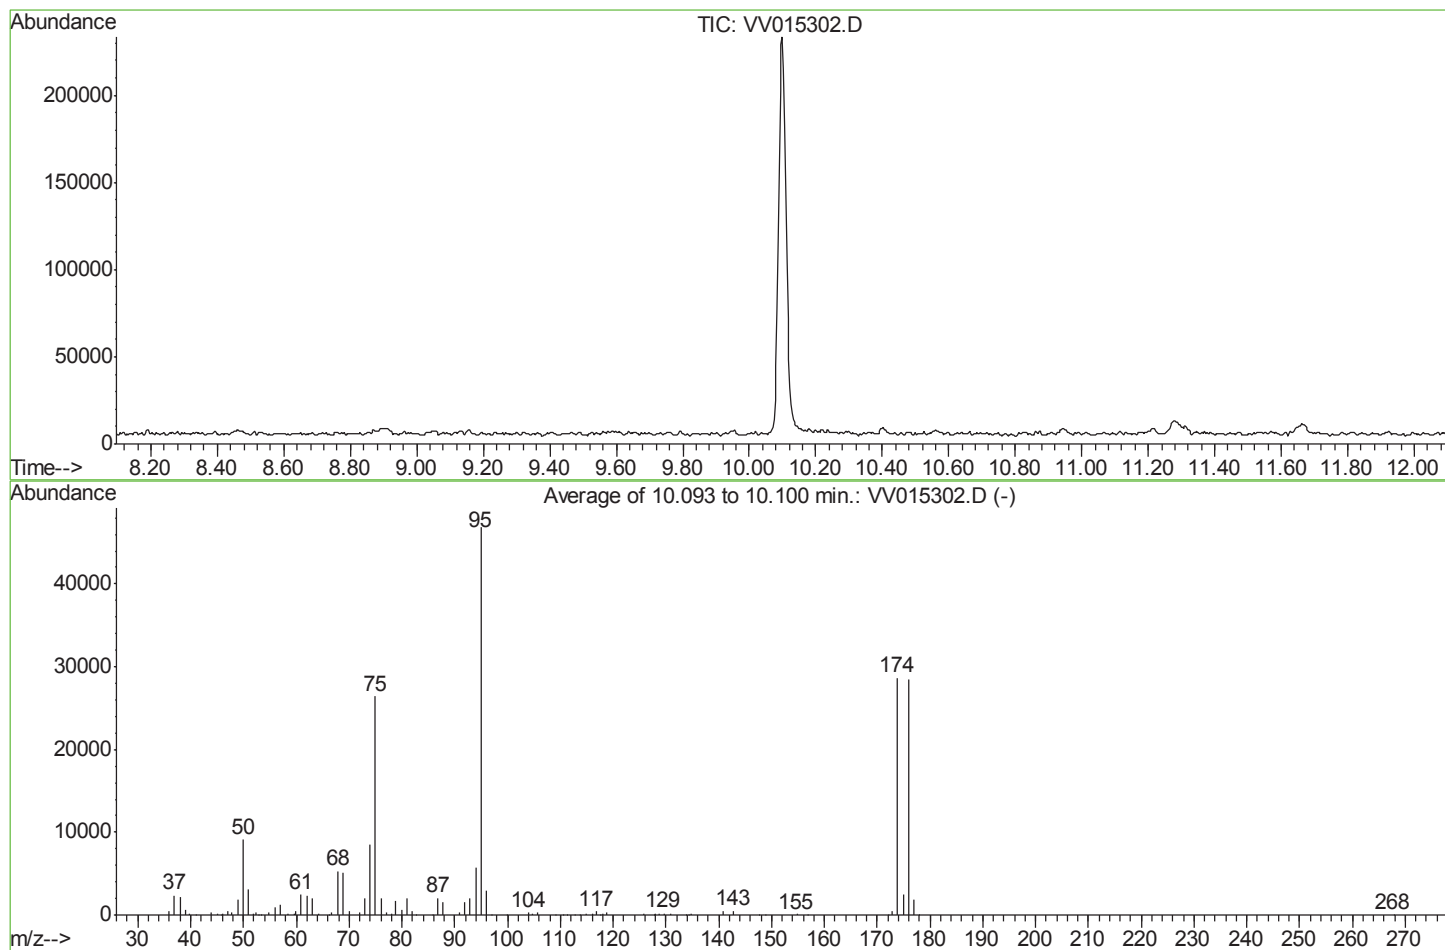

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.4	9091	PASS
75	95	30	80	56.4	26410	PASS
95	95	100	100	100.0	46837	PASS
96	95	5	9	6.2	2927	PASS
173	174	0.00	2	1.5	444	PASS
174	95	50	120	61.2	28648	PASS
175	174	5	9	8.4	2414	PASS
176	174	95	101	99.5	28501	PASS
177	176	5	9	6.5	1850	PASS

m/z	Abundance
36.00	458.0
36.90	2400.0
38.00	2116.0
39.00	914.0
39.80	854.0
41.00	349.0
42.10	117.0
43.00	251.0
44.00	1328.0
45.00	474.0
46.00	165.0
47.00	486.0
47.70	310.0
49.00	1734.0
50.00	8242.0
51.00	2936.0
51.80	221.0
52.30	191.0
52.90	113.0
54.80	403.0
55.90	948.0
57.00	1268.0
58.40	146.0
59.70	349.0
60.00	360.0
60.90	2208.0
62.00	2216.0
63.00	1849.0
64.10	210.0
66.70	371.0
68.00	4924.0
69.00	4721.0
70.10	518.0
72.00	264.0
72.90	1816.0
74.00	7983.0
75.00	23960.0
76.00	1986.0
77.00	288.0
78.00	192.0
78.80	1776.0
80.00	717.0
80.90	1816.0
81.90	361.0
82.60	153.0
86.90	1959.0
87.80	1022.0
90.90	348.0
91.90	1480.0
93.00	1723.0
94.00	5509.0
95.00	43832.0
96.00	2833.0
96.80	149.0
104.00	281.0
104.90	117.0
105.80	268.0
110.60	114.0
111.10	107.0
113.70	115.0
114.90	153.0
116.00	178.0
116.80	425.0
118.10	222.0
118.80	206.0
125.80	113.0
127.70	203.0
128.70	149.0
129.60	198.0
130.90	143.0
134.40	112.0
134.90	115.0
140.80	389.0
142.80	483.0
147.70	143.0
172.00	121.0
172.90	440.0
173.90	25144.0
174.90	2264.0
175.90	24616.0
176.90	1596.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
35.90	461.0
37.00	2513.0
38.00	2309.0
39.00	824.0
39.80	748.0
40.80	163.0
42.00	109.0
43.00	321.0
44.00	1305.0
45.00	435.0
46.10	156.0
46.90	558.0
47.70	418.0
49.00	2005.0
50.00	9616.0
51.00	3117.0
51.80	204.0
52.30	280.0
53.30	196.0
54.90	392.0
55.90	999.0
56.90	1484.0
58.30	126.0
59.90	597.0
61.00	2612.0
61.90	2380.0
63.00	2001.0
64.20	188.0
66.30	177.0
66.80	246.0
67.90	5491.0
68.90	5341.0
70.00	533.0
71.80	271.0
72.90	2500.0
74.00	8884.0
75.00	27880.0
76.00	1887.0
77.00	449.0
78.10	177.0
78.80	1660.0
79.90	532.0
80.90	2117.0
81.90	440.0
82.70	143.0
83.90	115.0
86.90	2180.0
87.90	1988.0
90.90	383.0
91.90	1709.0
92.90	2161.0
94.00	5761.0
95.00	48304.0
96.00	2943.0
97.00	132.0
99.90	125.0
104.10	322.0
104.70	172.0
105.60	234.0
112.70	121.0
114.80	108.0
116.00	248.0
116.80	494.0
117.60	202.0
118.00	162.0
118.80	273.0
125.90	131.0
128.00	266.0
128.60	128.0
129.60	155.0
133.90	103.0
134.80	209.0
140.90	604.0
142.70	535.0
148.90	121.0
154.90	142.0
156.80	103.0
173.00	439.0
173.90	31144.0
174.90	2462.0
175.90	31280.0
176.90	2077.0
178.00	129.0
267.80	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
36.00	512.0
37.00	2550.0
38.00	2270.0
39.00	840.0
39.80	808.0
41.00	241.0
42.10	126.0
43.00	279.0
44.00	1357.0
45.00	481.0
45.70	110.0
46.00	137.0
47.00	568.0
47.60	400.0
49.00	1954.0
50.00	9417.0
51.00	3235.0
51.80	238.0
52.30	271.0
54.90	432.0
55.90	1070.0
57.00	1379.0
58.30	160.0
60.00	492.0
61.00	2584.0
62.00	2377.0
63.00	2011.0
64.20	214.0
66.80	341.0
68.00	5547.0
68.90	5242.0
70.00	560.0
72.00	259.0
72.90	2137.0
74.00	8868.0
75.00	27392.0
76.00	2120.0
77.00	412.0
78.00	195.0
78.80	1778.0
79.90	656.0
80.90	2085.0
81.90	441.0
82.60	154.0
83.90	110.0
85.80	102.0
86.90	2112.0
87.90	1505.0
90.90	387.0
91.90	1732.0
93.00	2104.0
94.00	6025.0
95.00	48376.0
96.00	3005.0
96.90	157.0
104.00	326.0
104.70	135.0
105.80	264.0
109.10	120.0
111.20	111.0
112.70	125.0
114.90	141.0
116.00	210.0
116.90	454.0
118.10	199.0
118.80	274.0
125.80	133.0
127.90	194.0
128.70	128.0
129.60	174.0
130.90	117.0
134.40	104.0
134.90	182.0
140.90	516.0
142.90	522.0
154.90	139.0
156.70	101.0
172.90	455.0
173.90	29656.0
174.90	2517.0
175.90	29608.0
176.90	1878.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
36.80	136.0
37.70	124.0
39.00	169.0
39.80	602.0
40.80	197.0
42.00	263.0
42.90	284.0
44.00	1039.0
45.10	245.0
48.20	140.0
54.80	146.0
56.20	184.0
57.10	151.0
64.90	184.0
67.00	210.0
73.00	135.0
73.80	113.0
76.70	170.0
82.80	140.0
83.90	236.0
85.50	105.0
88.60	128.0
92.10	126.0
97.00	101.0
240.50	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75