

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW033121\
 Data File : VW020819.D
 Acq On : 31 Mar 2021 10:36
 Operator : SY/MD
 Sample : VSTD0.0536
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.05302

Quant Time: Apr 01 04:04:08 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM033121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 01 04:03:39 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Difluorobenzene	5.639	114	5270	0.50 ug/L	0.00
5) Chlorobenzene-d5	8.864	117	5181	0.50 ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	2832	0.50 ug/L	0.00
System Monitoring Compounds					
2) Vinyl Chloride-d3	1.303	65	222	0.04 ug/L	0.00
4) 1,2-Dichloroethane-d4	5.066	65	195	0.05 ug/L	0.02
7) 1,2-Dichloropropane-d6	6.069	67	192	0.04 ug/L	0.00
8) Toluene-d8	7.332	98	587	0.05 ug/L	0.02
10) 1,1,2,2-Tetrachloroeth...	10.216	84	142	0.05 ug/L	0.00
Target Compounds					
3) Vinyl chloride	1.310	62	190	0.04 ug/L	Qvalue # 55
6) Trichloroethene	5.925	95	198	0.05 ug/L	91
9) 1,2-Dibromoethane	8.369	107	107	0.04 ug/L	Qvalue # 81
12) 1,2,3-Trichloropropane	10.267	75	117	0.05 ug/L	96
13) 1,2-Dibromo-3-chloropr...	12.427	75	28	0.07 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033121\
Data File : VV020819.D
Acq On : 31 Mar 2021 10:36
Operator : SY/MD
Sample : VSTD0.0536
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.05302

Quant Time: Apr 01 04:04:08 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM033121.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 01 04:03:39 2021
Response via : Initial Calibration




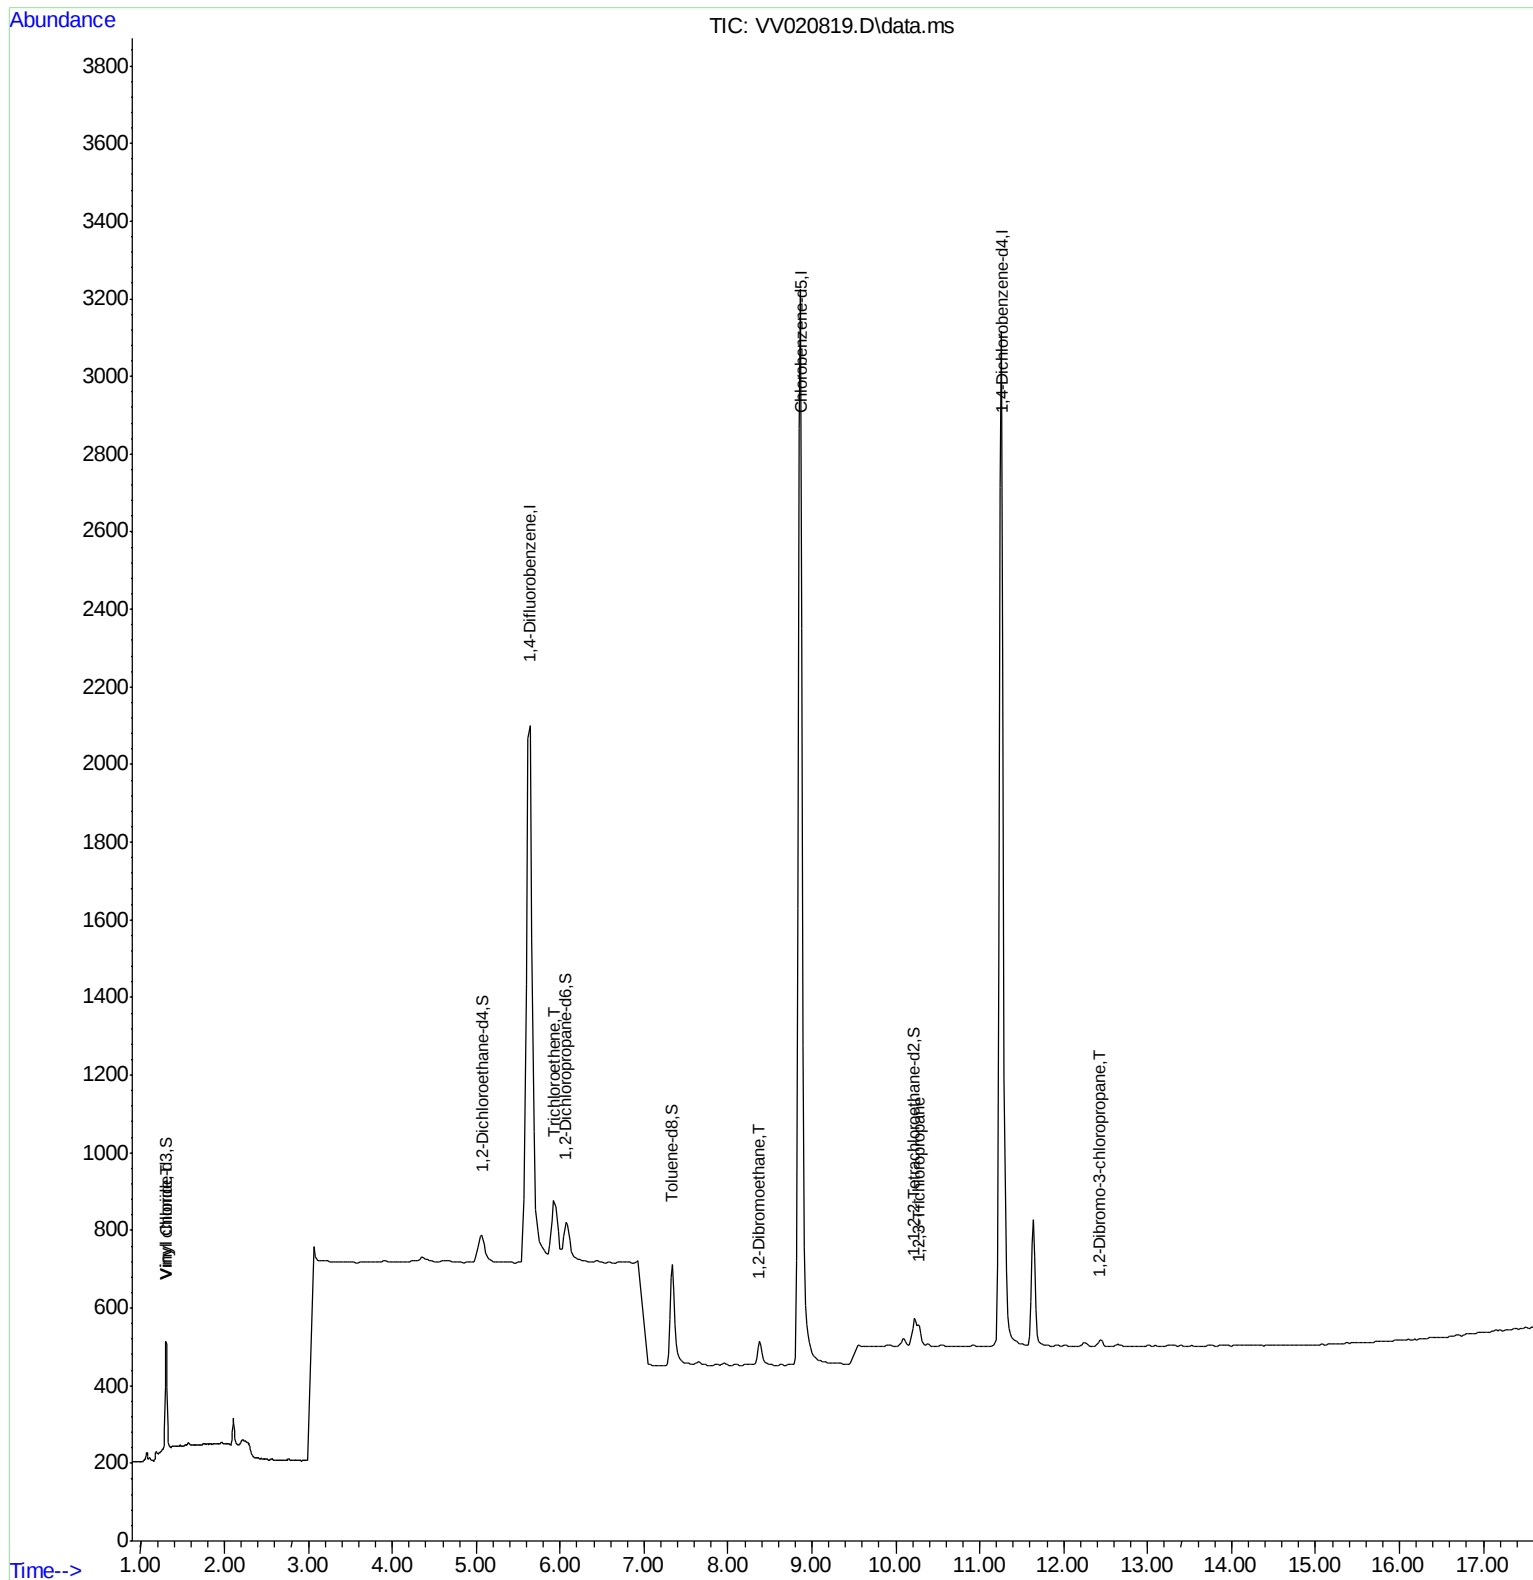


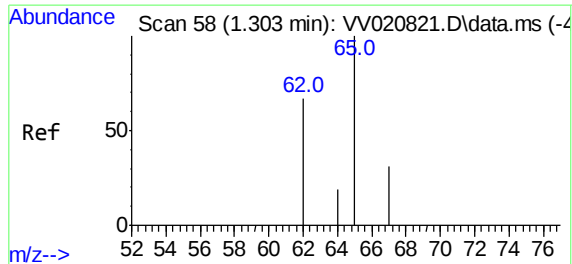

#3
Vinyl chloride
Concen: 0.04 ug/L
RT: 1.310 min Scan# 59
Delta R.T. 0.007 min
Lab File: VV020819.D
Acq: 31 Mar 2021 10:36




Instrument :
MSVOA_V
ClientSampleId :
VSTD0.05302


Tgt Ion: 62 Resp: 190
Ion Ratio Lower Upper
62 100
64 63.6 25.8 47.8#

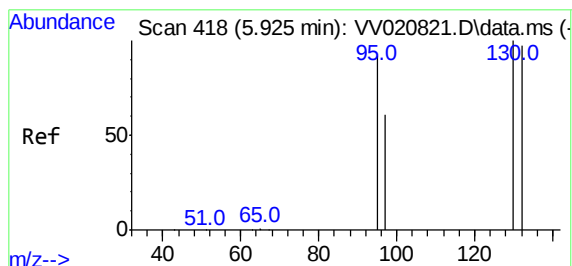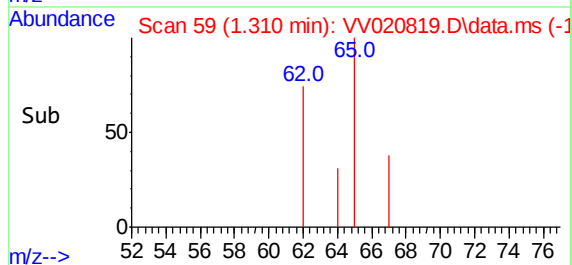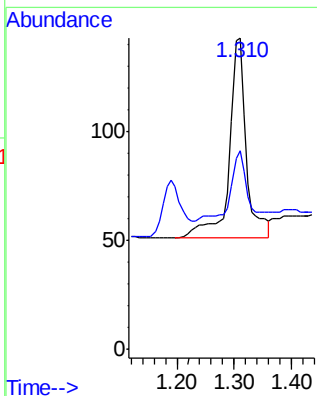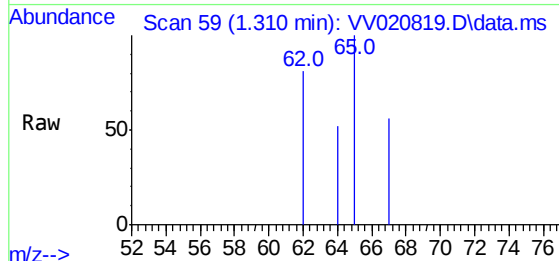

#6
Trichloroethene
Concen: 0.05 ug/L
RT: 5.925 min Scan# 418
Delta R.T. 0.000 min
Lab File: VV020819.D
Acq: 31 Mar 2021 10:36

Tgt Ion: 95 Resp: 198
Ion Ratio Lower Upper
95 100
97 82.4 48.5 90.1
132 97.8 73.0 135.6
130 100.0 75.0 139.2


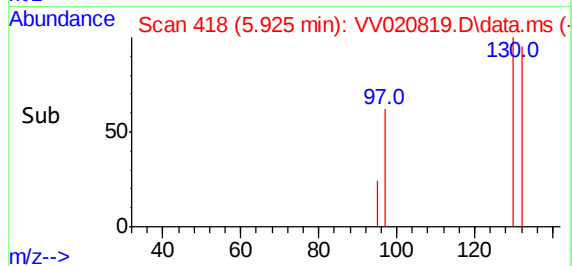
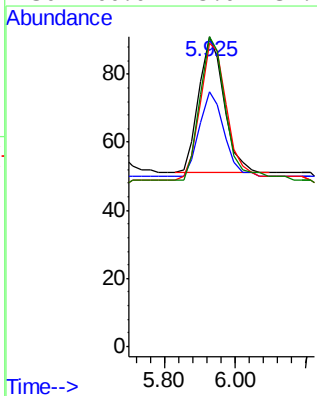
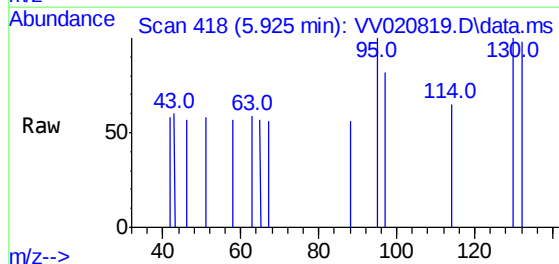


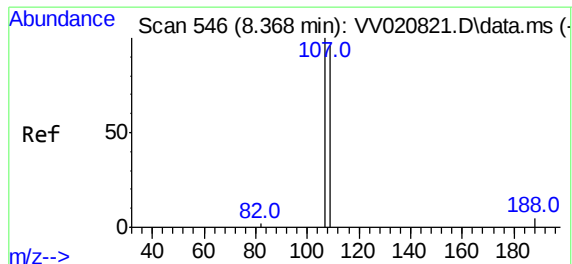

#9
1,2-Dibromoethane
Concen: 0.04 ug/L
RT: 8.369 min Scan# 546
Delta R.T. 0.000 min
Lab File: VV020819.D
Acq: 31 Mar 2021 10:36




Instrument :
MSVOA_V
ClientSampleId :
VSTD0.05302


Tgt Ion:107 Resp: 107
Ion Ratio Lower Upper
107 100
109 100.0 67.8 126.0
188 63.3 13.4 20.2#

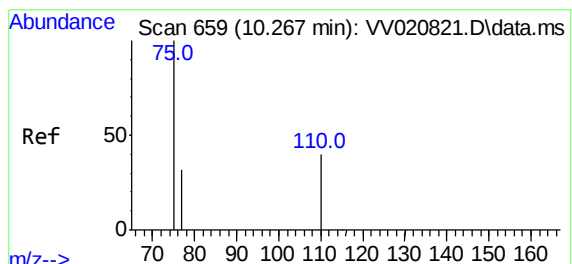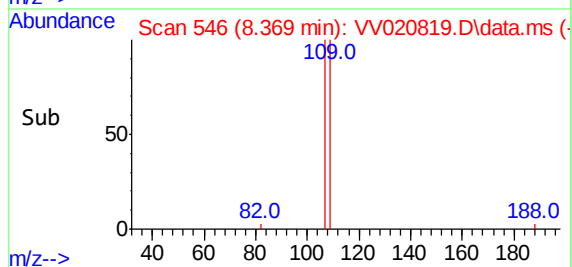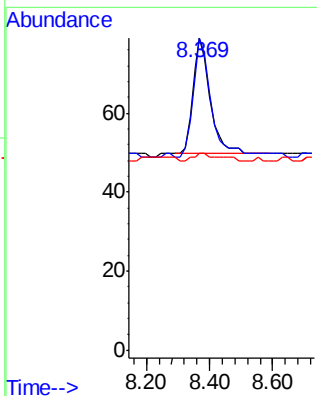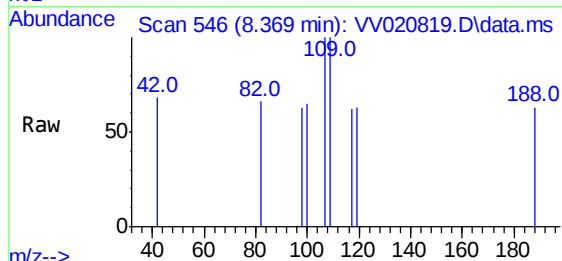

#12
1,2,3-Trichloropropane
Concen: 0.05 ug/L
RT: 10.267 min Scan# 659
Delta R.T. 0.000 min
Lab File: VV020819.D
Acq: 31 Mar 2021 10:36


Tgt Ion: 75 Resp: 117
Ion Ratio Lower Upper
75 100
110 42.7 35.5 53.3
77 36.8 27.1 40.7

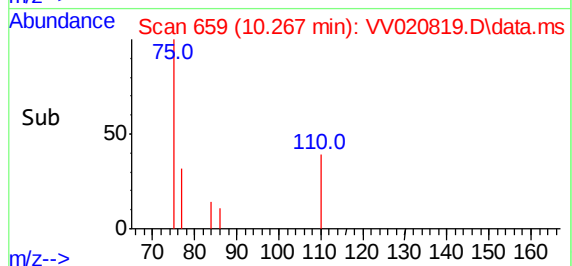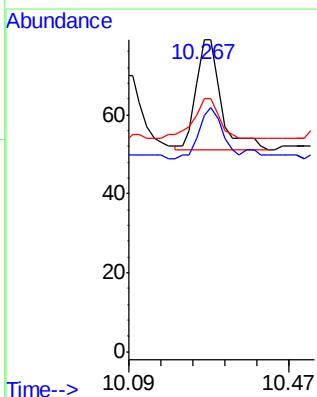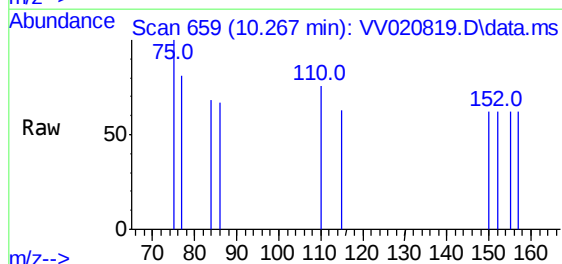

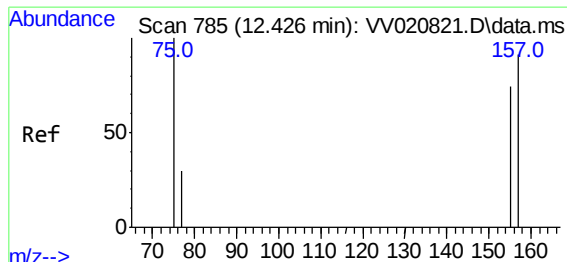

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.07 ug/L
 RT: 12.427 min Scan# 785
 Delta R.T. 0.000 min
 Lab File: VV020819.D
 Acq: 31 Mar 2021 10:36

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.05302

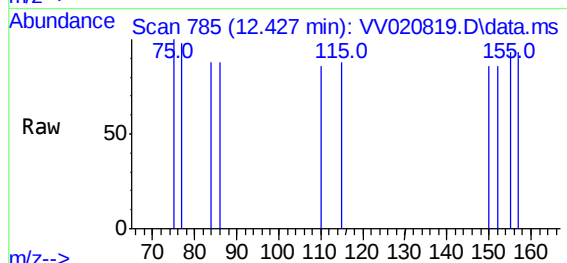

Tgt Ion: 75 Resp: 28
 Ion Ratio Lower Upper
 75 100
 157 93.0 74.8 112.2
 155 93.0 67.4 101.2

