

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW033121\
 Data File : VW020820.D
 Acq On : 31 Mar 2021 11:22
 Operator : SY/MD
 Sample : VSTD0.131
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.1303

Quant Time: Apr 01 04:04:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM033121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 01 04:03:39 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Difluorobenzene	5.639	114	4933	0.50 ug/L	0.00
5) Chlorobenzene-d5	8.864	117	4787	0.50 ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	2652	0.50 ug/L	0.00
System Monitoring Compounds					
2) Vinyl Chloride-d3	1.303	65	355	0.06 ug/L	0.00
4) 1,2-Dichloroethane-d4	5.042	65	362	0.10 ug/L	0.00
7) 1,2-Dichloropropane-d6	6.069	67	374	0.09 ug/L	0.00
8) Toluene-d8	7.332	98	1001	0.08 ug/L	0.02
10) 1,1,2,2-Tetrachloroeth...	10.216	84	261	0.10 ug/L	0.00
Target Compounds					
3) Vinyl chloride	1.303	62	284	0.06 ug/L	Qvalue # 72
6) Trichloroethene	5.925	95	326	0.09 ug/L	93
9) 1,2-Dibromoethane	8.369	107	214	0.10 ug/L	Qvalue # 89
12) 1,2,3-Trichloropropane	10.267	75	201	0.09 ug/L	98
13) 1,2-Dibromo-3-chloropr...	12.427	75	35	0.09 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033121\
Data File : VV020820.D
Acq On : 31 Mar 2021 11:22
Operator : SY/MD
Sample : VSTD0.131
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.1303

Quant Time: Apr 01 04:04:19 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM033121.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 01 04:03:39 2021
Response via : Initial Calibration




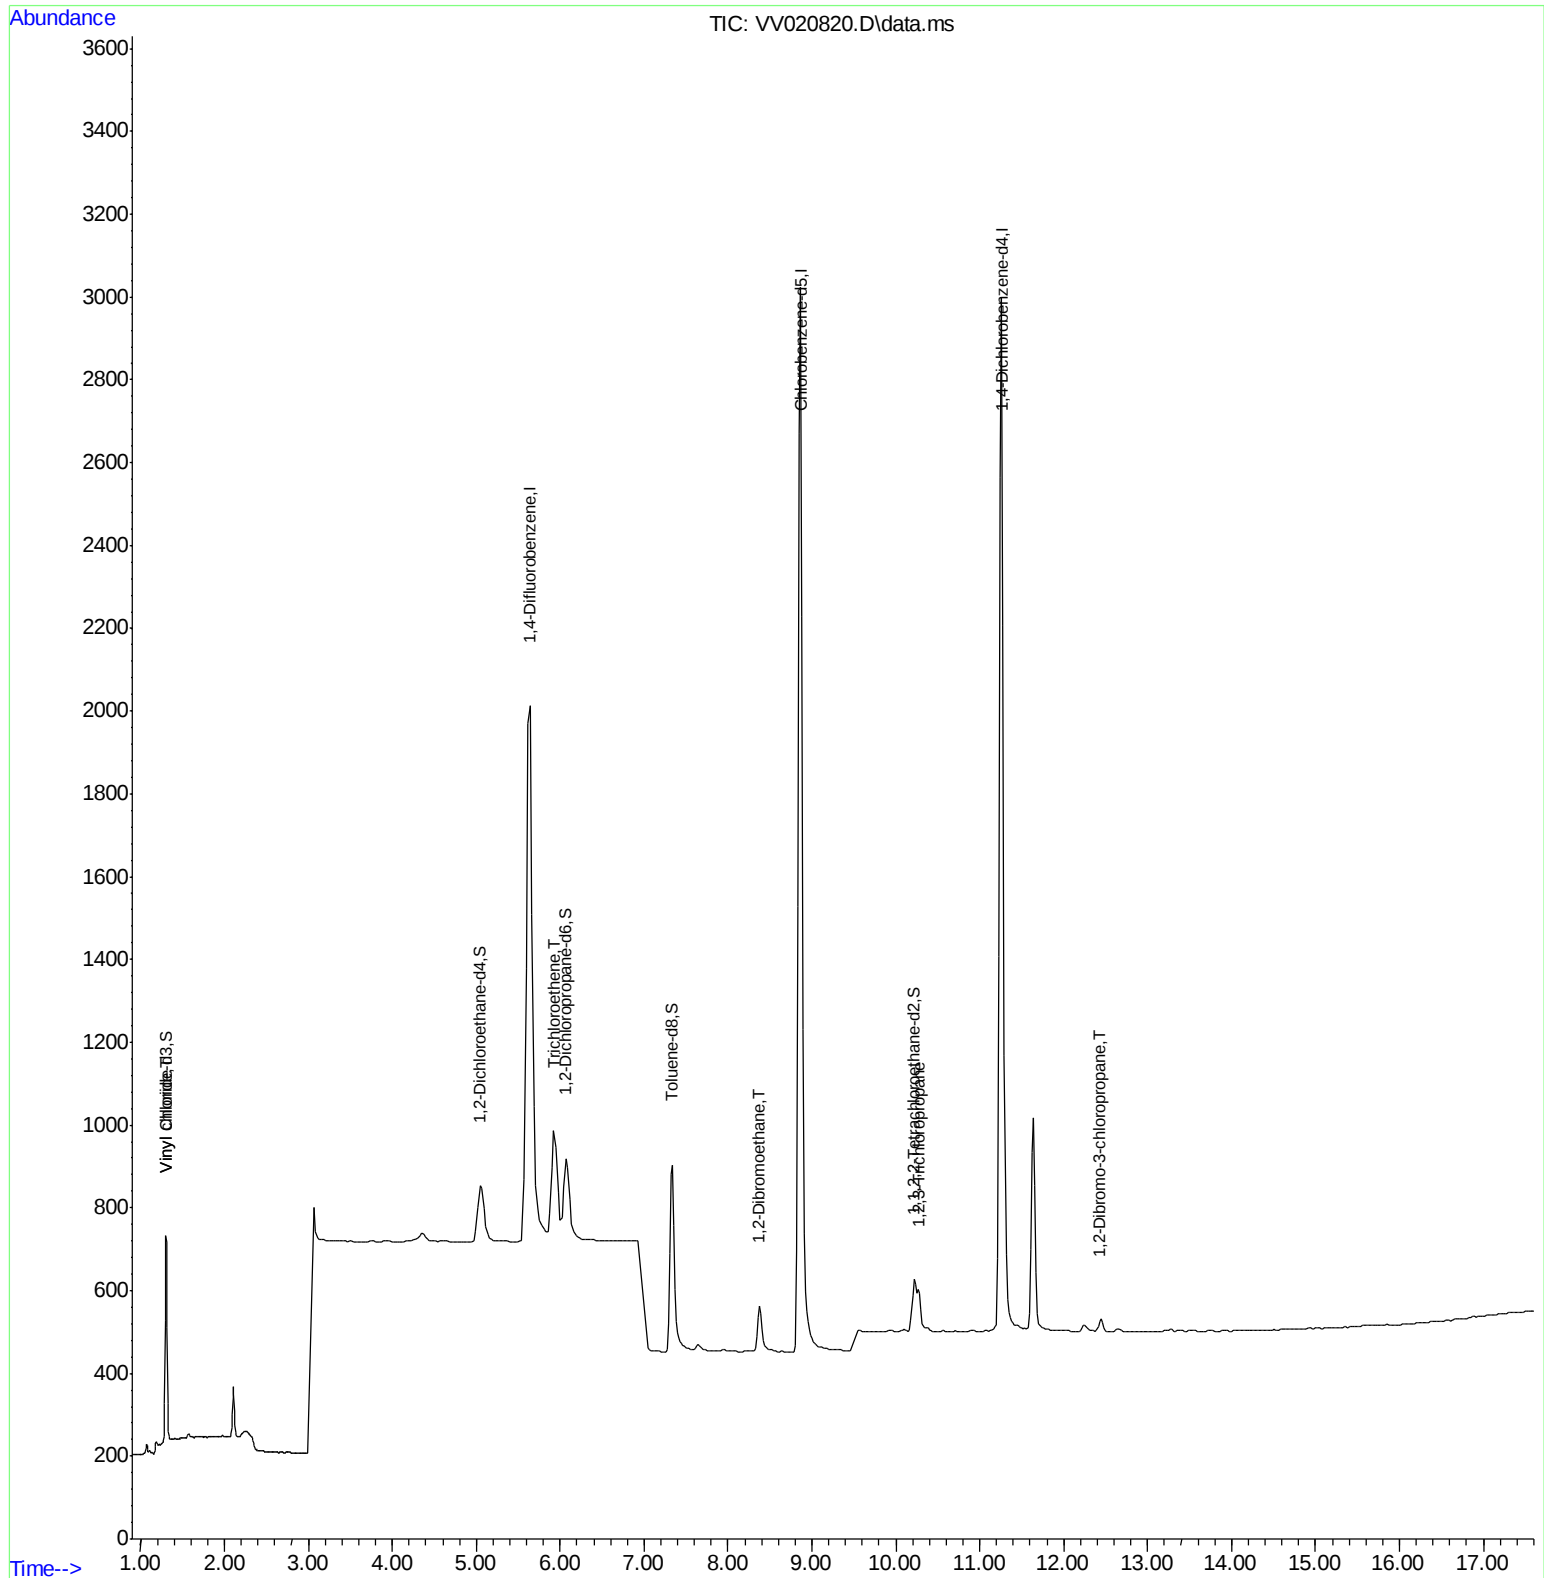


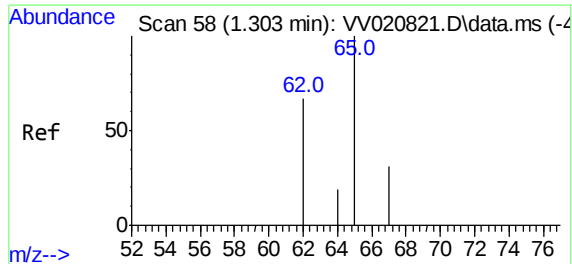

#3
 Vinyl chloride
 Concen: 0.06 ug/L
 RT: 1.303 min Scan# 58
 Delta R.T. 0.000 min
 Lab File: VV020820.D
 Acq: 31 Mar 2021 11:22




Instrument :
 MSVOA_V
 ClientSampled :
 VSTD0.1303


Tgt Ion: 62 Resp: 284
 Ion Ratio Lower Upper
 62 100
 64 53.1 25.8 47.8#

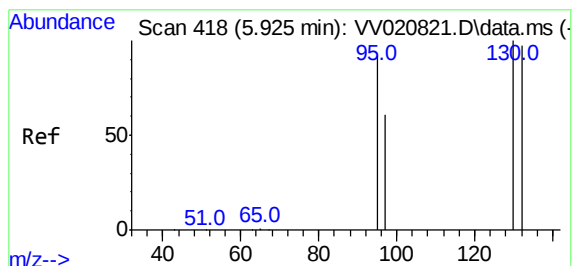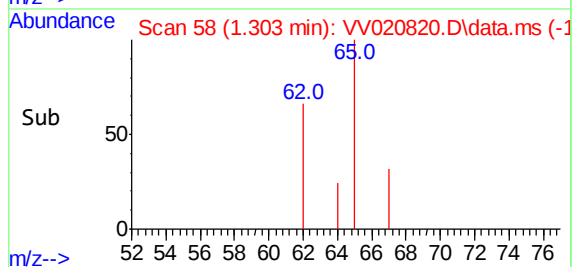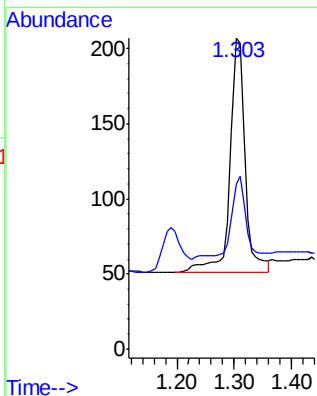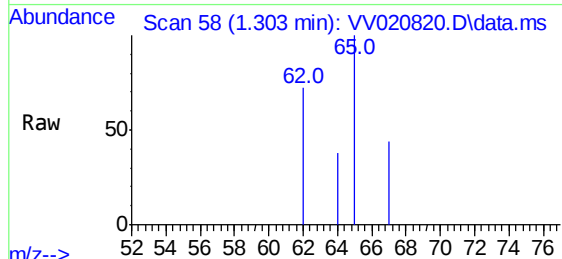

#6
 Trichloroethene
 Concen: 0.09 ug/L
 RT: 5.925 min Scan# 418
 Delta R.T. 0.000 min
 Lab File: VV020820.D
 Acq: 31 Mar 2021 11:22

Tgt Ion: 95 Resp: 326
 Ion Ratio Lower Upper
 95 100
 97 79.8 48.5 90.1
 132 99.2 73.0 135.6
 130 100.8 75.0 139.2


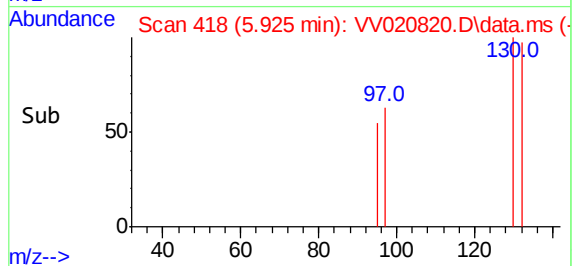
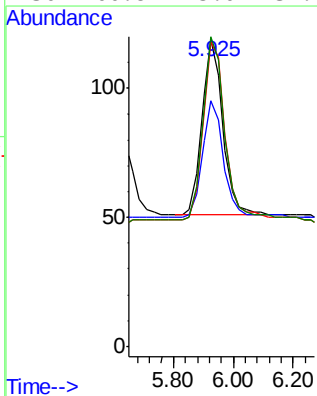
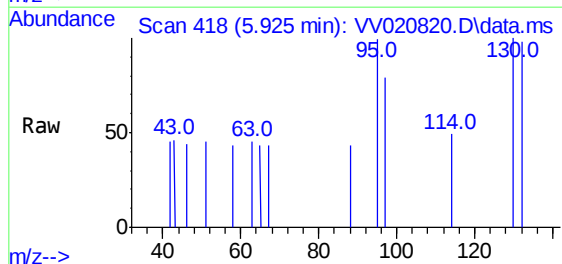


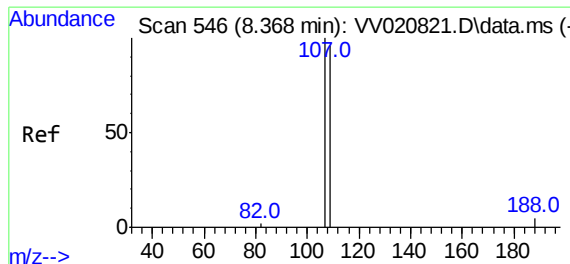

#9
1,2-Dibromoethane
Concen: 0.10 ug/L
RT: 8.369 min Scan# 546
Delta R.T. 0.000 min
Lab File: VV020820.D
Acq: 31 Mar 2021 11:22




Instrument :
MSVOA_V
ClientSampleId :
VSTD0.1303


Tgt Ion:107 Resp: 214
Ion Ratio Lower Upper
107 100
109 97.1 67.8 126.0
188 49.0 13.4 20.2#

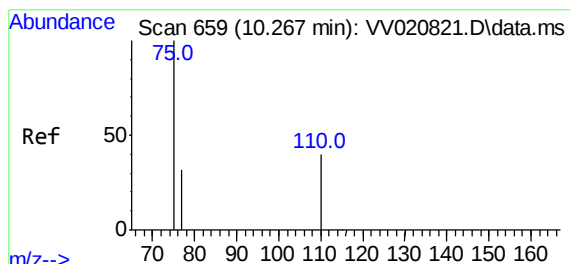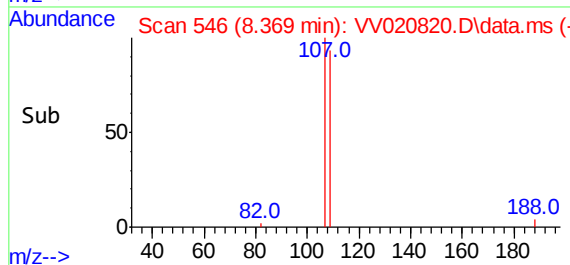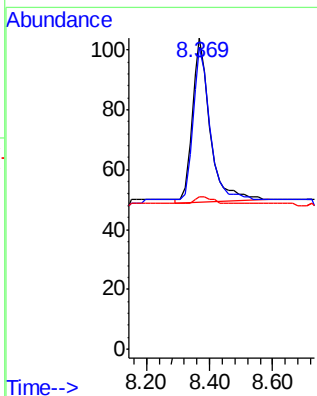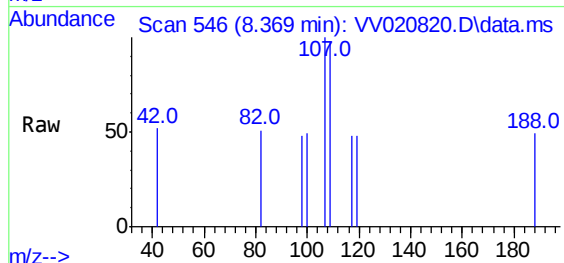

#12
1,2,3-Trichloropropane
Concen: 0.09 ug/L
RT: 10.267 min Scan# 659
Delta R.T. 0.000 min
Lab File: VV020820.D
Acq: 31 Mar 2021 11:22


Tgt Ion: 75 Resp: 201
Ion Ratio Lower Upper
75 100
110 42.8 35.5 53.3
77 34.3 27.1 40.7

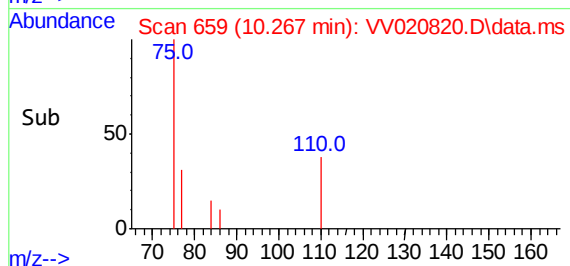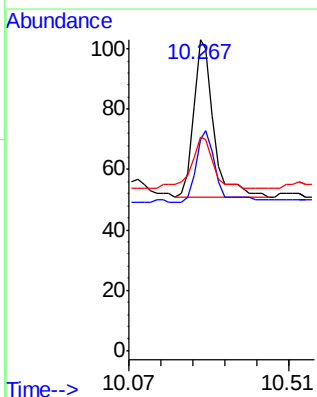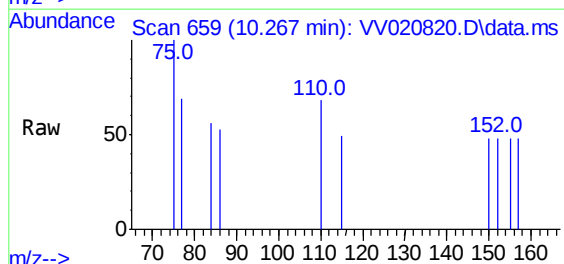

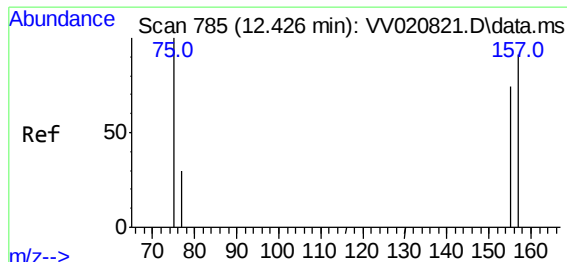

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.09 ug/L
 RT: 12.427 min Scan# 785
 Delta R.T. 0.000 min
 Lab File: VV020820.D
 Acq: 31 Mar 2021 11:22

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.1303

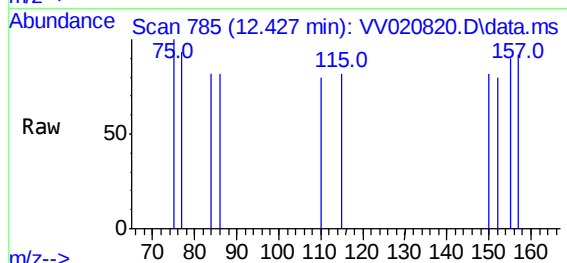

Tgt Ion: 75 Resp: 35
 Ion Ratio Lower Upper
 75 100
 157 91.8 74.8 112.2
 155 90.2 67.4 101.2

