


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033121\
 Data File : VV020818.D
 Acq On : 31 Mar 2021 09:51
 Operator : SY/MD
 Sample : BFB34
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB307

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM033121.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Apr 01 04:09:11 2021

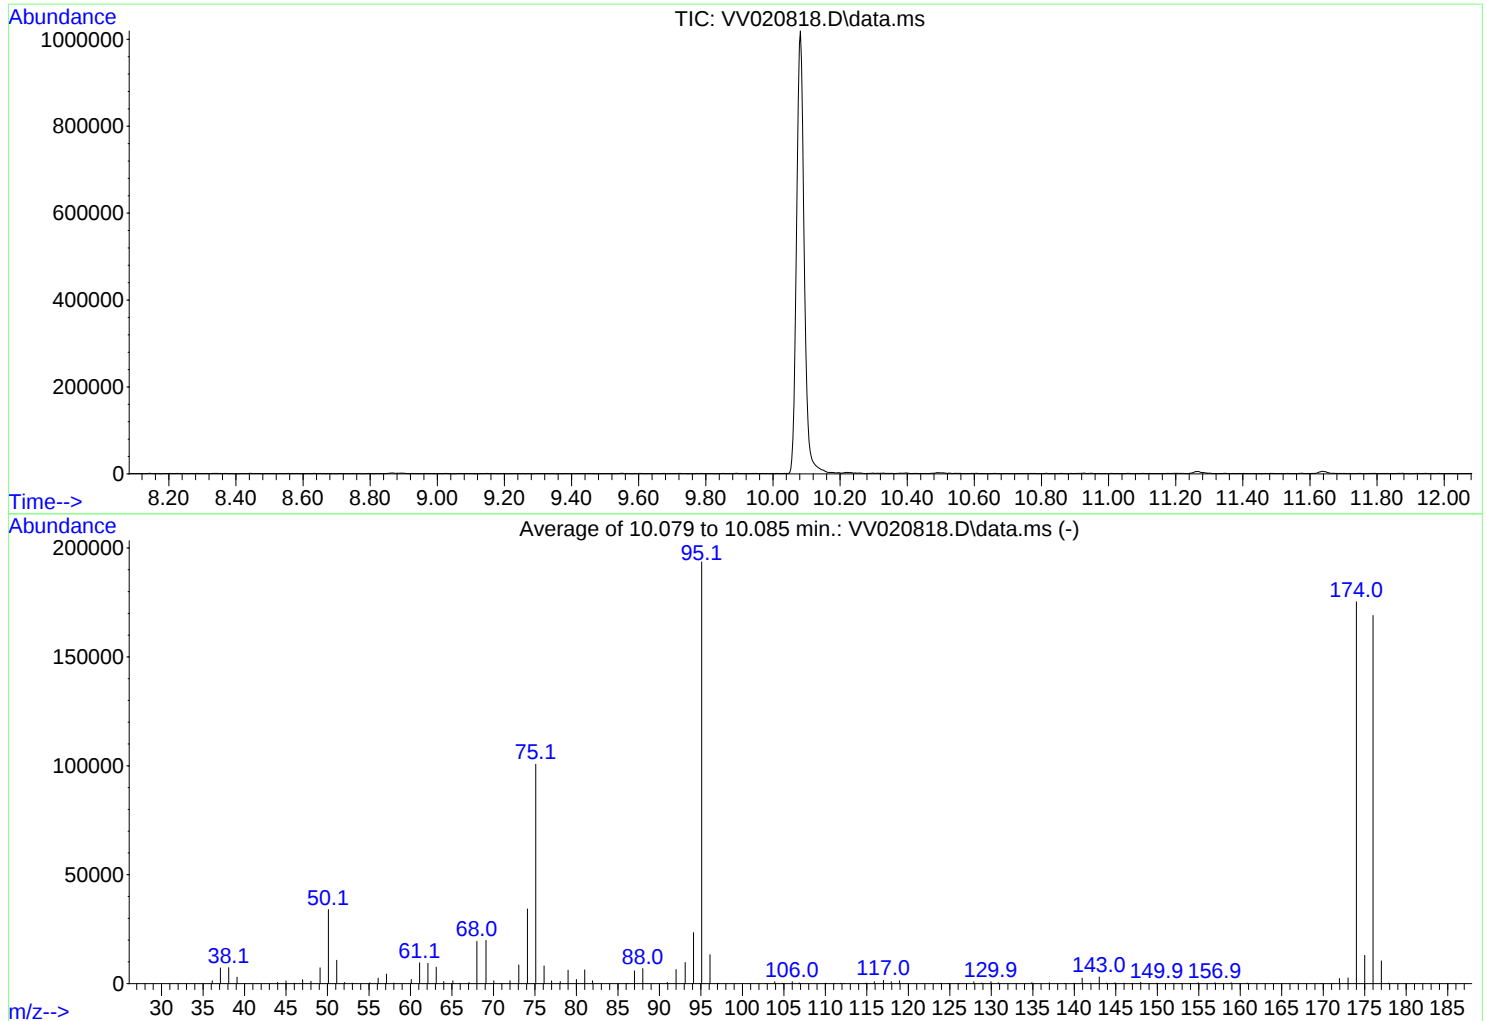

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	33992	PASS
75	95	30	80	52.0	100680	PASS
95	95	100	100	100.0	193643	PASS
96	95	5	9	6.9	13316	PASS
173	174	0.00	2	1.5	2672	PASS
174	95	50	120	90.5	175339	PASS
175	174	5	9	7.4	13035	PASS
176	174	95	101	96.4	169003	PASS
177	176	5	9	6.2	10459	PASS

m/z	Abundance
36.10	1315.0
37.10	7441.0
38.10	7775.0
39.10	3081.0
40.10	322.0
44.00	1030.0
45.00	1279.0
46.00	254.0
47.00	1955.0
48.00	1116.0
49.10	7228.0
50.10	34832.0
51.10	10886.0
52.10	474.0
53.00	238.0
55.10	477.0
56.10	2551.0
57.10	4430.0
58.00	342.0
60.10	1812.0
61.10	9591.0
62.10	9629.0
63.10	7624.0
64.00	978.0
65.10	1355.0
66.00	199.0
67.10	575.0
68.00	19464.0
69.10	20208.0
70.00	1261.0
70.90	110.0
72.00	1350.0
73.00	8999.0
74.10	34440.0
75.10	101744.0
76.10	7973.0
77.00	1374.0
78.00	994.0
79.00	6485.0
80.00	1868.0
81.00	6266.0
82.00	1421.0
83.00	174.0
86.20	227.0
87.00	6235.0
88.00	7143.0
90.90	524.0
92.00	6481.0
93.10	10259.0
94.10	23776.0
95.10	196992.0
96.10	14044.0
97.10	217.0
102.80	146.0
103.90	866.0
104.90	261.0
106.00	830.0
106.80	333.0
110.10	251.0
111.00	175.0
111.80	141.0
112.30	142.0
114.90	361.0
115.90	939.0
117.00	1397.0
118.00	863.0
118.90	1342.0
124.00	171.0
124.80	139.0
127.90	841.0
128.80	429.0
129.90	1078.0
130.80	460.0
134.90	519.0
137.00	417.0
138.80	117.0
140.00	208.0
140.90	2354.0
142.10	276.0
143.00	3337.0
143.90	360.0
144.90	412.0
146.00	240.0
146.90	109.0
148.00	573.0
149.00	199.0
149.90	266.0
152.10	114.0
153.00	176.0
154.00	147.0
155.00	415.0
156.90	496.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

158.80	353.0
160.80	306.0
169.70	111.0
171.20	439.0
171.90	2250.0
173.00	2690.0
174.00	172992.0
175.00	12627.0
176.00	165952.0
177.00	10647.0
177.90	361.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

m/z	Abundance
36.10	1350.0
37.10	7462.0
38.10	7745.0
39.10	3102.0
40.00	316.0
44.10	1109.0
45.10	1423.0
46.00	214.0
47.00	1884.0
48.00	1162.0
49.10	7518.0
50.10	35136.0
51.10	11136.0
52.00	529.0
53.00	267.0
55.10	413.0
56.10	2662.0
57.10	4548.0
58.00	341.0
60.10	1928.0
61.10	9814.0
62.10	9689.0
63.10	7937.0
64.00	945.0
65.10	1373.0
65.90	182.0
67.10	511.0
68.00	19936.0
69.10	20488.0
70.00	1370.0
72.00	1438.0
73.10	8922.0
74.10	35656.0
75.10	103848.0
76.10	8421.0
77.00	1274.0
78.10	1045.0
79.00	6414.0
80.00	1999.0
81.00	6584.0
81.90	1359.0
83.00	193.0
86.10	187.0
87.00	5934.0
88.00	7014.0
90.90	580.0
92.00	6566.0
93.10	10063.0
94.10	23936.0
95.10	200256.0
96.10	13820.0
97.00	249.0
103.90	942.0
104.90	260.0
106.00	986.0
106.90	365.0
110.00	271.0
111.00	185.0
111.80	247.0
112.30	206.0
114.90	299.0
115.90	978.0
117.00	1580.0
118.00	921.0
119.00	1380.0
123.90	251.0
124.80	163.0
126.00	105.0
127.90	911.0
128.90	425.0
129.90	977.0
130.80	597.0
134.90	514.0
137.00	442.0
138.80	157.0
140.00	224.0
141.00	2582.0
141.90	285.0
143.00	3273.0
143.90	307.0
144.90	474.0
146.00	305.0
148.00	687.0
149.00	199.0
150.00	226.0
151.90	179.0
152.80	161.0
155.00	433.0
157.00	448.0
158.90	410.0
160.80	340.0
169.70	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

171.90	2501.0
173.00	2787.0
174.00	181568.0
175.00	13577.0
176.00	175424.0
177.00	10780.0
177.90	361.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

m/z	Abundance
36.10	1270.0
37.10	6705.0
38.10	6542.0
39.10	2902.0
40.00	343.0
44.10	1226.0
45.10	1457.0
46.00	168.0
47.00	1645.0
48.00	1100.0
49.10	6999.0
50.10	32008.0
51.10	10085.0
52.00	470.0
53.00	243.0
55.10	347.0
56.10	2479.0
57.10	4281.0
58.00	301.0
60.10	1904.0
61.10	9210.0
62.10	8708.0
63.10	7159.0
64.00	860.0
65.10	1320.0
65.90	148.0
67.00	461.0
68.00	18848.0
69.10	18840.0
70.10	1314.0
72.00	1242.0
73.10	7764.0
74.10	32928.0
75.10	96448.0
76.10	8010.0
77.00	1105.0
78.10	780.0
79.00	5728.0
80.00	1906.0
81.00	6202.0
81.90	1182.0
83.00	204.0
86.10	150.0
87.00	5541.0
88.00	6509.0
91.00	664.0
92.00	6348.0
93.10	8741.0
94.10	22608.0
95.10	183680.0
96.10	12085.0
97.00	255.0
103.90	771.0
104.80	255.0
106.00	1027.0
106.90	327.0
110.00	181.0
111.10	190.0
111.90	298.0
112.30	203.0
115.00	213.0
115.90	851.0
117.00	1576.0
117.90	836.0
119.00	1288.0
123.80	275.0
124.90	155.0
127.90	884.0
129.10	463.0
130.00	776.0
130.90	532.0
134.90	510.0
137.00	456.0
138.90	176.0
140.00	157.0
141.00	2502.0
141.90	288.0
143.00	2740.0
143.90	242.0
144.90	501.0
146.00	299.0
148.00	637.0
149.00	118.0
150.00	192.0
151.90	224.0
152.80	166.0
154.90	427.0
156.10	122.0
157.00	359.0
159.00	461.0
160.90	321.0
169.80	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

170.80	215.0
172.00	2399.0
173.00	2538.0
174.00	171456.0
175.00	12901.0
176.00	165632.0
177.00	9949.0
177.90	228.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

m/z	Abundance
40.00	235.0
44.00	535.0
44.90	102.0
131.00	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307