

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033123\
 Data File : VV030375.D
 Acq On : 31 Mar 2023 11:25
 Operator : SY/MD
 Sample : 02130-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Apr 03 01:29:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 31 05:37:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	133095	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	128810	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	62221	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	33611	3.813	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.200%
7) Chloroethane-d5	1.539	69	38378	4.486	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.800%
11) 1,1-Dichloroethene-d2	2.063	63	62001	2.964	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.200%#
20) 2-Butanone-d5	3.822	46	111893	49.110	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.220%
24) Chloroform-d	4.259	84	102004	4.781	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
26) 1,2-Dichloroethane-d4	4.953	65	51458	5.112	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.200%
32) Benzene-d6	4.970	84	176075	4.851	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.000%
36) 1,2-Dichloropropane-d6	5.998	67	58275	5.128	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.600%
41) Toluene-d8	7.252	98	146715	4.401	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.000%
43) trans-1,3-Dichloroprop...	7.564	79	19274	4.505	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.000%
46) 2-Hexanone-d5	8.037	63	83693	48.679	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.360%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	41442	4.627	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.600%
66) 1,2-Dichlorobenzene-d4	11.567	152	58385	5.250	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.000%
Target Compounds						
16) Methylene chloride	2.458	84	5442	0.414	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033123\
Data File : VV030375.D
Acq On : 31 Mar 2023 11:25
Operator : SY/MD
Sample : 02130-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Apr 03 01:29:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 31 05:37:21 2023
Response via : Initial Calibration

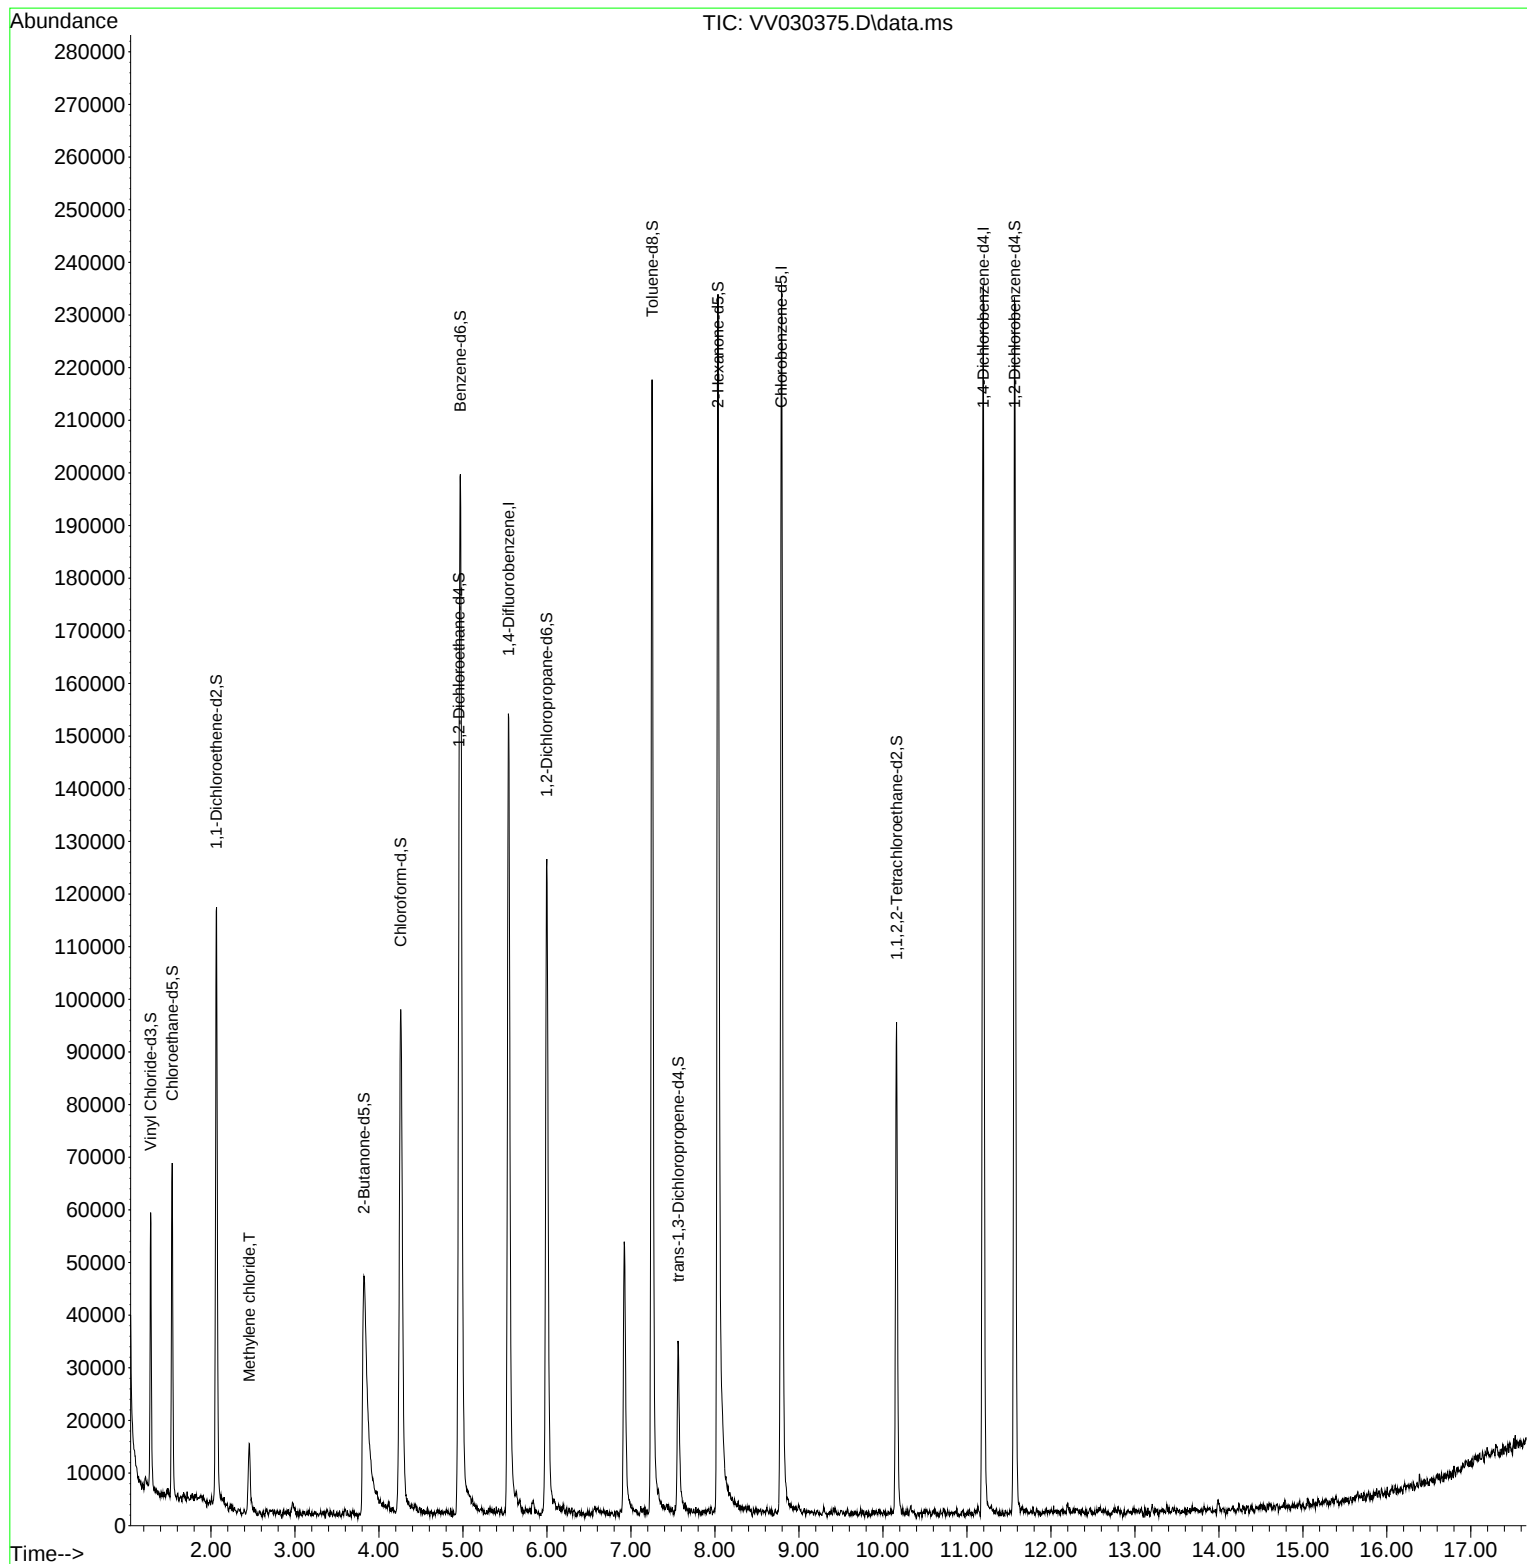

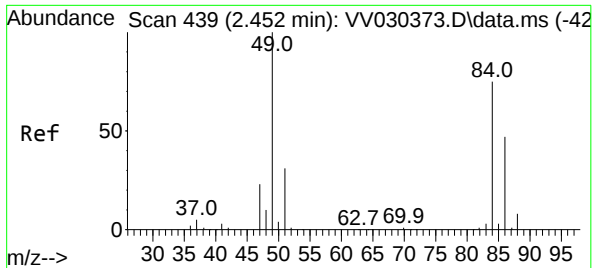

#16
Methylene chloride
Concen: 0.414 ug/L
RT: 2.458 min Scan# 441
Delta R.T. 0.006 min
Lab File: VV030375.D
Acq: 31 Mar 2023 11:25

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion:	84	Resp:	5442
Ion	Ratio	Lower	Upper
84	100		
86	66.0	44.0	81.6
49	124.9	90.6	168.3

