

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW033123\
 Data File : VW030379.D
 Acq On : 31 Mar 2023 13:07
 Operator : SY/MD
 Sample : VIBLK283
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK283

Quant Time: Apr 03 01:29:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 31 05:37:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	123061	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	125655	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	61517	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	32176	3.948	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.000%
7) Chloroethane-d5	1.539	69	34569	4.371	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.400%
11) 1,1-Dichloroethene-d2	2.066	63	49386	2.554	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	51.000%#
20) 2-Butanone-d5	3.815	46	110241	52.330	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.660%
24) Chloroform-d	4.262	84	89379	4.531	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.600%
26) 1,2-Dichloroethane-d4	4.953	65	46047	4.948	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.000%
32) Benzene-d6	4.973	84	141247	3.989	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.800%
36) 1,2-Dichloropropane-d6	5.998	67	48624	4.386	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.800%
41) Toluene-d8	7.252	98	114278	3.514	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	70.200%
43) trans-1,3-Dichloroprop...	7.564	79	15959	3.824	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.400%
46) 2-Hexanone-d5	8.034	63	79409	47.347	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.700%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	39445	4.515	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.200%
66) 1,2-Dichlorobenzene-d4	11.570	152	54559	4.962	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.200%
Target Compounds						Qvalue
3) Chloromethane	1.220	50	2696	0.137	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033123\
Data File : VV030379.D
Acq On : 31 Mar 2023 13:07
Operator : SY/MD
Sample : VIBLK283
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK283

Quant Time: Apr 03 01:29:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 31 05:37:21 2023
Response via : Initial Calibration

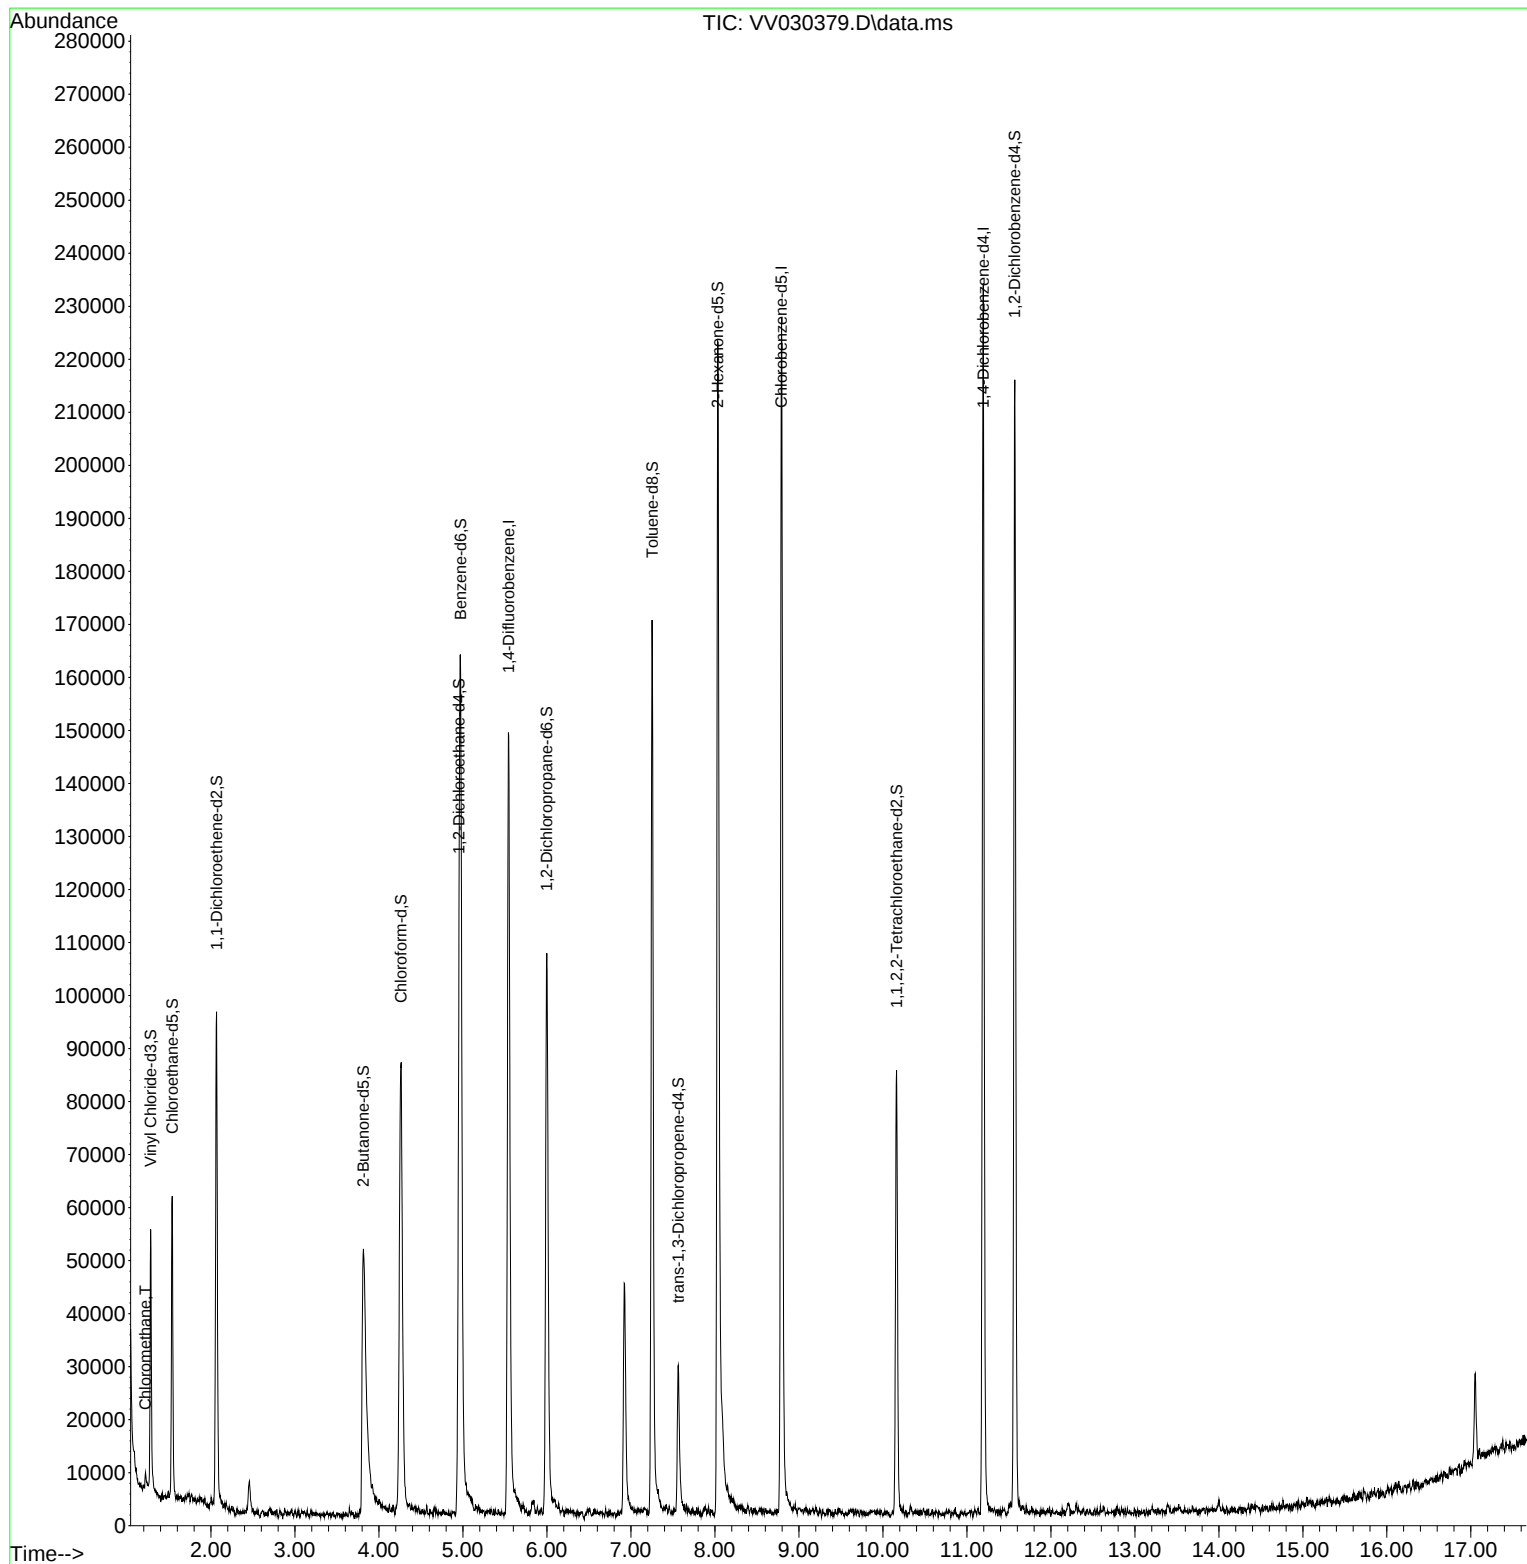

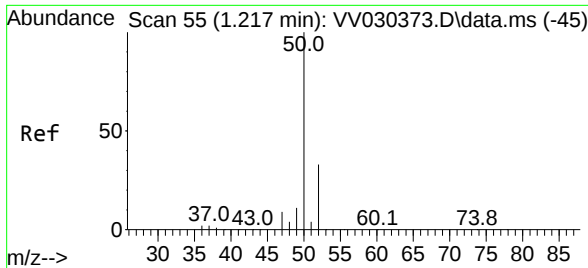

#3
 Chloromethane
 Concen: 0.137 ug/L
 RT: 1.220 min Scan# 50
 Delta R.T. 0.003 min
 Lab File: VV030379.D
 Acq: 31 Mar 2023 13:07

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK283

Tgt Ion: 50 Resp: 2696
 Ion Ratio Lower Upper
 50 100
 52 36.8 22.3 41.5

