

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW033123\
 Data File : VW030380.D
 Acq On : 31 Mar 2023 13:29
 Operator : SY/MD
 Sample : 02151-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C11C0

Quant Time: Apr 03 01:29:43 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 31 05:37:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	126500	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	120847	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	61845	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	47685	5.692	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	113.800%
7) Chloroethane-d5	1.539	69	43890	5.398	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.000%
11) 1,1-Dichloroethene-d2	2.066	63	80026	4.025	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.600%
20) 2-Butanone-d5	3.822	46	107553	49.667	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.340%
24) Chloroform-d	4.262	84	106701	5.262	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.200%
26) 1,2-Dichloroethane-d4	4.953	65	52858	5.525	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.400%
32) Benzene-d6	4.973	84	193110	5.671	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	113.400%
36) 1,2-Dichloropropane-d6	5.998	67	58532	5.490	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.800%
41) Toluene-d8	7.252	98	165406	5.289	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.800%
43) trans-1,3-Dichloroprop...	7.564	79	20637	5.141	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	102.800%
46) 2-Hexanone-d5	8.034	63	81079	50.266	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.540%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	41004	4.880	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.600%
66) 1,2-Dichlorobenzene-d4	11.570	152	64779	5.860	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.200%
Target Compounds						Qvalue
3) Chloromethane	1.217	50	3968	0.196	ug/L	92
13) Acetone	2.150	43	9066	4.378	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033123\
Data File : VV030380.D
Acq On : 31 Mar 2023 13:29
Operator : SY/MD
Sample : 02151-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C11C0

Quant Time: Apr 03 01:29:43 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 31 05:37:21 2023
Response via : Initial Calibration




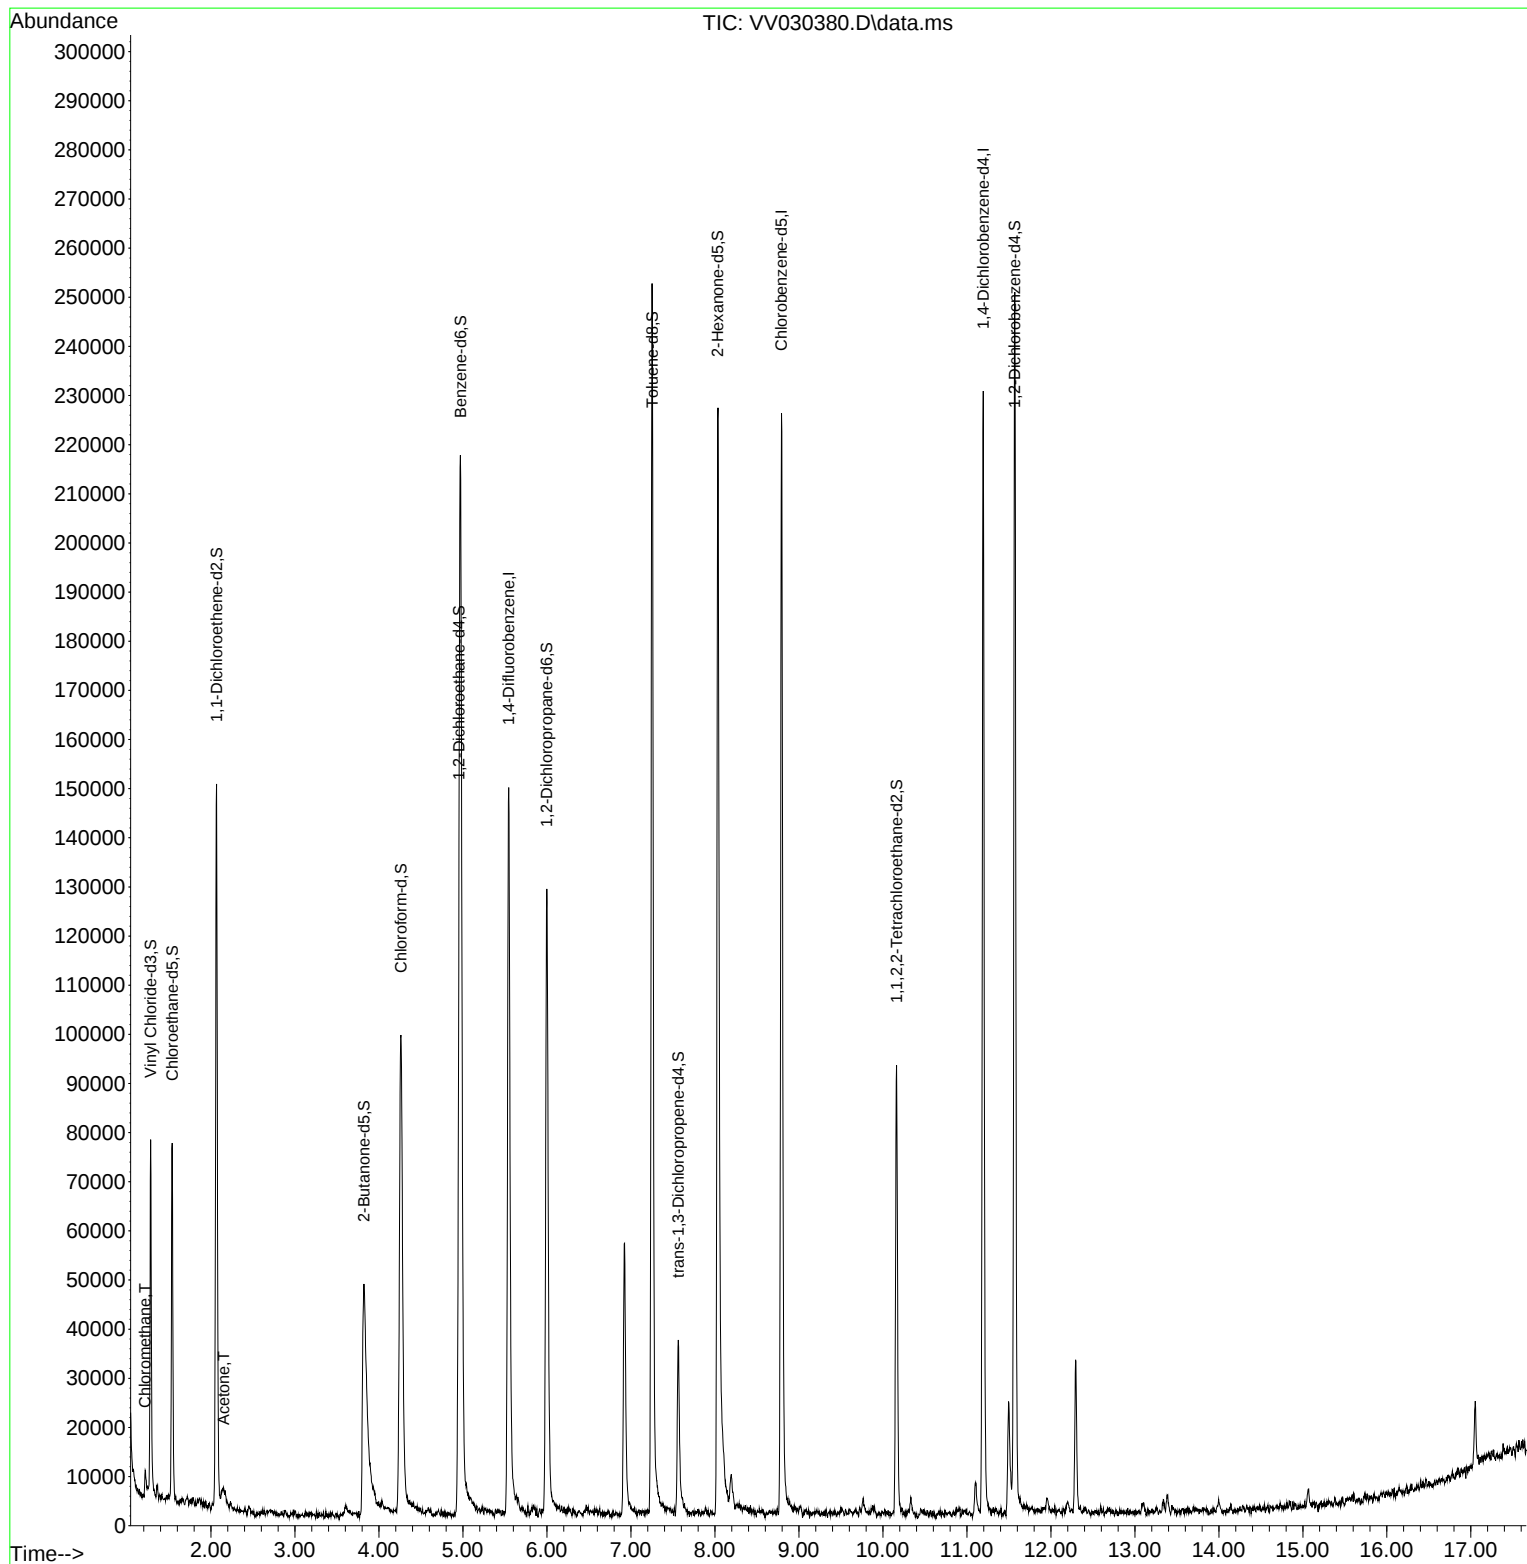


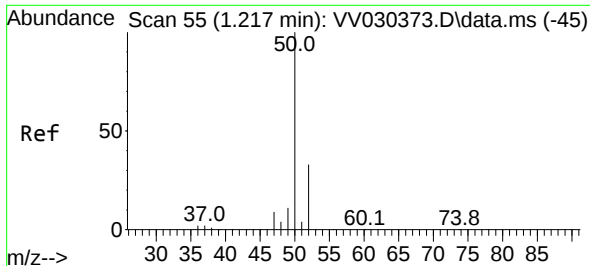

#3
Chloromethane
Concen: 0.196 ug/L
RT: 1.217 min Scan# 51
Delta R.T. -0.000 min
Lab File: VV030380.D
Acq: 31 Mar 2023 13:29

Instrument :
MSVOA_V
ClientSampleId :
C11C0

Tgt Ion: 50 Resp: 3968
Ion Ratio Lower Upper
50 100
52 36.4 22.3 41.5

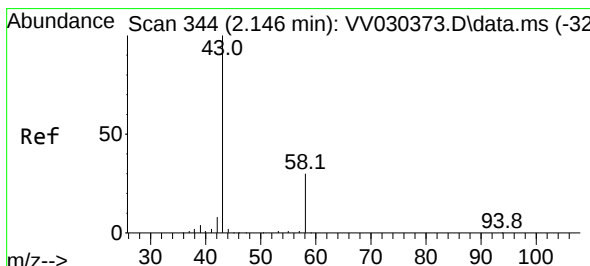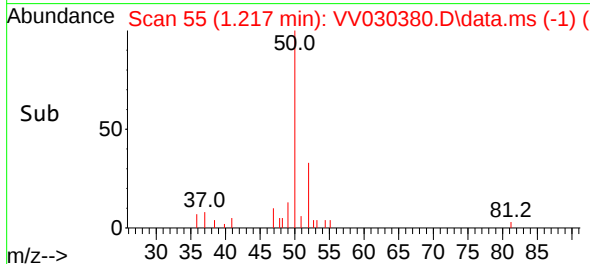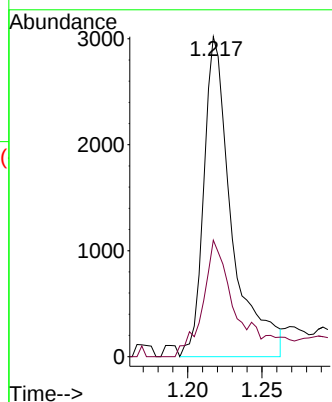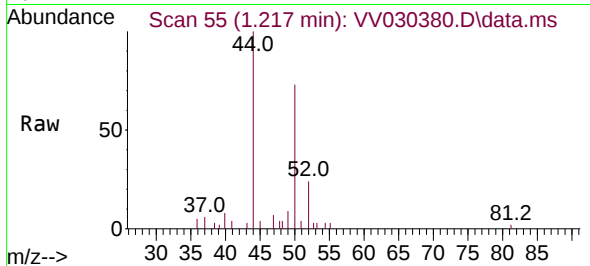

#13
Acetone
Concen: 4.378 ug/L
RT: 2.150 min Scan# 345
Delta R.T. 0.003 min
Lab File: VV030380.D
Acq: 31 Mar 2023 13:29

Tgt Ion: 43 Resp: 9066
Ion Ratio Lower Upper
43 100
58 25.9 0.0 40.8

