

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW033123\
 Data File : VW030386.D
 Acq On : 31 Mar 2023 15:49
 Operator : SY/MD
 Sample : 02130-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Apr 03 01:30:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 31 05:37:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	126878	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.796	117	125334	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	61602	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	42221	5.024	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	100.400%	
7) Chloroethane-d5	1.539	69	40157	4.924	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	98.400%	
11) 1,1-Dichloroethene-d2	2.066	63	72470	3.634	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.600%	
20) 2-Butanone-d5	3.828	46	95767	44.092	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	88.180%	
24) Chloroform-d	4.262	84	96429	4.741	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.800%	
26) 1,2-Dichloroethane-d4	4.956	65	49457	5.154	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.000%	
32) Benzene-d6	4.973	84	176724	5.004	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.000%	
36) 1,2-Dichloropropane-d6	5.998	67	53629	4.850	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.000%	
41) Toluene-d8	7.252	98	151192	4.662	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	93.200%	
43) trans-1,3-Dichloroprop...	7.564	79	17240	4.141	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.800%	
46) 2-Hexanone-d5	8.037	63	71539	42.764	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	85.520%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	38503	4.418	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	88.400%	
66) 1,2-Dichlorobenzene-d4	11.570	152	55720	5.061	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	101.200%	
Target Compounds						Qvalue
16) Methylene chloride	2.455	84	3455	0.276	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033123\
Data File : VV030386.D
Acq On : 31 Mar 2023 15:49
Operator : SY/MD
Sample : 02130-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Apr 03 01:30:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 31 05:37:21 2023
Response via : Initial Calibration

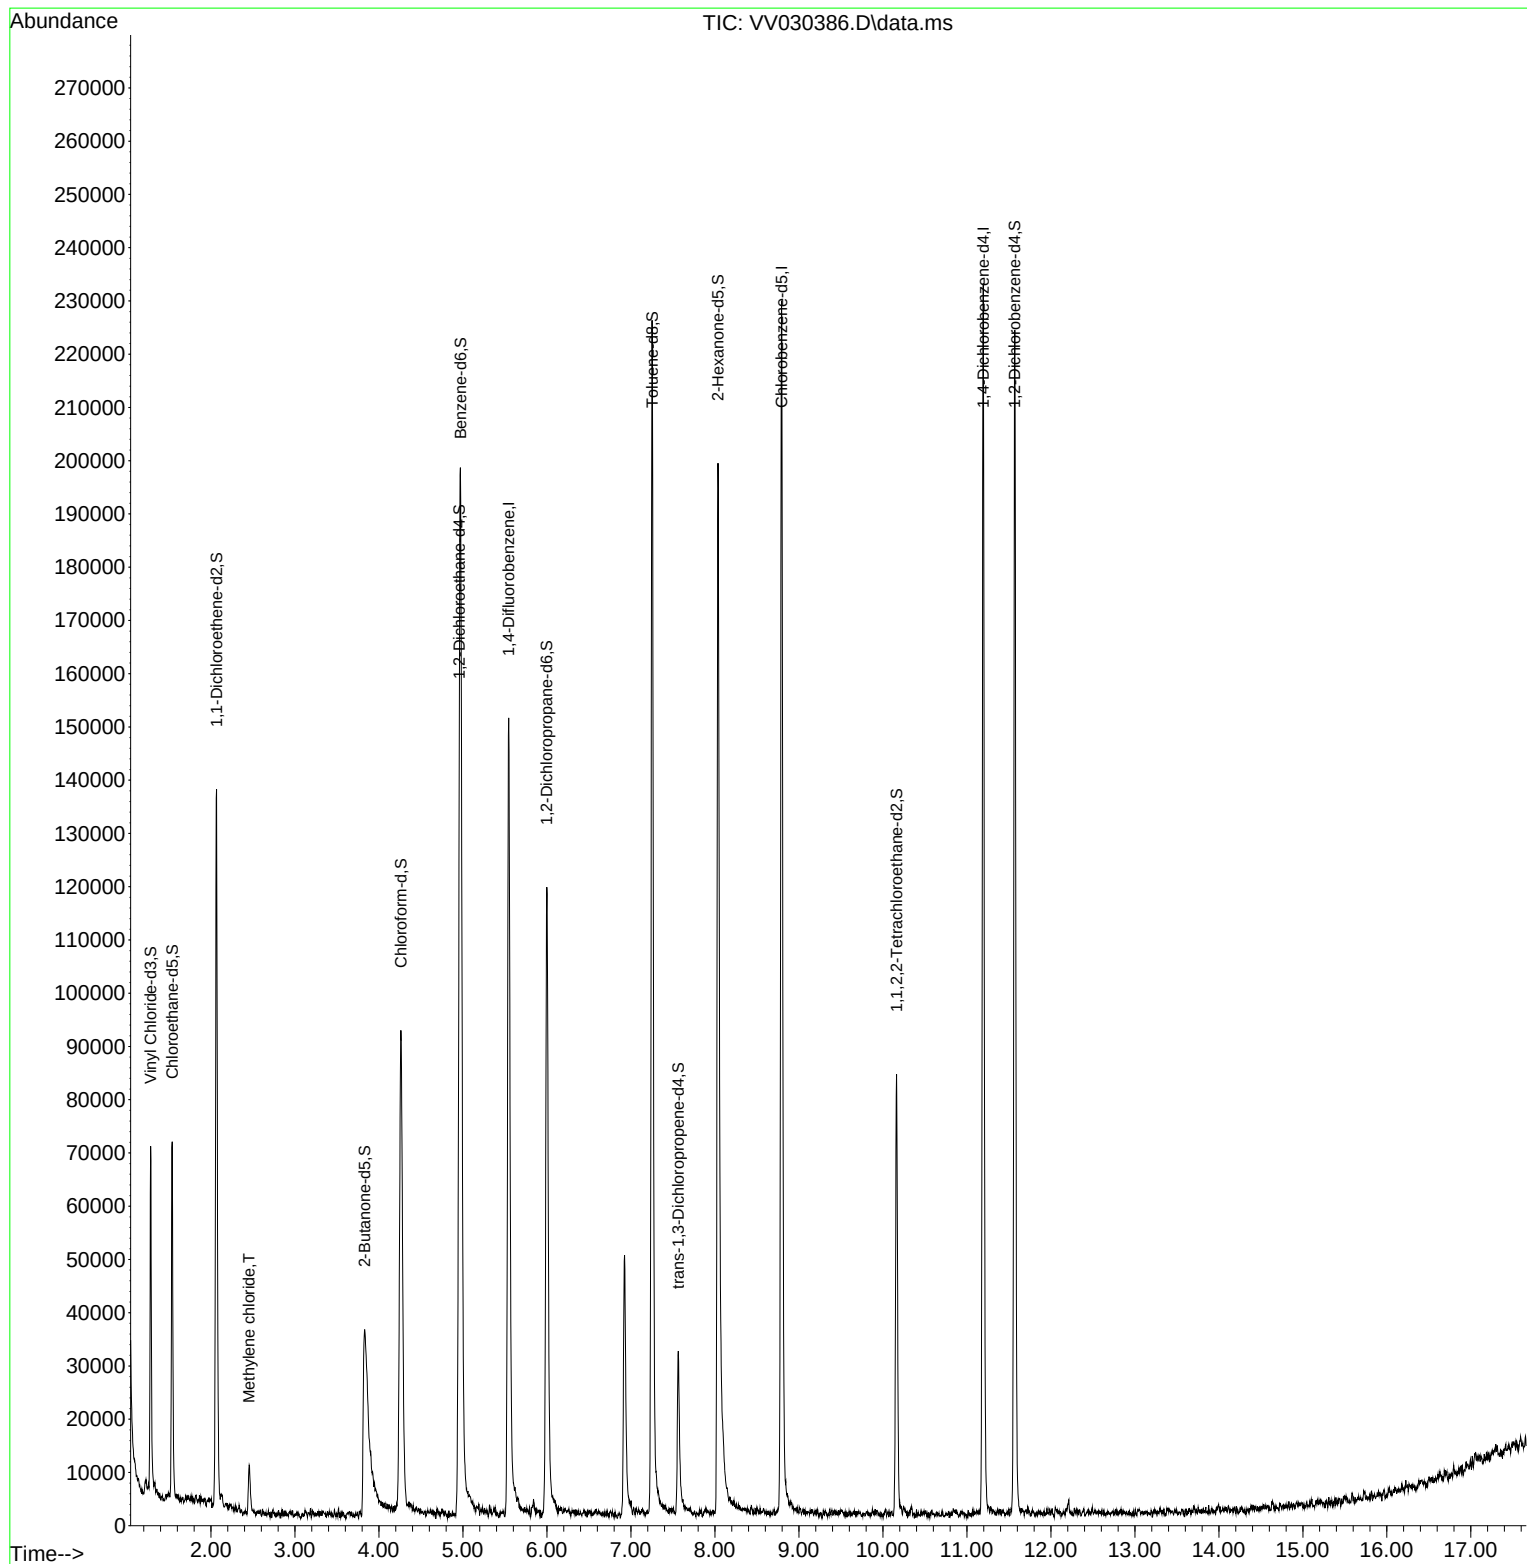

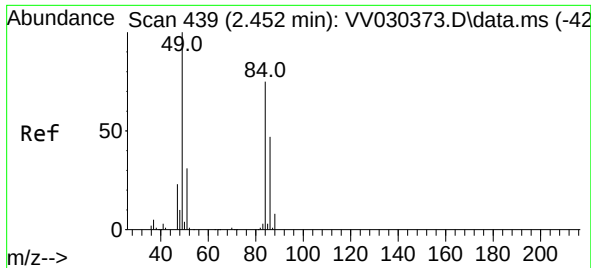

#16
Methylene chloride
Concen: 0.276 ug/L
RT: 2.455 min Scan# 44
Delta R.T. 0.003 min
Lab File: VV030386.D
Acq: 31 Mar 2023 15:49

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

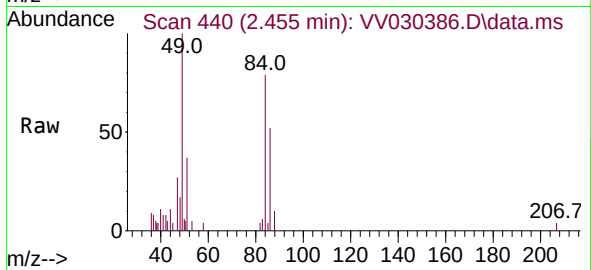

Tgt Ion:	84	Resp:	3455
Ion	Ratio	Lower	Upper
84	100		
86	66.3	44.0	81.6
49	126.5	90.6	168.3

