

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW033123\
 Data File : VW030387.D
 Acq On : 31 Mar 2023 16:11
 Operator : SY/MD
 Sample : 02150-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C11C3

Quant Time: Apr 03 01:30:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 31 05:37:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	130846	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	131535	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	64914	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	43502	5.020	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	100.400%	
7) Chloroethane-d5	1.539	69	42459	5.049	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	101.000%	
11) 1,1-Dichloroethene-d2	2.066	63	73457	3.572	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	71.400%	
20) 2-Butanone-d5	3.815	46	99768	44.541	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	89.080%	
24) Chloroform-d	4.265	84	97969	4.671	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.400%	
26) 1,2-Dichloroethane-d4	4.957	65	50045	5.057	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.200%	
32) Benzene-d6	4.973	84	180212	4.862	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.200%	
36) 1,2-Dichloropropane-d6	5.998	67	55414	4.775	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	95.600%	
41) Toluene-d8	7.252	98	154716	4.545	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.000%	
43) trans-1,3-Dichloroprop...	7.564	79	18120	4.147	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	83.000%	
46) 2-Hexanone-d5	8.034	63	74271	42.304	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	84.600%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	39645	4.335	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	86.600%	
66) 1,2-Dichlorobenzene-d4	11.571	152	61182	5.273	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	105.400%	
Target Compounds						Qvalue
3) Chloromethane	1.217	50	4492	0.214	ug/L	92
13) Acetone	2.147	43	7471	3.488	ug/L	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033123\
Data File : VV030387.D
Acq On : 31 Mar 2023 16:11
Operator : SY/MD
Sample : 02150-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C11C3

Quant Time: Apr 03 01:30:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 31 05:37:21 2023
Response via : Initial Calibration




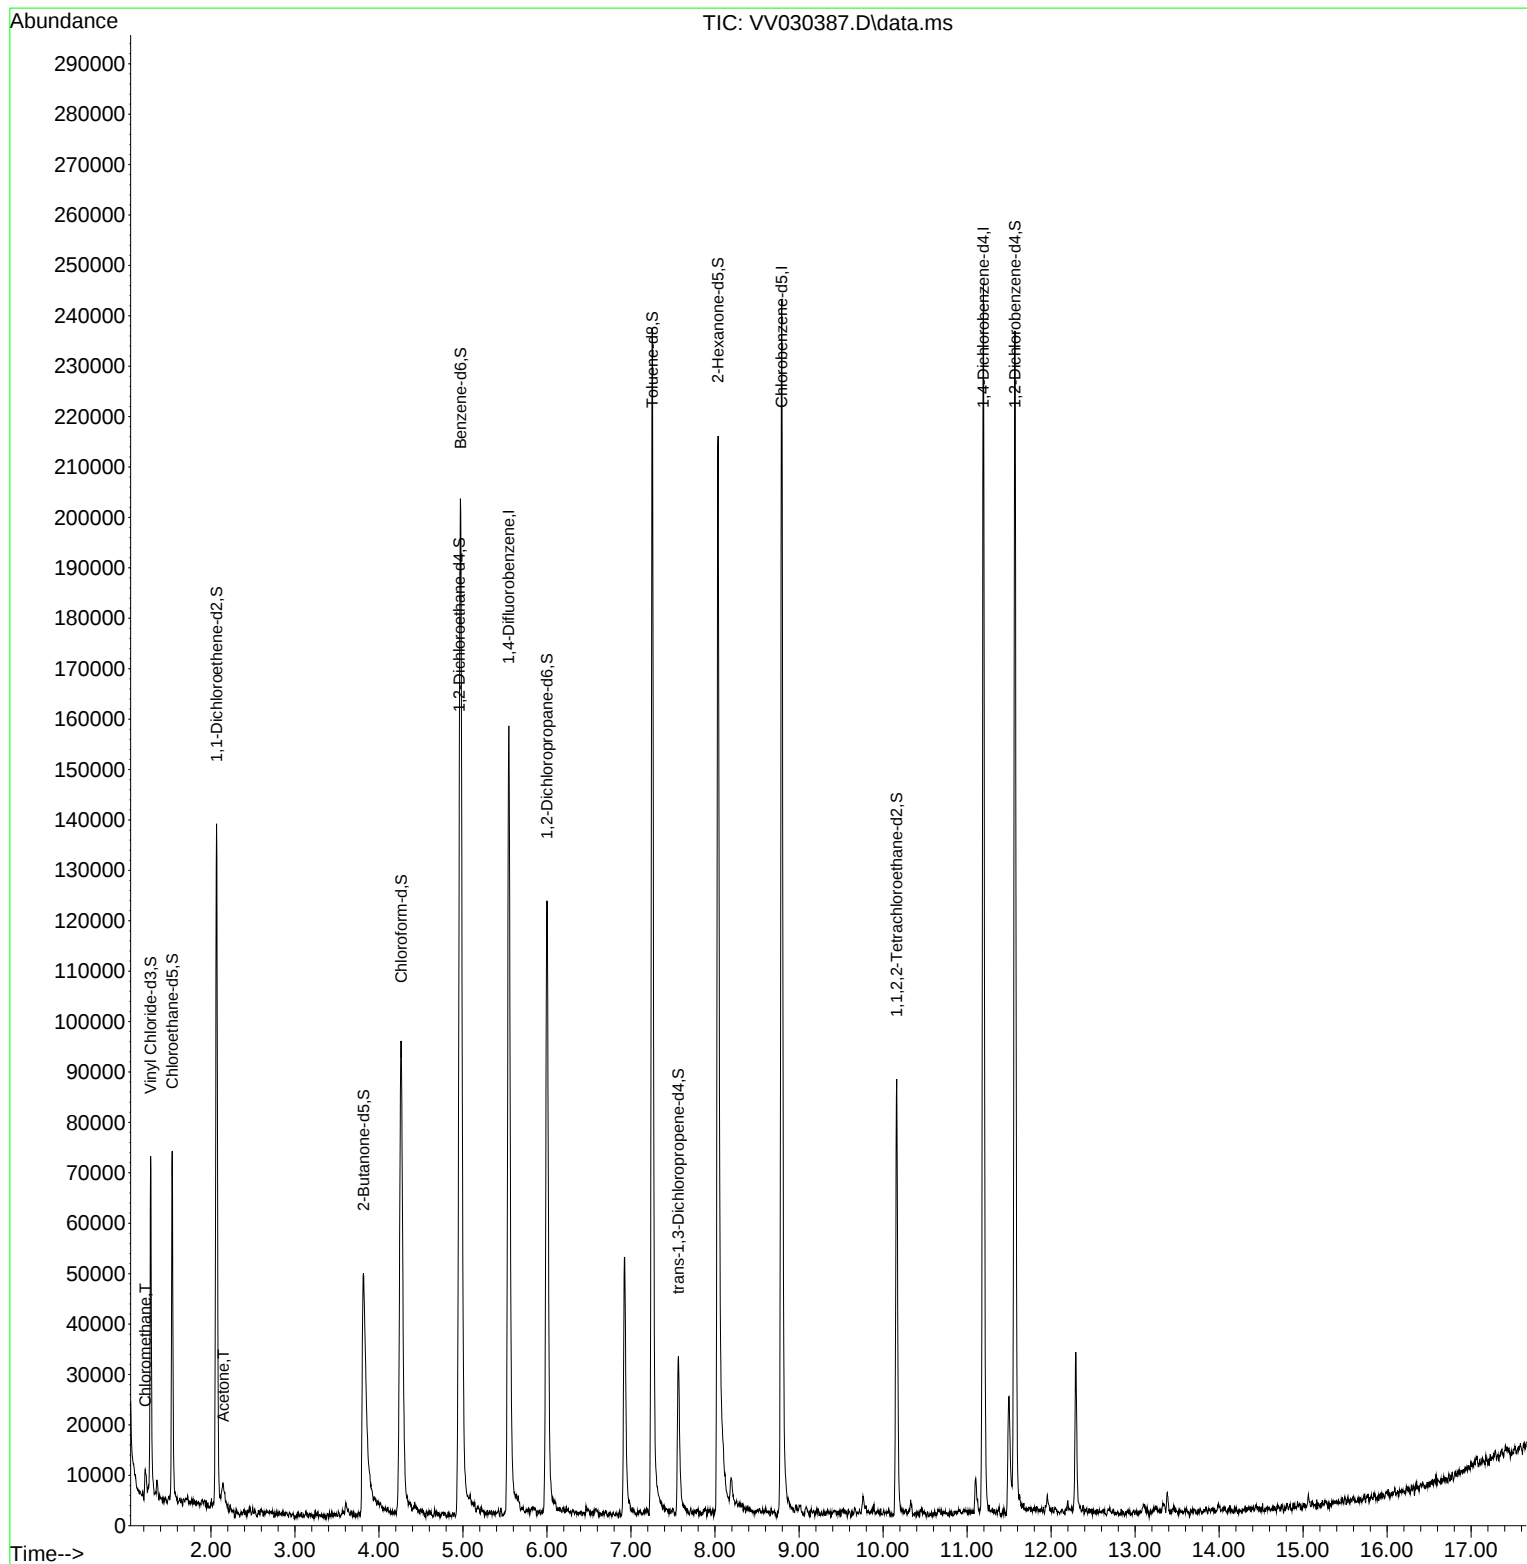


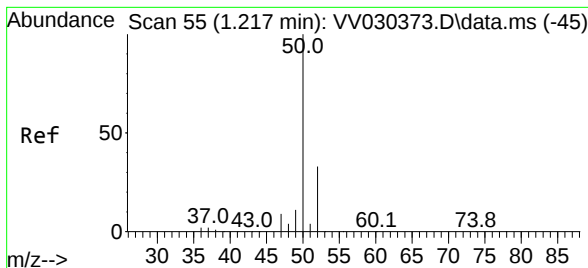

#3
Chloromethane
Concen: 0.214 ug/L
RT: 1.217 min Scan# 51
Delta R.T. 0.000 min
Lab File: VV030387.D
Acq: 31 Mar 2023 16:11

Instrument :
MSVOA_V
ClientSampleId :
C11C3

Tgt Ion: 50 Resp: 4492
Ion Ratio Lower Upper
50 100
52 27.6 22.3 41.5

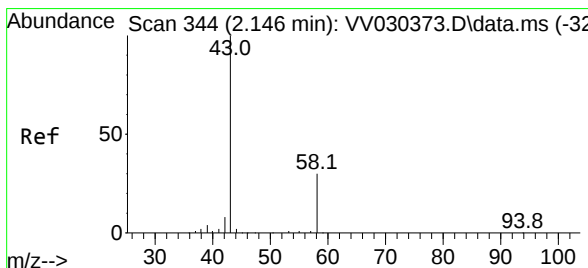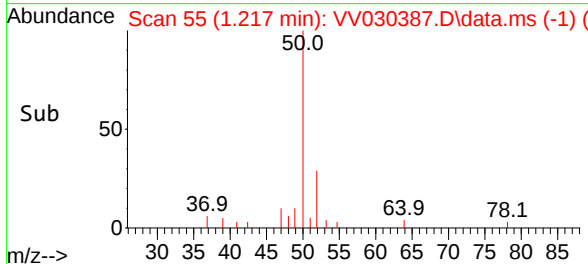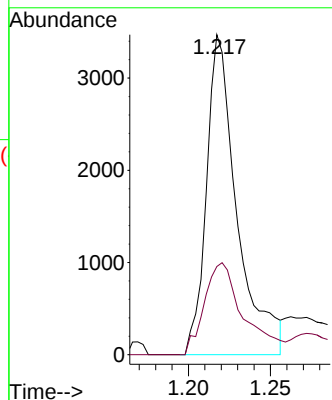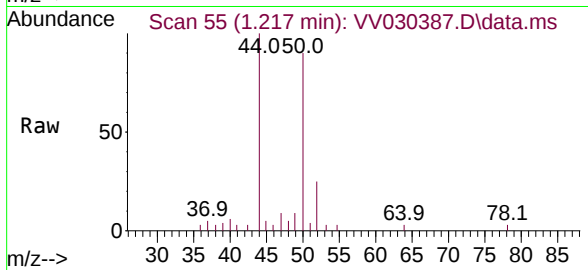

#13
Acetone
Concen: 3.488 ug/L
RT: 2.147 min Scan# 344
Delta R.T. 0.000 min
Lab File: VV030387.D
Acq: 31 Mar 2023 16:11

Tgt Ion: 43 Resp: 7471
Ion Ratio Lower Upper
43 100
58 32.0 0.0 40.8

