

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033123\
 Data File : VV030382.D
 Acq On : 31 Mar 2023 14:15
 Operator : SY/MD
 Sample : 02092-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030382.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	86	rVV	72064	77195	13.66%	1.793%
2	1.539	148	155	166	rBV	69768	83703	14.81%	1.945%
3	2.066	307	319	334	rBV	146870	216656	38.33%	5.033%
4	2.455	430	440	452	rBV2	7534	13552	2.40%	0.315%
5	3.822	854	865	888	rBV	42330	156709	27.73%	3.641%
6	4.259	983	1001	1028	rBV	100002	260117	46.02%	6.043%
7	4.969	1203	1222	1247	rBV2	214193	565211	100.00%	13.131%
8	5.545	1387	1401	1421	rBV2	141862	302785	53.57%	7.034%
9	5.998	1529	1542	1560	rBV2	129383	273365	48.37%	6.351%
10	6.921	1819	1829	1843	rBV	54667	102422	18.12%	2.379%
11	7.252	1920	1932	1953	rBV	248620	451441	79.87%	10.488%
12	7.561	2018	2028	2046	rBV2	34063	66166	11.71%	1.537%
13	8.037	2165	2176	2204	rBV	220382	447028	79.09%	10.385%
14	8.792	2399	2411	2434	rBV	222469	383540	67.86%	8.910%
15	10.162	2827	2837	2856	rVB	89318	145637	25.77%	3.383%
16	11.194	3146	3158	3174	rBV	223687	355735	62.94%	8.265%
17	11.570	3260	3275	3292	rBV	242542	392365	69.42%	9.116%
18	17.056	4971	4981	4987	rBV10	5940	10735	1.90%	0.249%




Sum of corrected areas: 4304362

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033123\
Data File : VV030382.D
Acq On : 31 Mar 2023 14:15
Operator : SY/MD
Sample : 02092-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

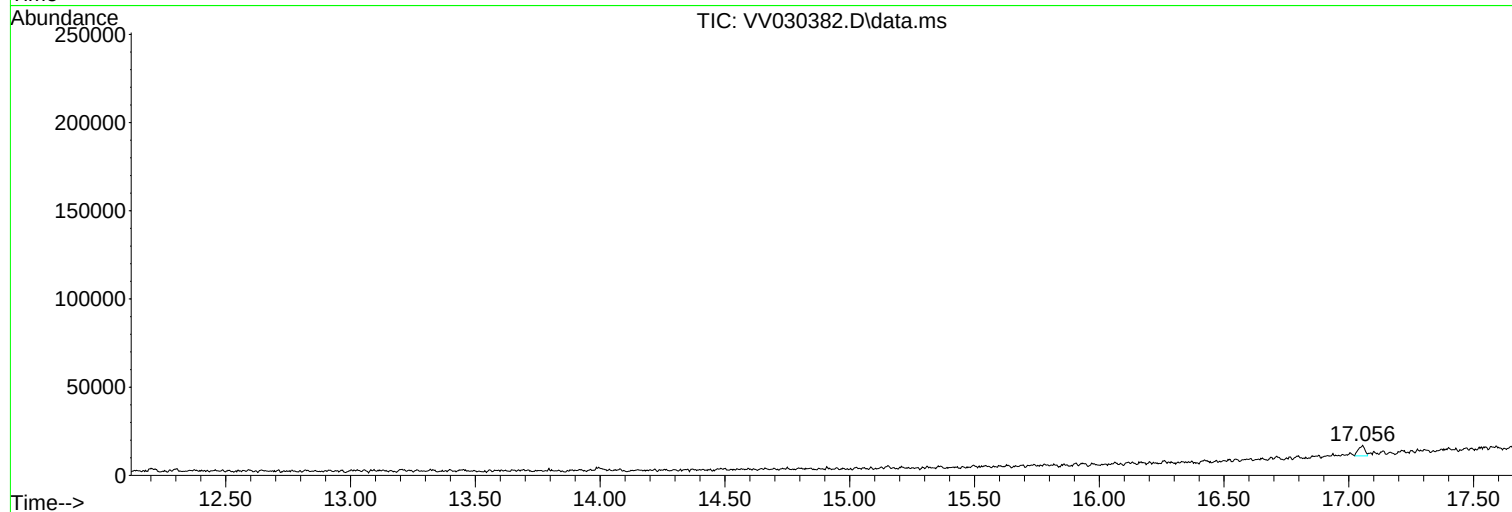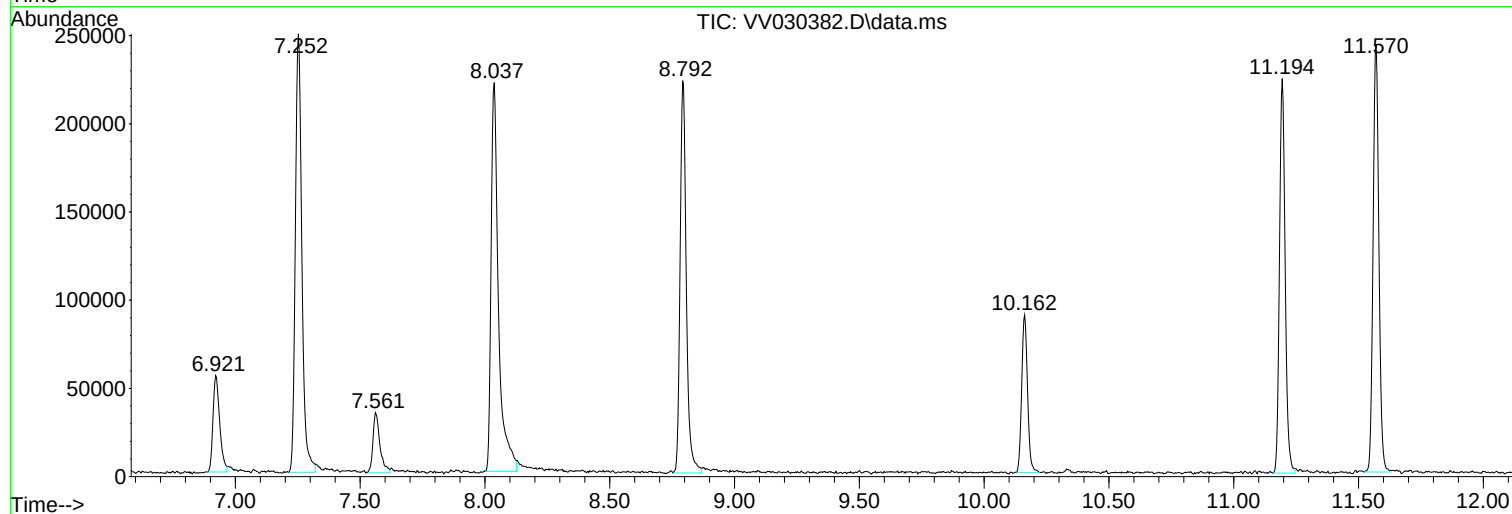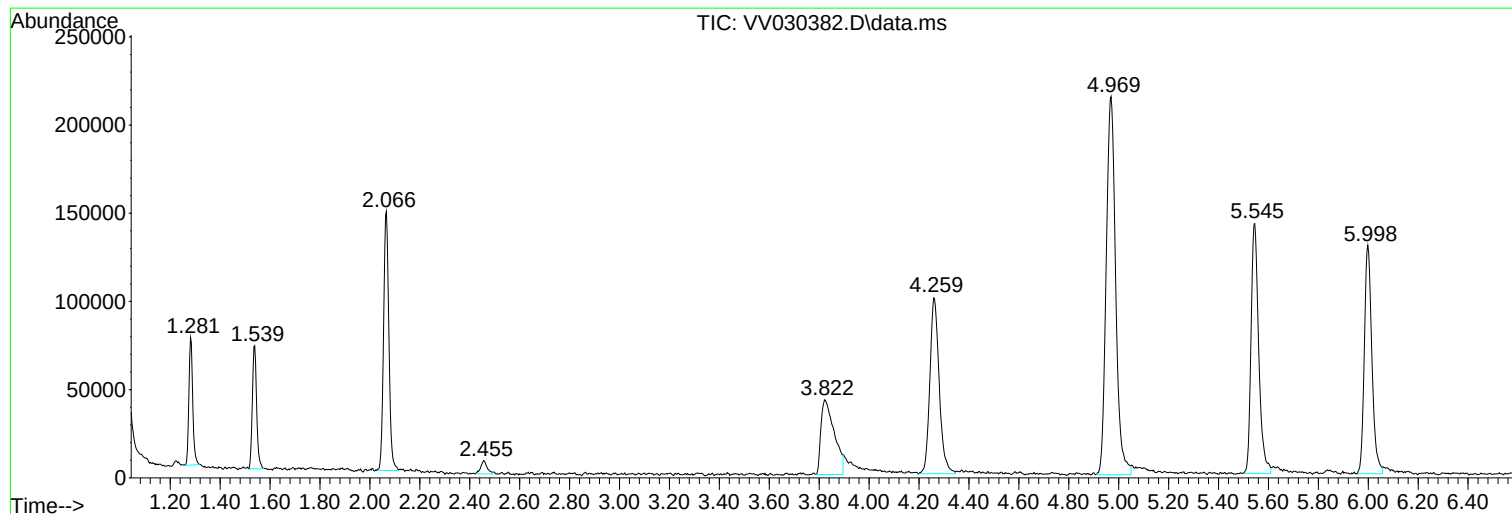

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033123\
Data File : VV030382.D
Acq On : 31 Mar 2023 14:15
Operator : SY/MD
Sample : 02092-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033123\
Data File : VV030382.D
Acq On : 31 Mar 2023 14:15
Operator : SY/MD
Sample : 02092-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc