


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV040119\
 Data File : VV010045.D
 Acq On : 01 Apr 2019 10:09
 Operator : SY/MD
 Sample : BFB81
 Misc : 5.00G/10mL/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB81

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040119S.M
 Title : VOC Analysis
 Last Update : Mon Apr 01 21:03:00 2019

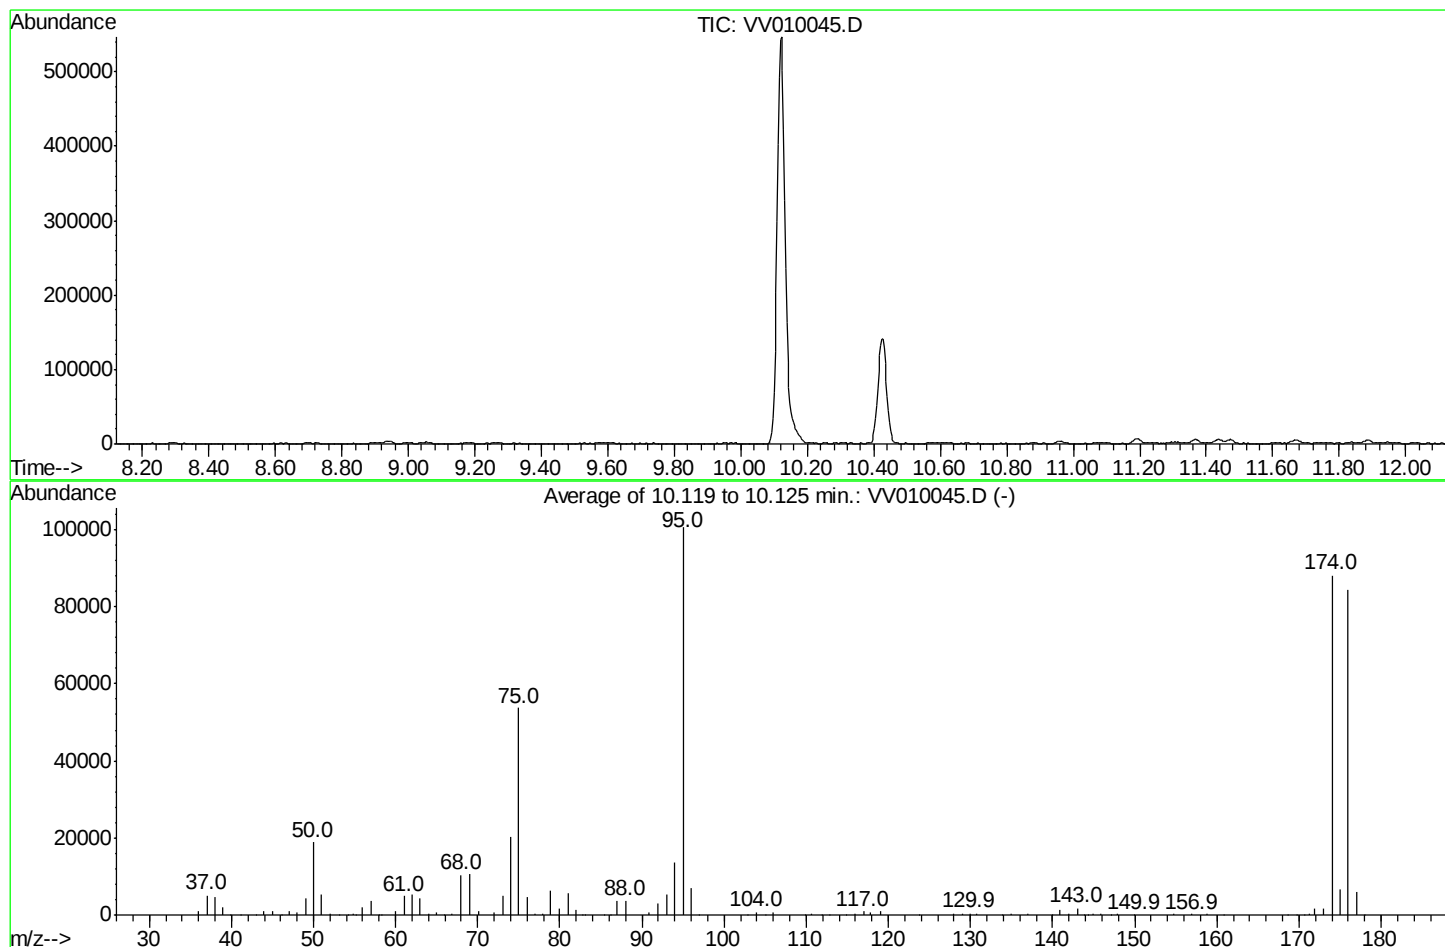

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	18808	PASS
75	95	30	80	53.4	53693	PASS
95	95	100	100	100.0	100600	PASS
96	95	5	9	6.8	6820	PASS
173	174	0.00	2	1.9	1672	PASS
174	95	50	120	87.6	88154	PASS
175	174	5	9	7.6	6732	PASS
176	174	95	101	95.6	84258	PASS
177	176	5	9	7.0	5879	PASS

Scan 2795 (10.077 min): VV010045.D
BFB81

m/z	Abundance
39.90	172.0
42.90	133.0
43.90	239.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
36.00	1096.0
37.00	5220.0
38.00	4848.0
39.00	2242.0
40.00	164.0
43.10	246.0
44.00	1227.0
45.00	916.0
46.10	172.0
47.00	1053.0
47.90	743.0
49.10	4731.0
50.00	19744.0
51.00	5895.0
52.00	452.0
53.10	130.0
54.80	256.0
55.20	272.0
55.90	1819.0
57.00	3856.0
58.10	149.0
60.00	881.0
61.00	4765.0
62.00	6002.0
63.00	4679.0
63.90	455.0
64.90	853.0
65.90	202.0
66.90	421.0
68.00	11146.0
69.00	10932.0
70.00	918.0
71.90	557.0
73.00	4857.0
74.00	20440.0
75.00	55936.0
76.10	4543.0
77.10	479.0
77.80	490.0
78.90	6681.0
79.90	1834.0
80.90	5687.0
81.90	1270.0
83.10	299.0
85.40	104.0
87.00	4070.0
88.00	4158.0
90.90	712.0
92.00	3021.0
93.00	5187.0
94.00	13565.0
95.00	102464.0
96.00	7259.0
96.90	171.0
103.90	753.0
105.00	153.0
105.90	662.0
109.80	146.0
110.70	163.0
111.90	192.0
112.80	117.0
114.90	161.0
115.90	534.0
116.90	1016.0
117.80	597.0
119.00	1044.0
123.80	195.0
127.90	474.0
129.00	208.0
129.90	508.0
130.80	291.0
133.80	164.0
134.90	210.0
137.00	230.0
140.90	1351.0
142.00	242.0
143.00	1726.0
143.90	113.0
144.90	410.0
145.90	197.0
147.10	114.0
147.80	265.0
150.00	102.0
154.90	193.0
156.90	334.0
158.80	163.0
168.60	109.0
169.70	123.0
171.20	318.0
172.00	1587.0
173.00	1653.0
174.00	88736.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

175.00	7095.0
176.00	84344.0
177.00	6100.0
178.00	160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
36.00	1088.0
37.00	5223.0
38.00	4744.0
39.00	2193.0
40.00	163.0
43.10	257.0
43.90	1102.0
45.00	916.0
46.10	198.0
47.00	1084.0
47.90	741.0
49.10	4561.0
50.00	19352.0
51.00	5434.0
52.00	410.0
53.10	127.0
54.20	116.0
54.80	214.0
56.00	1968.0
57.00	3864.0
57.90	167.0
60.10	862.0
61.00	5007.0
62.00	5447.0
63.00	4558.0
64.00	480.0
65.00	734.0
65.90	149.0
66.90	419.0
68.00	10752.0
69.00	11027.0
70.00	899.0
71.90	627.0
73.00	5037.0
74.00	21080.0
75.00	55048.0
76.10	4693.0
76.90	456.0
77.90	478.0
78.90	6507.0
80.00	1658.0
81.00	5669.0
81.90	1214.0
83.10	234.0
86.20	132.0
87.00	3917.0
88.00	3873.0
90.90	718.0
92.00	2993.0
93.00	5314.0
94.00	13912.0
95.00	103736.0
96.00	7066.0
96.90	169.0
104.00	688.0
105.00	158.0
106.00	620.0
109.80	179.0
110.70	220.0
112.00	144.0
112.80	123.0
114.90	147.0
115.90	482.0
117.00	1020.0
117.80	557.0
119.00	1004.0
123.80	116.0
128.00	454.0
129.00	203.0
130.00	459.0
130.80	277.0
133.80	145.0
135.00	201.0
137.00	220.0
140.00	113.0
140.90	1526.0
142.00	236.0
143.00	1873.0
144.30	109.0
144.90	329.0
145.90	231.0
147.80	264.0
149.90	101.0
154.80	224.0
157.00	336.0
158.90	212.0
160.90	127.0
169.70	145.0
170.70	203.0
171.20	284.0
172.00	1588.0
173.10	1662.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

174.00	91208.0
175.00	6914.0
176.00	86704.0
177.00	6084.0
178.00	181.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
36.00	1019.0
37.00	4666.0
38.00	4434.0
39.00	1946.0
39.90	203.0
41.10	115.0
43.00	227.0
44.00	969.0
45.00	846.0
46.10	157.0
47.00	881.0
47.90	716.0
49.00	3878.0
50.00	17328.0
51.00	4949.0
52.00	366.0
52.90	106.0
54.10	127.0
54.80	189.0
56.00	2026.0
57.00	3505.0
57.90	152.0
58.20	145.0
60.10	937.0
61.00	4885.0
62.00	4547.0
63.00	4181.0
64.00	526.0
65.10	664.0
65.90	105.0
66.90	319.0
68.00	9488.0
69.00	10148.0
70.10	795.0
71.90	632.0
73.00	4715.0
74.00	19072.0
75.00	50096.0
76.10	4315.0
76.90	468.0
78.00	539.0
78.90	5678.0
80.00	1373.0
81.00	5235.0
81.90	1134.0
82.80	139.0
86.10	118.0
87.00	3387.0
88.00	3381.0
90.90	609.0
92.00	2873.0
93.00	5087.0
94.00	13165.0
95.00	95600.0
96.00	6136.0
96.90	156.0
102.80	146.0
104.00	620.0
105.00	194.0
106.00	558.0
109.80	171.0
110.70	210.0
112.70	133.0
114.80	152.0
115.90	405.0
116.90	951.0
117.80	495.0
119.00	804.0
128.00	400.0
129.10	210.0
130.00	401.0
130.80	193.0
135.10	209.0
137.00	215.0
139.90	181.0
140.90	1507.0
141.90	155.0
143.00	1672.0
144.80	298.0
145.90	215.0
147.90	274.0
154.70	284.0
157.00	247.0
158.90	246.0
160.90	155.0
169.80	135.0
170.70	149.0
171.20	282.0
171.90	1461.0
173.10	1701.0
174.00	84520.0
175.00	6189.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

176.00	81728.0
177.00	5453.0
177.90	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81