
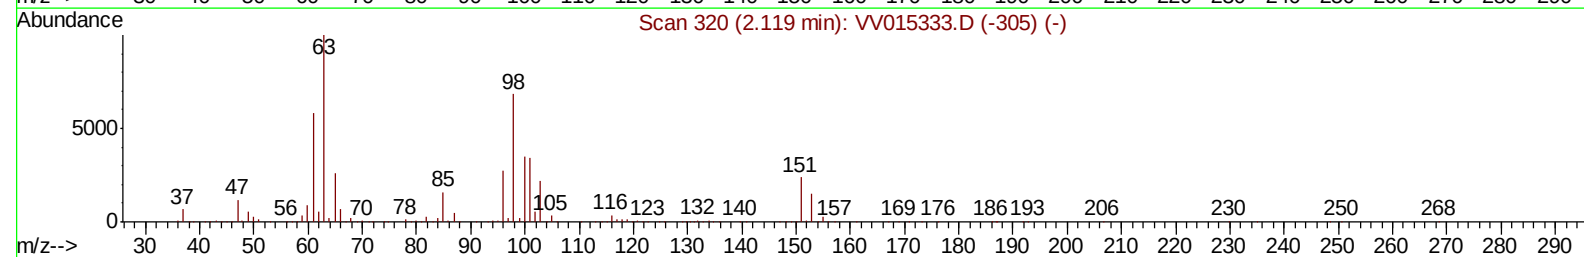
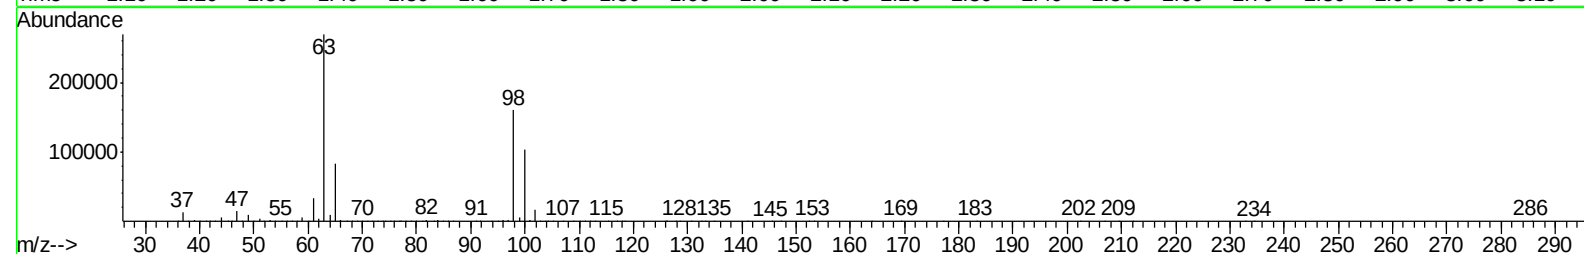


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015337.D
 Acq On : 01 Apr 2020 18:13
 Operator : SY/MD
 Sample : L1975-23
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 03:30:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 02 03:22:54 2020
 Response via : Initial Calibration

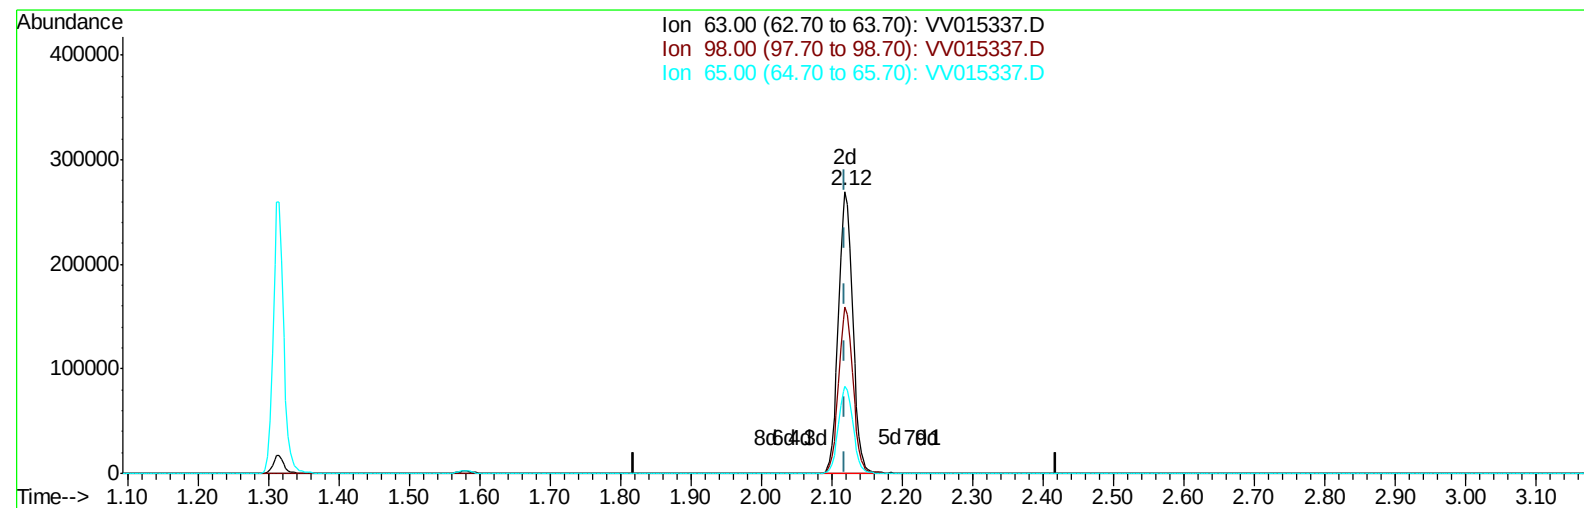

TIC: VV015337.D

(11) 1,1-Dichloroethene-d2 (S)

2.119min (-0.000) 32.89ug/L m

response 377441

Ion	Exp%	Act%
63.00	100	100
98.00	73.70	0.05#
65.00	24.00	0.03#
0.00	0.00	0.00