
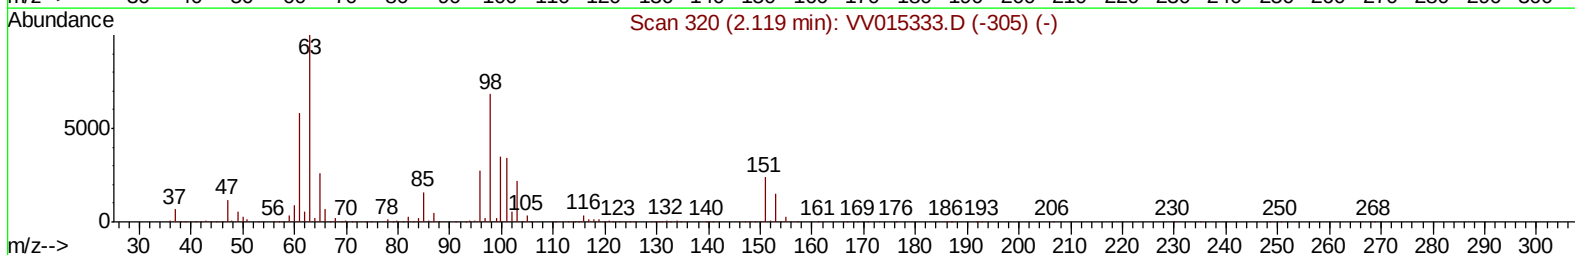
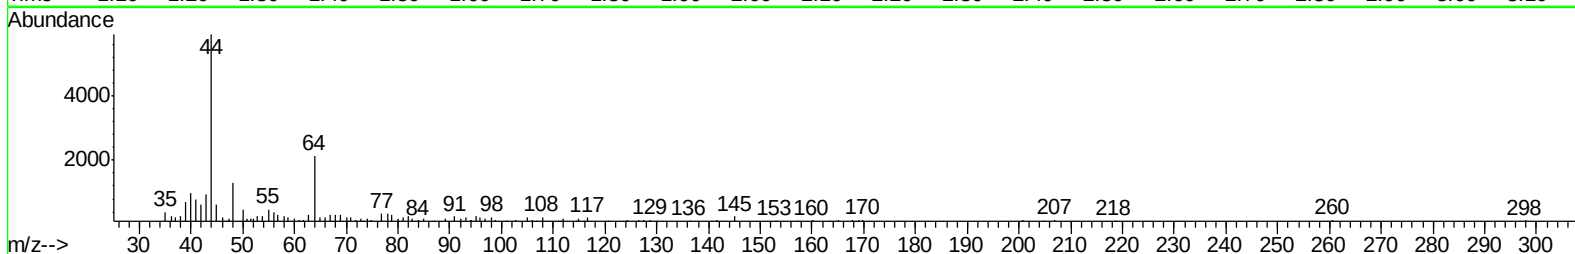


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015341.D
 Acq On : 01 Apr 2020 19:50
 Operator : SY/MD
 Sample : L2003-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 03:30:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 02 03:22:54 2020
 Response via : Initial Calibration

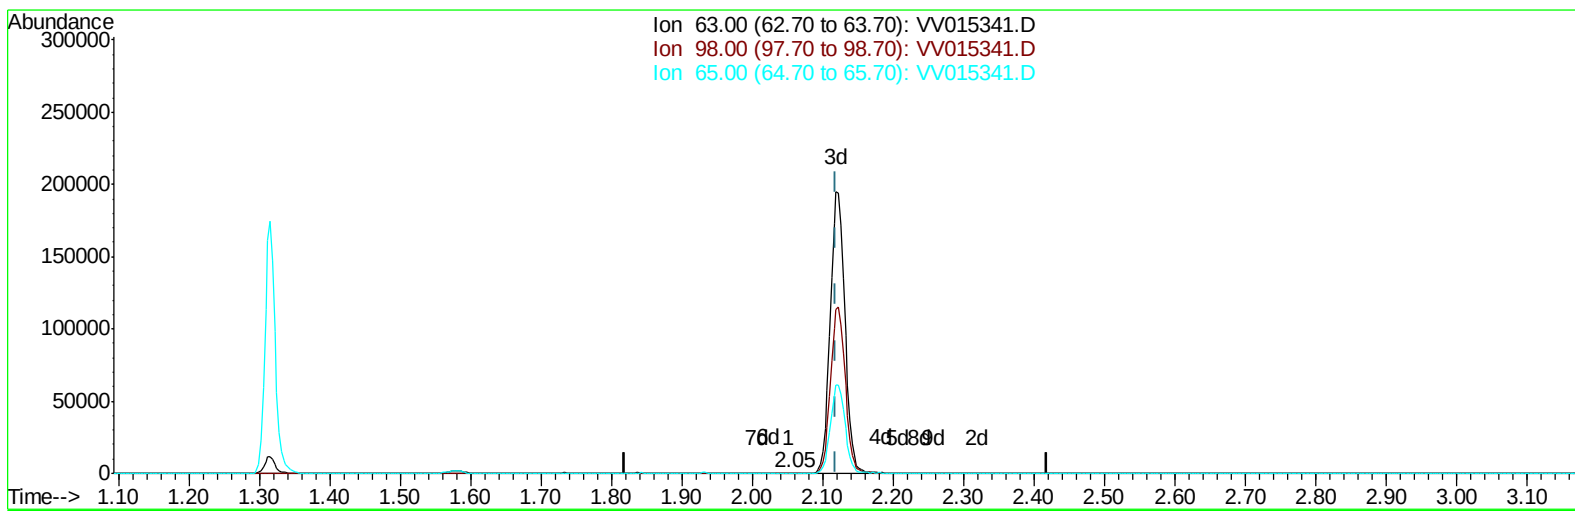

TIC: VV015341.D

(11) 1,1-Dichloroethene-d2 (S)

2.052min (-0.068) 0.03ug/L

response 378

Ion	Exp%	Act%
63.00	100	100
98.00	73.70	71.69
65.00	24.00	21.16
0.00	0.00	0.00