
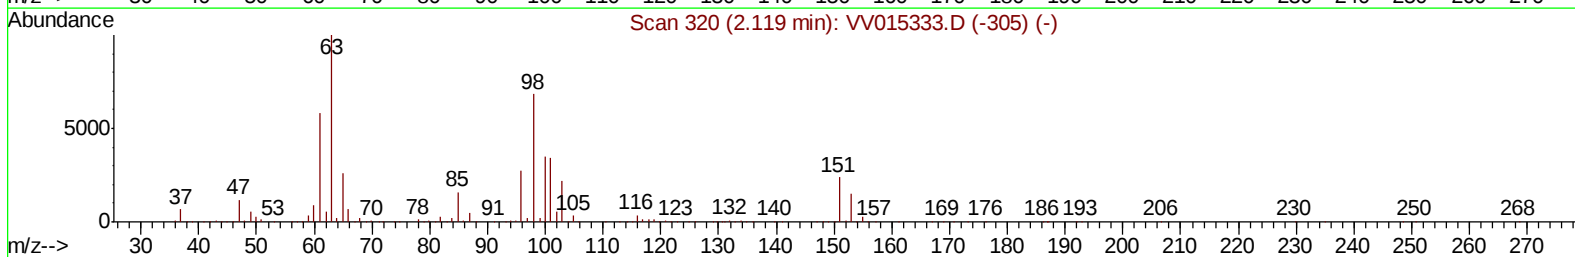
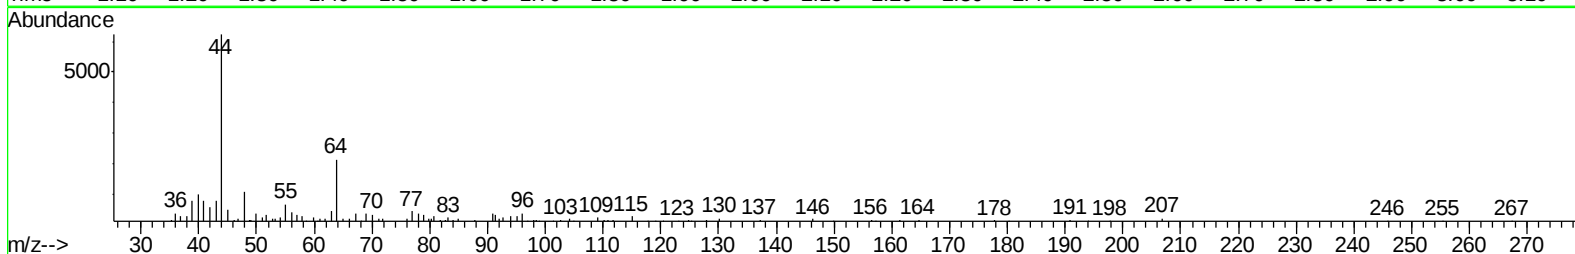


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015344.D
 Acq On : 01 Apr 2020 21:03
 Operator : SY/MD
 Sample : L2003-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 03:30:59 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 02 03:22:54 2020
 Response via : Initial Calibration

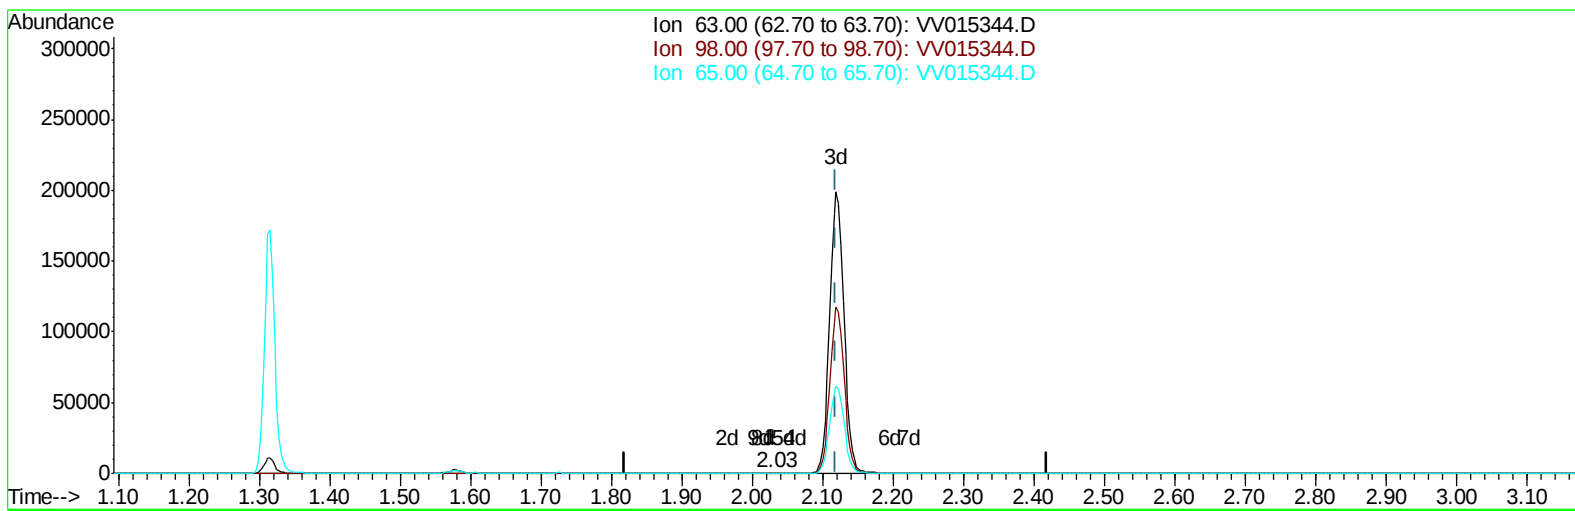

TIC: VV015344.D

(11) 1,1-Dichloroethene-d2 (S)

2.026min (-0.093) 0.02ug/L

response 280

Ion	Exp%	Act%
63.00	100	100
98.00	73.70	57.14
65.00	24.00	19.29
0.00	0.00	0.00