
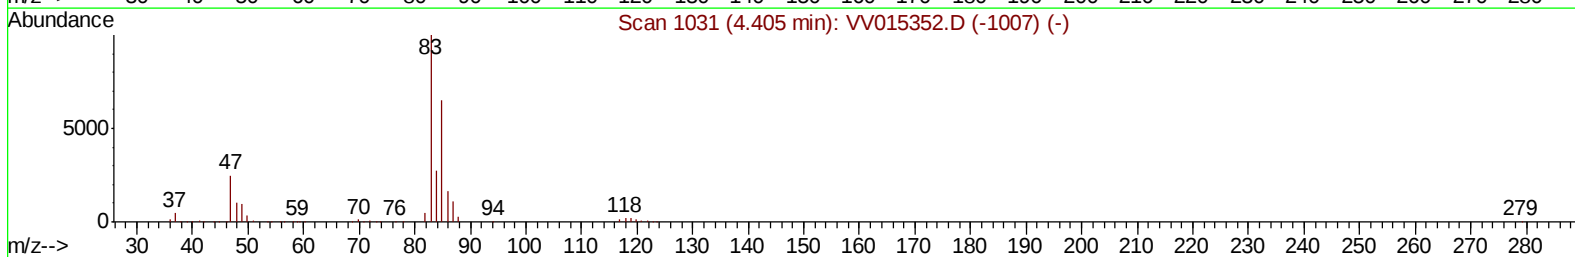
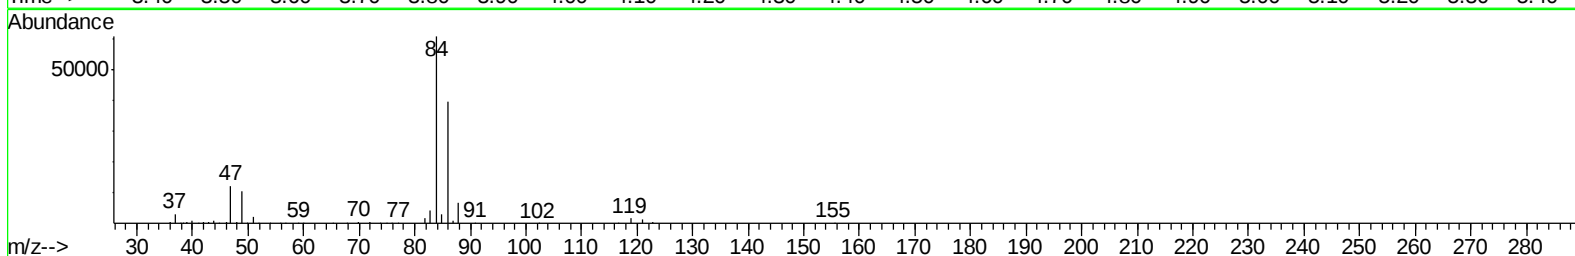


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
Data File : VV015353.D
Acq On : 02 Apr 2020 01:30
Operator : SY/MD
Sample : VV0401WBL02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 06:41:30 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 02 06:34:01 2020
Response via : Initial Calibration

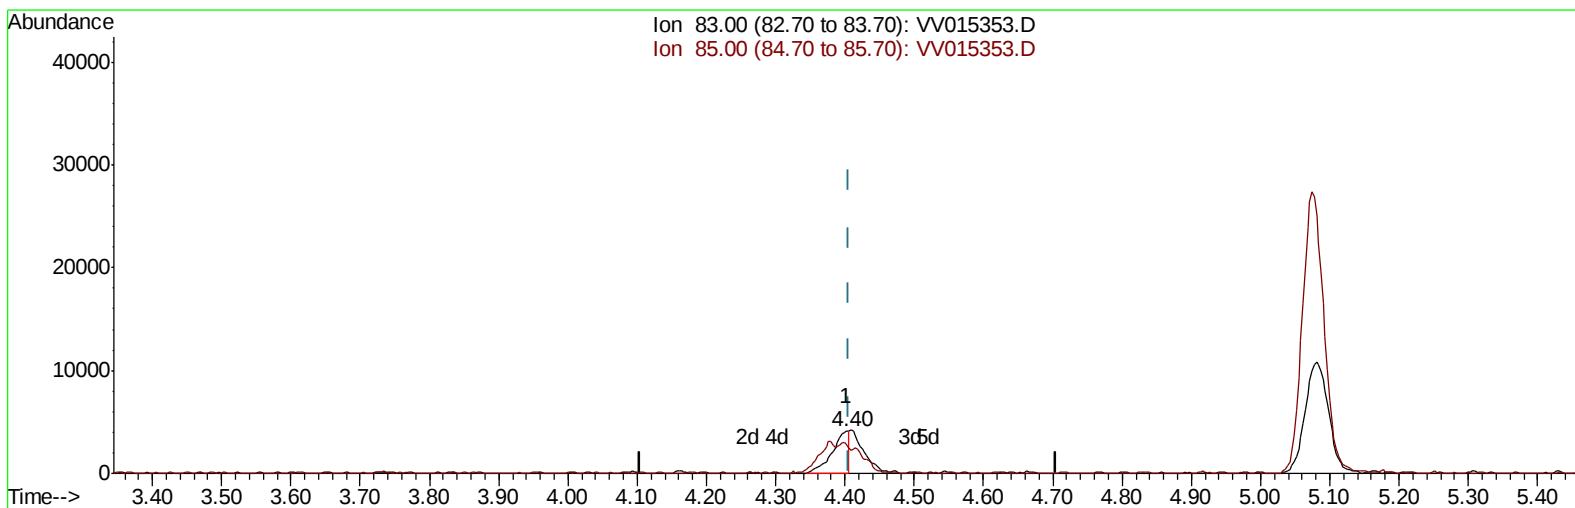

TIC: VV015353.D

(25) Chloroform (T)

4.402min (-0.003) 0.71ug/L

response 6940

Ion	Exp%	Act%
83.00	100	100
85.00	64.50	70.99
0.00	0.00	0.00
0.00	0.00	0.00