

Quantitation Report (LSC Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015348.D
 Acq On : 01 Apr 2020 22:40
 Operator : SY/MD
 Sample : L2003-01DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK0DL

Quant Time: Apr 02 06:26:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 02 03:22:54 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 4/2/2020 4:27:11 PM

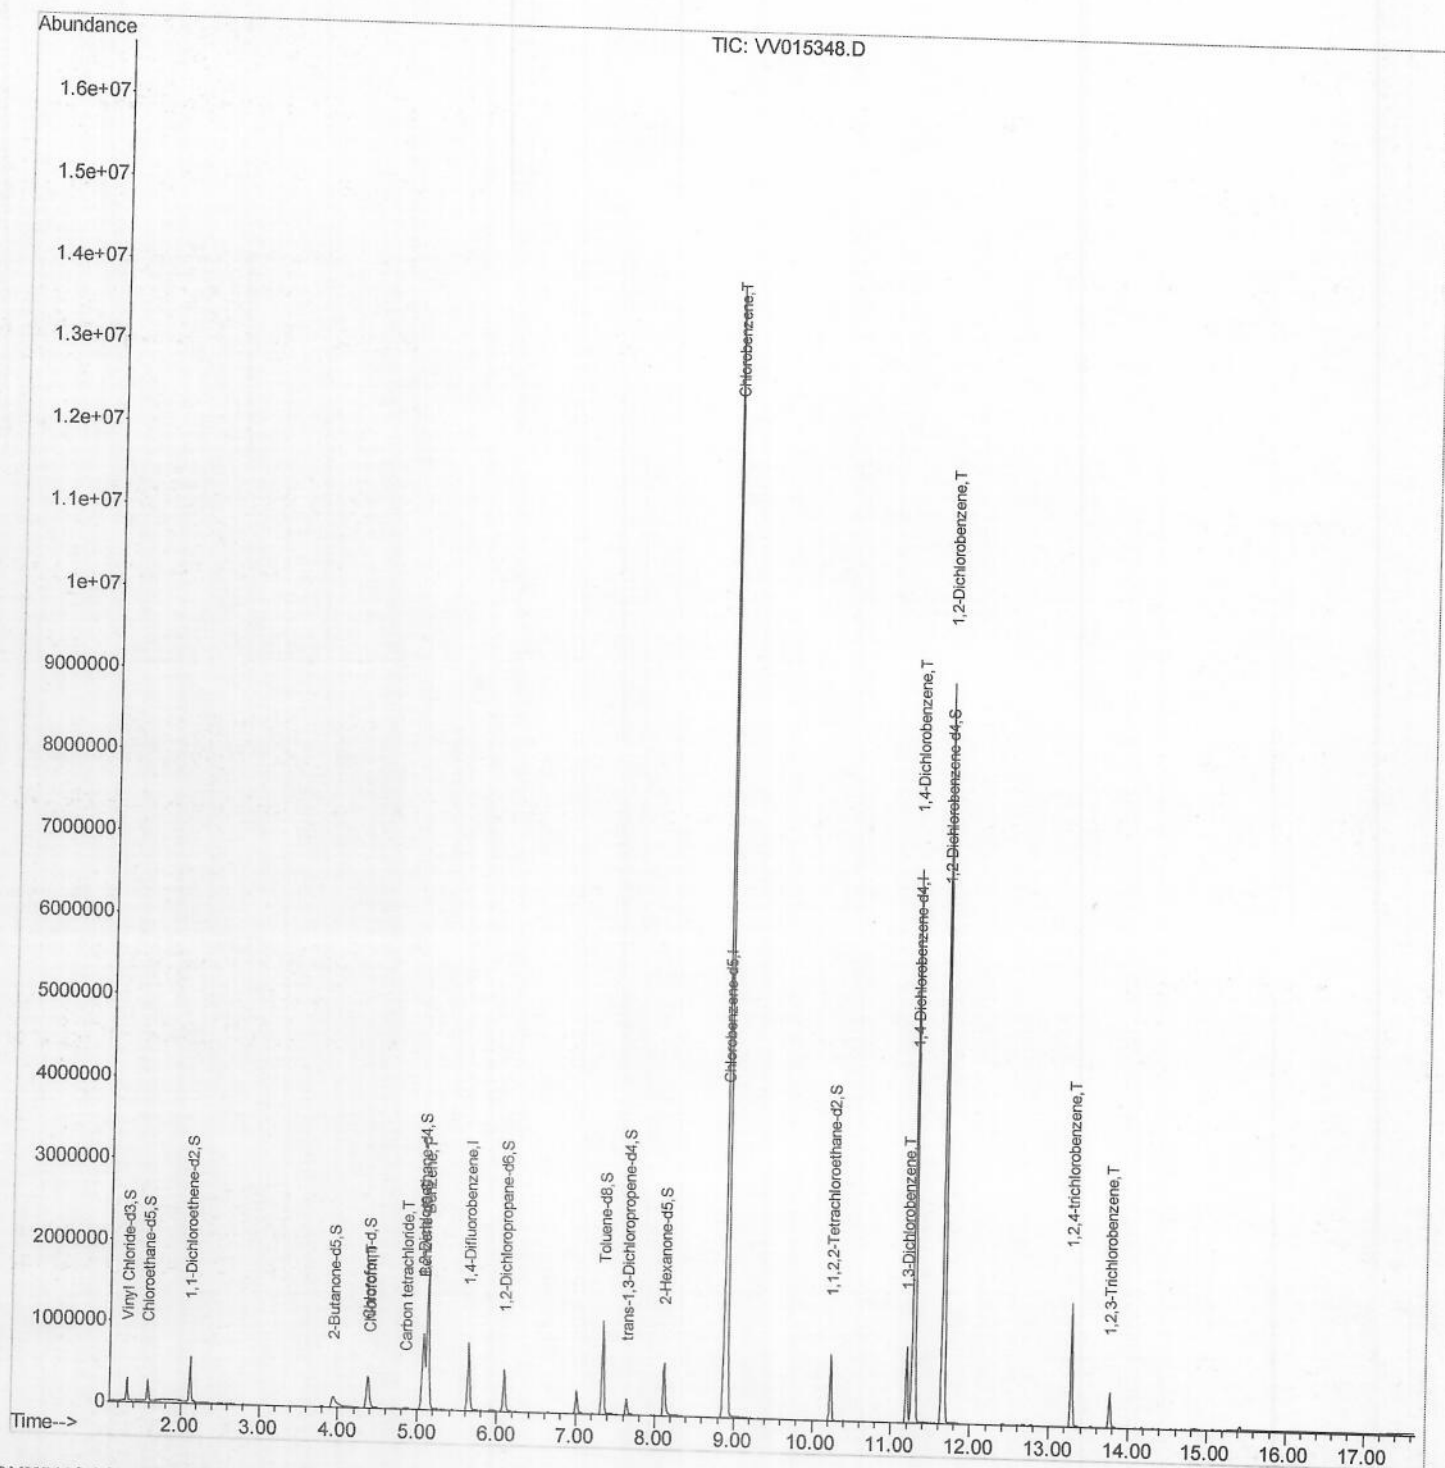

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015348.D
 Acq On : 01 Apr 2020 22:40
 Operator : SY/MD
 Sample : L2003-01DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK0DL

Manual Integrations
 APPROVED

apatel
 4/2/2020 4:27:11 PM

Quant Time: Apr 02 06:18:38 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 02 03:22:54 2020
 Response via : Initial Calibration

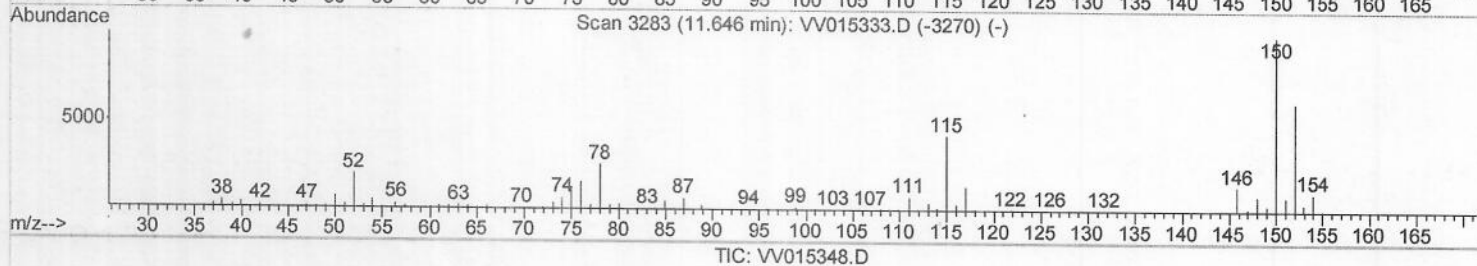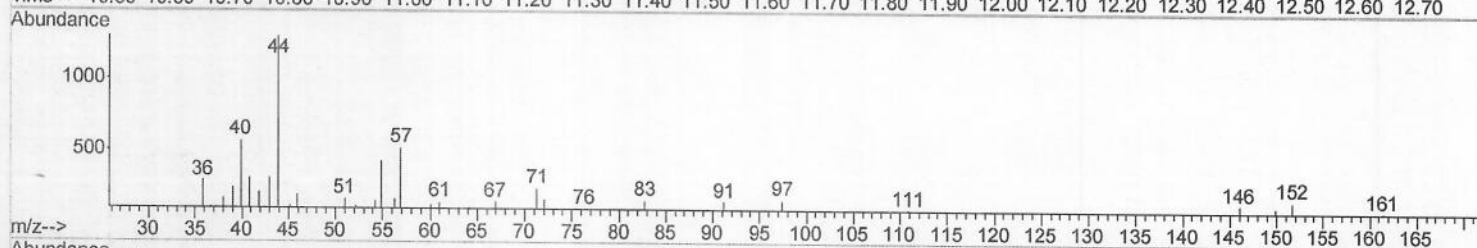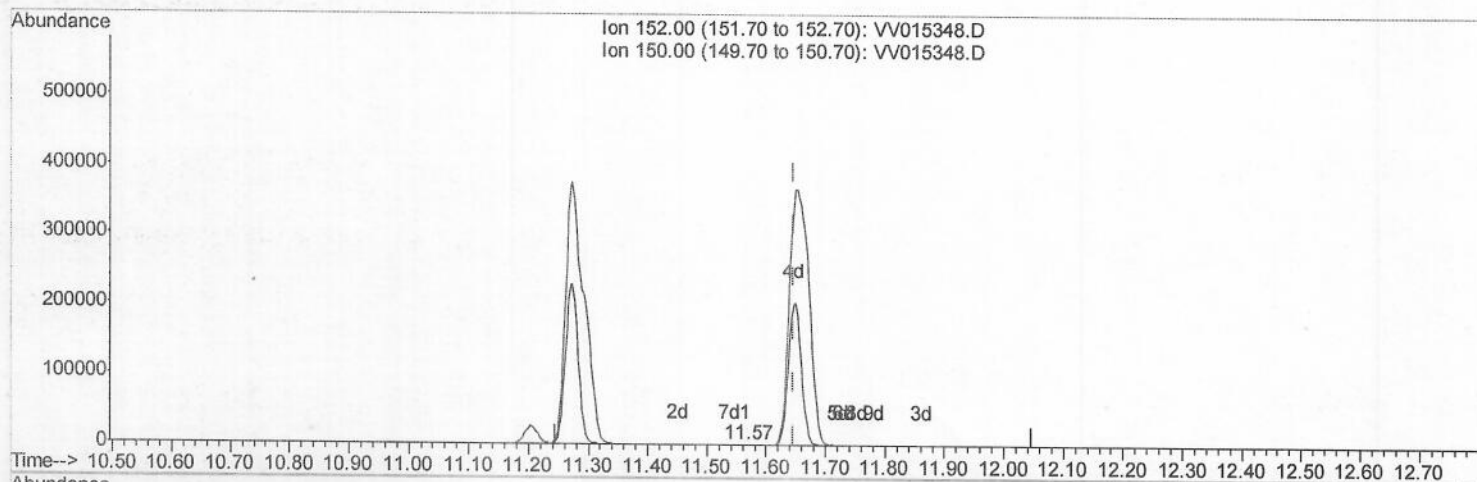

TIC: VV015348.D

(64) 1,2-Dichlorobenzene-d4 (S)

11.566min (-0.080) 0.01ug/L

response 89

Ion	Exp%	Act%
152.00	100	100
150.00	174.90	139.33
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015348.D
 Acq On : 01 Apr 2020 22:40
 Operator : SY/MD
 Sample : L2003-01DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EK0DL

Manual Integrations
 APPROVED

apatel
 4/2/2020 4:27:11 PM

Quant Time: Apr 02 06:18:38 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 02 03:22:54 2020
 Response via : Initial Calibration

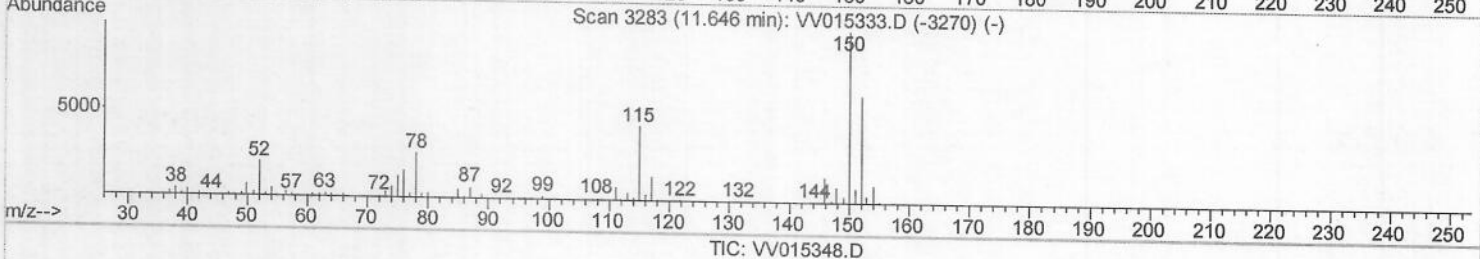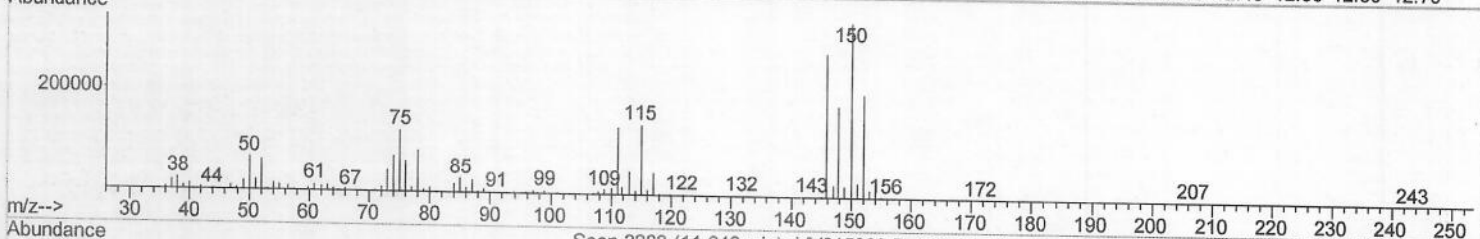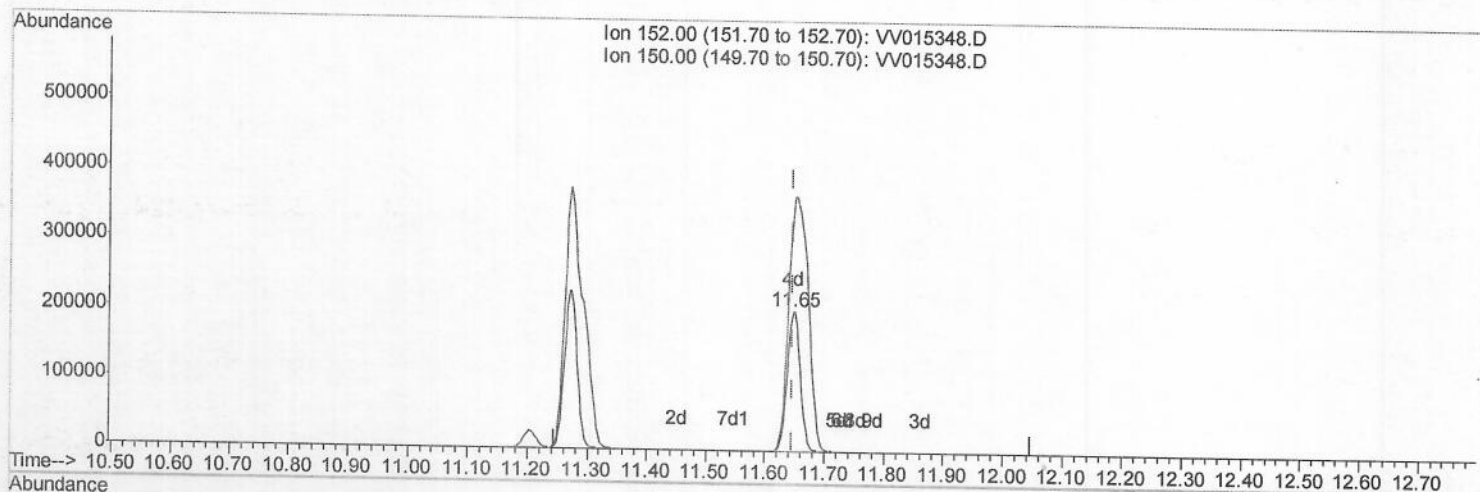

(64) 1,2-Dichlorobenzene-d4 (S)

11.646min (-0.000) 40.46ug/L m

response 315518

Ion	Exp%	Act%
152.00	100	100
150.00	174.90	0.04#
0.00	0.00	0.00
0.00	0.00	0.00

MD
 04/2/2020

Quantitation Report (LSC Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015348.D
 Acq On : 01 Apr 2020 22:40
 Operator : SY/MD
 Sample : L2003-01DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COEK0DL

Manual Integrations
 APPROVED

apatel
 4/2/2020 4:27:11 PM

Quant Time: Apr 02 06:26:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 02 03:22:54 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	734773	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	710990	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	342828	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	174201	26.44	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	52.88%#		
7) Chloroethane-d5	1.58	69	173031	30.74	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	61.48%#		
11) 1,1-Dichloroethene-d2	2.12	63	282927	24.03	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	48.06%#		
21) 2-Butanone-d5	3.94	46	312263	89.17	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	89.17%		
24) Chloroform-d	4.38	84	389260	35.79	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	71.58%		
26) 1,2-Dichloroethane-d4	5.06	65	254895	37.62	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	75.24%		
32) Benzene-d6	5.08	84	786013	35.90	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	71.80%		
36) 1,2-Dichloropropane-d6	6.09	67	242391	37.55	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	75.10%		
41) Toluene-d8	7.34	98	762761	36.43	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	72.86%#		
43) trans-1,3-Dichloropropene-	7.64	79	110975	31.11	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	62.22%		
47) 2-Hexanone-d5	8.12	63	242263	82.17	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	82.17%		
57) 1,1,2,2-Tetrachloroethane-	10.24	84	373847	40.70	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	81.40%		
64) 1,2-Dichlorobenzene-d4	11.65	152	315518m	40.46	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	80.92%		

Target Compounds

					Ovalue	
25) Chloroform	4.41	83	31508	3.181	ug/L	99
31) Carbon tetrachloride	4.86	117	8353	1.069	ug/L	100
33) Benzene	5.13	78	1741983	82.778	ug/L	100
51) Chlorobenzene	8.90	112	7399972	482.768	ug/L	98
62) 1,3-Dichlorobenzene	11.20	146	365301	31.651	ug/L	99
63) 1,4-Dichlorobenzene	11.30	146	2647565	226.185	ug/L	98
65) 1,2-Dichlorobenzene	11.67	146	3472574	294.992	ug/L	99
68) 1,2,4-trichlorobenzene	13.29	180	433586	62.059	ug/L	99
70) 1,2,3-Trichlorobenzene	13.77	180	120117	16.690	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed