

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015342.D
 Acq On : 01 Apr 2020 20:14
 Operator : SY/MD
 Sample : L2005-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	298819	294563	12.87%	1.535%
2	1.579	146	152	164	rVB	265026	308931	13.50%	1.610%
3	2.119	312	320	334	rVB	538828	758097	33.13%	3.951%
4	3.241	667	669	670	rBV2	1535	815	0.04%	0.004%
5	3.331	695	697	699	rBV2	785	439	0.02%	0.002%
6	3.470	737	740	744	rBV4	2757	2751	0.12%	0.014%
7	3.708	812	814	816	rBV3	1390	516	0.02%	0.003%
8	3.833	849	853	854	rBV3	1186	747	0.03%	0.004%
9	3.933	872	884	916	rBV	139408	511398	22.35%	2.665%
10	4.376	1003	1022	1044	rBV	392564	971585	42.46%	5.063%
11	4.685	1114	1118	1122	rVB6	2047	1786	0.08%	0.009%
12	4.711	1122	1126	1128	rBV5	1743	1363	0.06%	0.007%
13	4.817	1157	1159	1161	rBV3	1592	672	0.03%	0.004%
14	4.933	1192	1195	1198	rBV3	1657	1142	0.05%	0.006%
15	5.074	1222	1239	1264	rBV2	905662	2288272	100.00%	11.925%
16	5.592	1397	1400	1401	rBV3	2340	1378	0.06%	0.007%
17	5.643	1402	1416	1446	rVV	818321	1653169	72.25%	8.615%
18	6.093	1544	1556	1578	rBV	521567	1055040	46.11%	5.498%
19	6.389	1645	1648	1651	rBV5	1386	1248	0.05%	0.007%
20	6.453	1665	1668	1670	rBV3	1825	1111	0.05%	0.006%
21	6.495	1679	1681	1684	rBV3	1240	890	0.04%	0.005%
22	6.540	1691	1695	1698	rBV5	2947	2701	0.12%	0.014%
23	6.675	1736	1737	1743	rVB5	1961	1374	0.06%	0.007%
24	6.920	1811	1813	1816	rVB4	1760	851	0.04%	0.004%
25	6.958	1823	1825	1827	rBV3	1042	477	0.02%	0.002%
26	7.010	1829	1841	1864	rVV	290695	530314	23.18%	2.764%
27	7.257	1913	1918	1920	rBV7	1892	1496	0.07%	0.008%
28	7.338	1931	1943	1963	rBV	1128328	1942606	84.89%	10.124%
29	7.585	2017	2020	2024	rVB6	1856	1298	0.06%	0.007%
30	7.643	2028	2038	2058	rVV	205603	349660	15.28%	1.822%
31	7.887	2112	2114	2115	rBV2	1273	351	0.02%	0.002%
32	7.965	2130	2138	2146	rBV3	8798	14657	0.64%	0.076%
33	8.116	2173	2185	2221	rBV2	626061	1297937	56.72%	6.764%
34	8.530	2312	2314	2315	rBV2	1331	553	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015342.D
 Acq On : 01 Apr 2020 20:14
 Operator : SY/MD
 Sample : L2005-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DE7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

35	8.598	2332	2335	2338	rBV4	1927	1389	0.06%	0.007%
36	8.720	2371	2373	2375	rBV3	1090	458	0.02%	0.002%
37	8.736	2376	2378	2381	rVV3	1465	938	0.04%	0.005%
38	8.772	2384	2389	2392	rVB7	1917	1707	0.07%	0.009%
39	8.797	2395	2397	2400	rBV4	1513	1017	0.04%	0.005%
40	8.874	2408	2421	2447	rBV	1247523	2027523	88.60%	10.566%
41	9.270	2540	2544	2547	rVB5	2059	1688	0.07%	0.009%
42	9.286	2547	2549	2550	rBV2	1208	445	0.02%	0.002%
43	9.331	2561	2563	2565	rBV3	1109	675	0.03%	0.004%
44	9.373	2572	2576	2578	rBV5	1724	1146	0.05%	0.006%
45	9.466	2602	2605	2607	rBV4	1094	754	0.03%	0.004%
46	9.505	2614	2617	2619	rVB4	1413	805	0.04%	0.004%
47	9.665	2665	2667	2668	rBV3	848	462	0.02%	0.002%
48	9.698	2674	2677	2678	rBV3	1725	931	0.04%	0.005%
49	9.717	2681	2683	2684	rBV2	1705	788	0.03%	0.004%
50	9.755	2693	2695	2701	rBV7	2293	1790	0.08%	0.009%
51	9.810	2709	2712	2715	rBV4	1727	1006	0.04%	0.005%
52	9.836	2716	2720	2721	rBV3	2040	1325	0.06%	0.007%
53	9.948	2752	2755	2757	rBV3	1613	1060	0.05%	0.006%
54	10.048	2778	2786	2787	rBV7	6166	6211	0.27%	0.032%
55	10.093	2798	2800	2804	rVB5	2226	1405	0.06%	0.007%
56	10.119	2805	2808	2812	rVB5	1223	811	0.04%	0.004%
57	10.141	2812	2815	2816	rBV3	737	366	0.02%	0.002%
58	10.238	2832	2845	2860	rBV	805218	1251944	54.71%	6.524%
59	10.405	2888	2897	2910	rBV4	14082	25289	1.11%	0.132%
60	10.460	2912	2914	2917	rBV4	1325	692	0.03%	0.004%
61	10.476	2917	2919	2922	rBV3	1762	970	0.04%	0.005%
62	10.534	2935	2937	2939	rVB3	1009	356	0.02%	0.002%
63	10.553	2939	2943	2945	rBV4	2441	1815	0.08%	0.009%
64	10.672	2978	2980	2982	rVB3	2241	898	0.04%	0.005%
65	10.682	2982	2983	2984	rBV	618	231	0.01%	0.001%
66	10.698	2985	2988	2991	rVB5	1693	987	0.04%	0.005%
67	10.723	2991	2996	2998	rBV5	1926	1570	0.07%	0.008%
68	10.862	3037	3039	3040	rBV2	1028	429	0.02%	0.002%
69	11.083	3103	3108	3109	rBV5	2459	1631	0.07%	0.008%
70	11.122	3116	3120	3126	rBV9	2124	2369	0.10%	0.012%
71	11.270	3154	3166	3188	rBV	1243353	1943904	84.95%	10.130%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015342.D
 Acq On : 01 Apr 2020 20:14
 Operator : SY/MD
 Sample : L2005-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DE7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

72	11.646	3272	3283	3303	rBV	1175798	1875166	81.95%	9.772%
73	12.373	3503	3509	3519	rBV	7021	11870	0.52%	0.062%
74	12.450	3531	3533	3537	rBV5	2146	1579	0.07%	0.008%
75	12.482	3541	3543	3546	rBV4	1756	1162	0.05%	0.006%
76	12.508	3549	3551	3556	rVB5	1623	1091	0.05%	0.006%
77	12.665	3594	3600	3601	rBV4	2566	2436	0.11%	0.013%
78	12.743	3621	3624	3625	rBV3	2175	1111	0.05%	0.006%
79	13.006	3702	3706	3708	rBV4	1756	1615	0.07%	0.008%
80	13.215	3767	3771	3772	rBV3	1543	1004	0.04%	0.005%
81	13.714	3923	3926	3927	rBV3	1684	981	0.04%	0.005%
82	14.138	4055	4058	4059	rBV2	1734	990	0.04%	0.005%
83	14.286	4100	4104	4107	rBV4	2486	1779	0.08%	0.009%


Sum of corrected areas: 19188757

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV040120\
Data File : VV015342.D
Acq On : 01 Apr 2020 20:14
Operator : SY/MD
Sample : L2005-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CODE7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

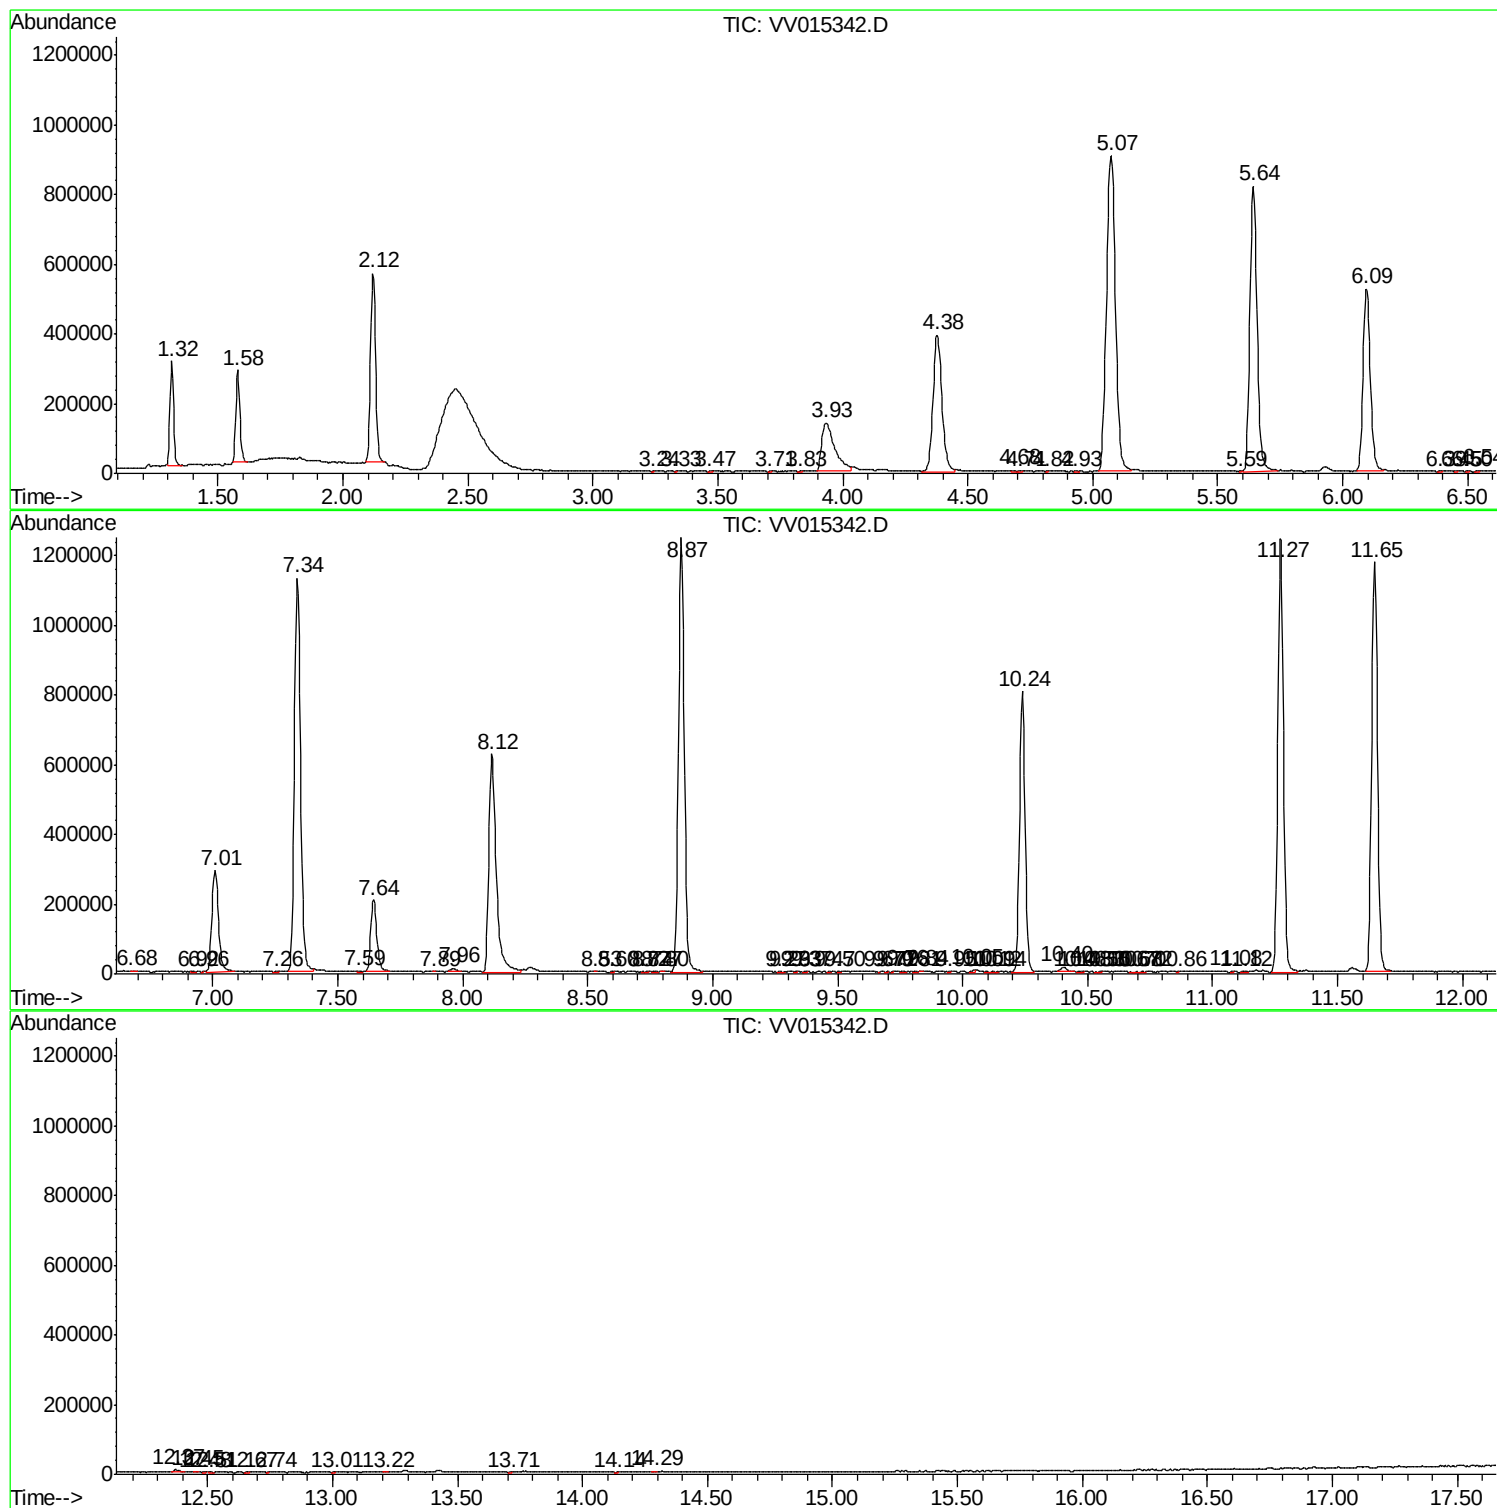

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV040120\
Data File : VV015342.D
Acq On : 01 Apr 2020 20:14
Operator : SY/MD
Sample : L2005-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DE7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV040120\
Data File : VV015342.D
Acq On : 01 Apr 2020 20:14
Operator : SY/MD
Sample : L2005-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DE7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc