

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015348.D
 Acq On : 01 Apr 2020 22:40
 Operator : SY/MD
 Sample : L2003-01DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EKODL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	83	rVB	278935	291942	1.20%	0.418%
2	1.579	145	152	164	rBV	260598	310728	1.28%	0.445%
3	2.119	312	320	331	rVB	545948	765739	3.15%	1.097%
4	3.033	602	604	607	rBV4	1890	1290	0.01%	0.002%
5	3.296	682	686	688	rBV5	2935	2158	0.01%	0.003%
6	3.344	698	701	706	rVB6	2134	1888	0.01%	0.003%
7	3.373	706	710	715	rBV7	3095	3226	0.01%	0.005%
8	3.396	715	717	721	rBV5	1547	1024	0.00%	0.001%
9	3.428	725	727	729	rBV3	1921	1182	0.00%	0.002%
10	3.457	734	736	740	rBV4	1253	672	0.00%	0.001%
11	3.582	772	775	777	rBV3	1931	1305	0.01%	0.002%
12	3.650	793	796	800	rVB5	1616	1037	0.00%	0.001%
13	3.679	802	805	808	rBV5	1903	1406	0.01%	0.002%
14	3.788	828	839	852	rBV5	5288	14056	0.06%	0.020%
15	3.885	866	869	872	rBV4	1244	779	0.00%	0.001%
16	3.939	873	886	929	rBV	128919	601417	2.47%	0.862%
17	4.377	1008	1022	1047	rVB	379344	963432	3.96%	1.380%
18	4.650	1104	1107	1110	rBV4	2115	1370	0.01%	0.002%
19	4.672	1110	1114	1116	rBV5	1561	1302	0.01%	0.002%
20	5.074	1219	1239	1246	rBV2	923975	2214301	9.11%	3.173%
21	5.431	1345	1350	1353	rBV6	3509	3013	0.01%	0.004%
22	5.569	1389	1393	1396	rBV5	2763	2699	0.01%	0.004%
23	5.640	1402	1415	1449	rBV	832032	1656401	6.82%	2.373%
24	5.881	1487	1490	1494	rVB5	2290	1596	0.01%	0.002%
25	5.936	1494	1507	1516	rBV8	12253	27893	0.11%	0.040%
26	6.039	1535	1539	1540	rBV3	1419	826	0.00%	0.001%
27	6.093	1544	1556	1580	rVB	510413	1026364	4.22%	1.471%
28	6.412	1653	1655	1659	rVB5	1095	565	0.00%	0.001%
29	6.438	1659	1663	1665	rBV5	1838	1490	0.01%	0.002%
30	6.508	1680	1685	1688	rBV6	2305	1868	0.01%	0.003%
31	6.528	1688	1691	1693	rVV5	1249	659	0.00%	0.001%
32	6.582	1705	1708	1713	rVB5	2123	1730	0.01%	0.002%
33	6.614	1713	1718	1719	rBV5	1915	1305	0.01%	0.002%
34	6.634	1719	1724	1725	rBV4	2408	1981	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015348.D
 Acq On : 01 Apr 2020 22:40
 Operator : SY/MD
 Sample : L2003-01DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EKODL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

35	6.749	1758	1760	1763	rVB3	1624	814	0.00%	0.001%
36	6.778	1766	1769	1770	rBV3	1073	653	0.00%	0.001%
37	6.820	1778	1782	1783	rBV3	1056	711	0.00%	0.001%
38	6.855	1791	1793	1795	rVB3	2590	1194	0.00%	0.002%
39	6.868	1795	1797	1800	rBV4	1190	967	0.00%	0.001%
40	6.939	1810	1819	1820	rBV8	1911	1741	0.01%	0.002%
41	7.007	1828	1840	1867	rBV	284679	522277	2.15%	0.748%
42	7.145	1881	1883	1886	rBV5	1314	893	0.00%	0.001%
43	7.338	1931	1943	1962	rBV	1144171	1965617	8.09%	2.816%
44	7.643	2027	2038	2051	rBV	200900	336622	1.39%	0.482%
45	7.843	2098	2100	2106	rVB5	1364	621	0.00%	0.001%
46	7.875	2108	2110	2113	rBV3	1240	841	0.00%	0.001%
47	8.000	2145	2149	2152	rBV4	2673	2374	0.01%	0.003%
48	8.116	2174	2185	2225	rBV2	649259	1322278	5.44%	1.895%
49	8.563	2321	2324	2325	rBV3	2239	1236	0.01%	0.002%
50	8.646	2348	2350	2354	rBV4	1240	817	0.00%	0.001%
51	8.724	2372	2374	2379	rVB3	1488	1076	0.00%	0.002%
52	8.759	2382	2385	2388	rVB5	1900	1122	0.00%	0.002%
53	8.814	2399	2402	2404	rBV4	1326	788	0.00%	0.001%
54	8.830	2404	2407	2408	rBV3	1289	723	0.00%	0.001%
55	8.904	2409	2430	2465	rVV	13830334	24303767	100.00%	34.824%
56	9.322	2558	2560	2563	rVB3	1988	1011	0.00%	0.001%
57	9.547	2626	2630	2632	rBV5	2280	1663	0.01%	0.002%
58	9.560	2632	2634	2636	rBV3	1645	904	0.00%	0.001%
59	9.688	2672	2674	2675	rBV2	1592	756	0.00%	0.001%
60	9.756	2691	2695	2698	rBV6	2090	1492	0.01%	0.002%
61	9.772	2698	2700	2702	rVV3	1257	582	0.00%	0.001%
62	9.833	2717	2719	2723	rVB5	2451	1425	0.01%	0.002%
63	9.852	2723	2725	2728	rBV3	1387	1067	0.00%	0.002%
64	9.923	2744	2747	2748	rBV3	1296	789	0.00%	0.001%
65	9.949	2752	2755	2756	rBV2	1632	760	0.00%	0.001%
66	10.000	2768	2771	2772	rBV3	1516	736	0.00%	0.001%
67	10.142	2810	2815	2820	rBV9	1943	2316	0.01%	0.003%
68	10.161	2820	2821	2825	rBV3	1473	888	0.00%	0.001%
69	10.187	2827	2829	2830	rBV2	1332	567	0.00%	0.001%
70	10.238	2833	2845	2858	rBV	812630	1249016	5.14%	1.790%
71	10.334	2872	2875	2876	rBV3	1917	885	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015348.D
 Acq On : 01 Apr 2020 22:40
 Operator : SY/MD
 Sample : L2003-01DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EKODL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

72	10.402	2892	2896	2898	rBV4	3178	2880	0.01%	0.004%
73	10.437	2902	2907	2909	rBV5	2482	2197	0.01%	0.003%
74	10.479	2918	2920	2923	rVB3	2146	1206	0.00%	0.002%
75	10.495	2923	2925	2927	rBV2	1614	826	0.00%	0.001%
76	10.633	2966	2968	2970	rBV3	1487	890	0.00%	0.001%
77	10.704	2988	2990	2995	rBV5	1405	1114	0.00%	0.002%
78	10.833	3029	3030	3035	rVV5	1589	978	0.00%	0.001%
79	10.945	3061	3065	3066	rBV4	1496	1074	0.00%	0.002%
80	11.006	3080	3084	3086	rBV4	890	622	0.00%	0.001%
81	11.109	3114	3116	3119	rVB4	1609	757	0.00%	0.001%
82	11.125	3119	3121	3123	rBV3	1560	731	0.00%	0.001%
83	11.203	3132	3145	3156	rBV	920898	1420109	5.84%	2.035%
84	11.296	3157	3174	3194	rVB2	6753980	12200331	50.20%	17.482%
85	11.550	3249	3253	3258	rBV7	2842	3403	0.01%	0.005%
86	11.666	3271	3289	3311	rBV2	9056615	15475914	63.68%	22.175%
87	12.026	3397	3401	3404	rBV5	1456	1216	0.01%	0.002%
88	12.064	3411	3413	3418	rVB4	1942	1448	0.01%	0.002%
89	12.315	3488	3491	3494	rBV4	1316	1284	0.01%	0.002%
90	12.421	3512	3524	3533	rBV4	11759	22894	0.09%	0.033%
91	12.579	3568	3573	3574	rBV5	2047	1672	0.01%	0.002%
92	12.669	3593	3601	3613	rBV5	9558	16894	0.07%	0.024%
93	12.868	3659	3663	3666	rVB4	1803	1529	0.01%	0.002%
94	12.907	3671	3675	3677	rBV5	1209	964	0.00%	0.001%
95	12.945	3682	3687	3689	rBV6	1696	1427	0.01%	0.002%
96	13.067	3721	3725	3727	rBV5	1406	1229	0.01%	0.002%
97	13.203	3762	3767	3768	rBV5	1325	995	0.00%	0.001%
98	13.286	3780	3793	3808	rBV	1496753	2310948	9.51%	3.311%
99	13.768	3931	3943	3964	rBV	428486	672721	2.77%	0.964%
100	14.096	4044	4045	4048	rVB3	1843	928	0.00%	0.001%


Sum of corrected areas: 69789814

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV040120\
Data File : VV015348.D
Acq On : 01 Apr 2020 22:40
Operator : SY/MD
Sample : L2003-01DL 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EKODL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

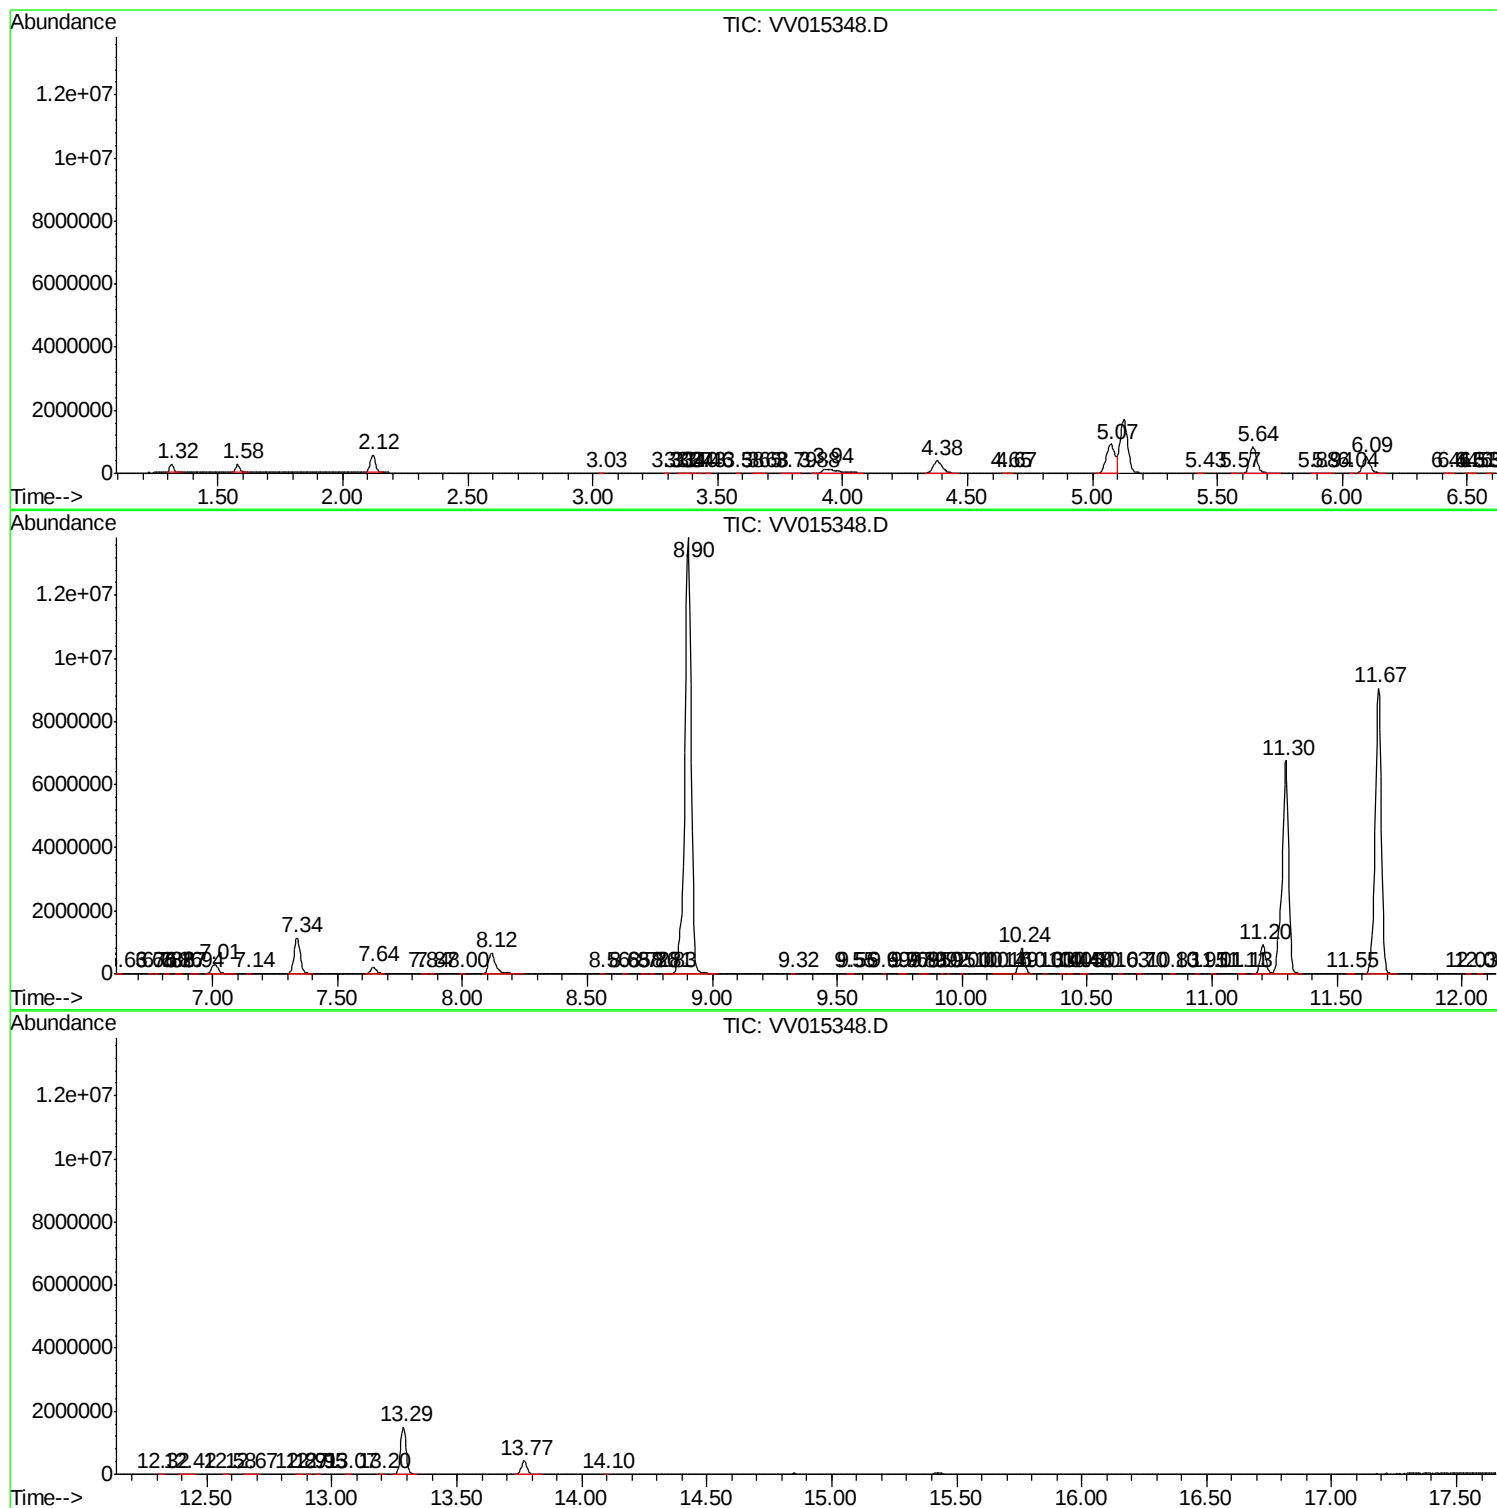

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV040120\
Data File : VV015348.D
Acq On : 01 Apr 2020 22:40
Operator : SY/MD
Sample : L2003-01DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV040120\
Data File : VV015348.D
Acq On : 01 Apr 2020 22:40
Operator : SY/MD
Sample : L2003-01DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EK0DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc