

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015353.D
 Acq On : 02 Apr 2020 03:00
 Operator : SY/MD
 Sample : L2005-03 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

Signal : TIC: VV015354.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	65	70	84	rVB	274603	271393	2.88%	0.890%
2	1.579	146	152	168	rVB	247590	300732	3.19%	0.986%
3	2.123	313	321	332	rVB	469434	670283	7.11%	2.198%
4	3.004	593	595	600	rBV5	1318	1295	0.01%	0.004%
5	3.203	652	657	658	rBV3	1818	1290	0.01%	0.004%
6	3.492	744	747	751	rBV5	2318	2092	0.02%	0.007%
7	3.560	765	768	769	rBV3	1932	866	0.01%	0.003%
8	3.666	799	801	805	rVB4	1412	740	0.01%	0.002%
9	3.746	822	826	827	rBV3	1498	921	0.01%	0.003%
10	3.878	863	867	869	rVB5	1282	691	0.01%	0.002%
11	3.939	871	886	935	rBV	113010	599257	6.35%	1.965%
12	4.373	1006	1021	1044	rBV2	367449	909482	9.64%	2.983%
13	4.952	1199	1201	1203	rBV3	1753	687	0.01%	0.002%
14	4.991	1211	1213	1216	rVB4	1988	1093	0.01%	0.004%
15	5.071	1216	1238	1267	rBV2	862545	2225941	23.60%	7.300%
16	5.640	1401	1415	1440	rBV	755476	1521342	16.13%	4.989%
17	6.093	1543	1556	1586	rVB	500616	1016376	10.77%	3.333%
18	6.466	1669	1672	1675	rBV5	1614	1438	0.02%	0.005%
19	6.601	1711	1714	1716	rBV4	1702	1163	0.01%	0.004%
20	6.765	1763	1765	1768	rBV3	1641	1024	0.01%	0.003%
21	6.801	1772	1776	1778	rBV5	916	574	0.01%	0.002%
22	6.823	1778	1783	1786	rBV8	1463	1068	0.01%	0.004%
23	6.843	1786	1789	1793	rBV6	1957	1556	0.02%	0.005%
24	6.891	1800	1804	1806	rBV4	1703	1352	0.01%	0.004%
25	6.962	1823	1826	1828	rBV3	1485	992	0.01%	0.003%
26	7.007	1829	1840	1861	rVV2	270998	490675	5.20%	1.609%
27	7.145	1880	1883	1888	rVB6	2066	1873	0.02%	0.006%
28	7.335	1930	1942	1963	rBV	1029360	1787338	18.95%	5.862%
29	7.592	2019	2022	2025	rBV4	1562	1327	0.01%	0.004%
30	7.640	2026	2037	2058	rVV	194100	335521	3.56%	1.100%
31	7.827	2092	2095	2098	rBV5	1797	1098	0.01%	0.004%
32	7.843	2098	2100	2103	rVB3	1766	723	0.01%	0.002%
33	7.923	2123	2125	2128	rVB4	1985	1073	0.01%	0.004%
34	7.952	2131	2134	2136	rBV3	2501	1843	0.02%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015353.D
 Acq On : 02 Apr 2020 03:00
 Operator : SY/MD
 Sample : L2005-03 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DE4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

35	8.039	2159	2161	2164	rVB4	1578	835	0.01%	0.003%
36	8.058	2164	2167	2170	rVB3	2142	1143	0.01%	0.004%
37	8.074	2170	2172	2174	rBV3	2030	1237	0.01%	0.004%
38	8.116	2174	2185	2214	rBV2	582250	1242210	13.17%	4.074%
39	8.524	2310	2312	2314	rBV3	1308	575	0.01%	0.002%
40	8.585	2326	2331	2333	rBV5	1775	1588	0.02%	0.005%
41	8.669	2353	2357	2360	rBV5	1584	1354	0.01%	0.004%
42	8.685	2360	2362	2365	rBV4	1191	632	0.01%	0.002%
43	8.704	2365	2368	2369	rBV3	1320	694	0.01%	0.002%
44	8.778	2385	2391	2395	rVV8	1730	1889	0.02%	0.006%
45	8.900	2408	2429	2460	rBV2	4707368	9433702	100.00%	30.939%
46	9.145	2503	2505	2508	rBV4	2128	1541	0.02%	0.005%
47	9.235	2528	2533	2534	rBV5	1777	1564	0.02%	0.005%
48	9.322	2557	2560	2562	rBV4	1664	996	0.01%	0.003%
49	9.450	2594	2600	2604	rBV7	2415	2252	0.02%	0.007%
50	9.534	2624	2626	2627	rBV2	1725	687	0.01%	0.002%
51	9.560	2631	2634	2635	rBV3	3431	1972	0.02%	0.006%
52	9.662	2664	2666	2668	rBV3	1367	568	0.01%	0.002%
53	9.798	2706	2708	2711	rVB4	1345	577	0.01%	0.002%
54	9.949	2750	2755	2761	rBV10	3287	4544	0.05%	0.015%
55	10.129	2809	2811	2814	rBV4	998	623	0.01%	0.002%
56	10.174	2823	2825	2827	rBV3	1180	585	0.01%	0.002%
57	10.238	2833	2845	2861	rBV	765670	1212427	12.85%	3.976%
58	10.341	2876	2877	2881	rBV3	2030	1586	0.02%	0.005%
59	10.505	2925	2928	2930	rBV4	1464	971	0.01%	0.003%
60	10.560	2939	2945	2955	rVB9	4898	8148	0.09%	0.027%
61	10.598	2955	2957	2958	rBV2	1750	744	0.01%	0.002%
62	10.627	2964	2966	2968	rVB3	1536	710	0.01%	0.002%
63	10.643	2968	2971	2975	rBV4	1610	1100	0.01%	0.004%
64	10.662	2975	2977	2981	rVB5	1959	1104	0.01%	0.004%
65	10.691	2981	2986	2988	rBV5	1227	1173	0.01%	0.004%
66	10.727	2995	2997	2998	rBV2	1209	524	0.01%	0.002%
67	10.814	3021	3024	3025	rBV2	1193	559	0.01%	0.002%
68	10.846	3032	3034	3036	rBV3	1053	570	0.01%	0.002%
69	10.939	3057	3063	3066	rBV7	2390	3198	0.03%	0.010%
70	11.026	3087	3090	3092	rBV4	1074	830	0.01%	0.003%
71	11.071	3101	3104	3105	rBV3	1359	827	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015353.D
 Acq On : 02 Apr 2020 03:00
 Operator : SY/MD
 Sample : L2005-03 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

72	11.090	3108	3110	3114	rVB5	1975	1063	0.01%	0.003%
73	11.135	3118	3124	3126	rBV5	1676	1423	0.02%	0.005%
74	11.161	3129	3132	3133	rBV3	1638	710	0.01%	0.002%
75	11.206	3133	3146	3155	rBV2	78362	128533	1.36%	0.422%
76	11.270	3156	3166	3197	rVB2	1253124	2455698	26.03%	8.054%
77	11.521	3240	3244	3250	rBV9	1560	1742	0.02%	0.006%
78	11.595	3265	3267	3269	rBV3	1366	776	0.01%	0.003%
79	11.662	3269	3288	3307	rVV2	2511943	5278470	55.95%	17.311%
80	11.807	3331	3333	3334	rBV2	2109	866	0.01%	0.003%
81	12.093	3420	3422	3425	rBV4	1582	1120	0.01%	0.004%
82	12.109	3425	3427	3429	rVV3	1496	754	0.01%	0.002%
83	12.129	3429	3433	3436	rVB6	1614	1289	0.01%	0.004%
84	12.180	3445	3449	3451	rBV5	2024	1624	0.02%	0.005%
85	12.232	3460	3465	3468	rBV7	1455	1374	0.01%	0.005%
86	12.363	3503	3506	3508	rBV4	1747	1232	0.01%	0.004%
87	12.534	3557	3559	3564	rBV6	1777	1532	0.02%	0.005%
88	12.598	3577	3579	3583	rBV5	1386	1059	0.01%	0.003%
89	12.707	3611	3613	3617	rBV4	1576	1290	0.01%	0.004%
90	12.810	3643	3645	3647	rVB3	1504	525	0.01%	0.002%
91	12.952	3685	3689	3690	rBV4	1709	1062	0.01%	0.003%
92	13.132	3742	3745	3748	rBV4	1710	1211	0.01%	0.004%
93	13.222	3770	3773	3774	rBV3	1815	830	0.01%	0.003%
94	13.286	3782	3793	3811	rVB	271298	421948	4.47%	1.384%
95	13.424	3833	3836	3840	rBV5	1749	1536	0.02%	0.005%
96	13.649	3904	3906	3911	rVB5	1989	1150	0.01%	0.004%
97	13.768	3932	3943	3958	rBV3	53390	88009	0.93%	0.289%
98	13.862	3970	3972	3975	rBV4	1370	1034	0.01%	0.003%
99	14.154	4061	4063	4065	rBV3	3054	1469	0.02%	0.005%
100	14.209	4078	4080	4084	rBV4	1301	912	0.01%	0.003%


Sum of corrected areas: 30491599

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV040120\
Data File : VV015353.D
Acq On : 02 Apr 2020 03:00
Operator : SY/MD
Sample : L2005-03 500X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CODE4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

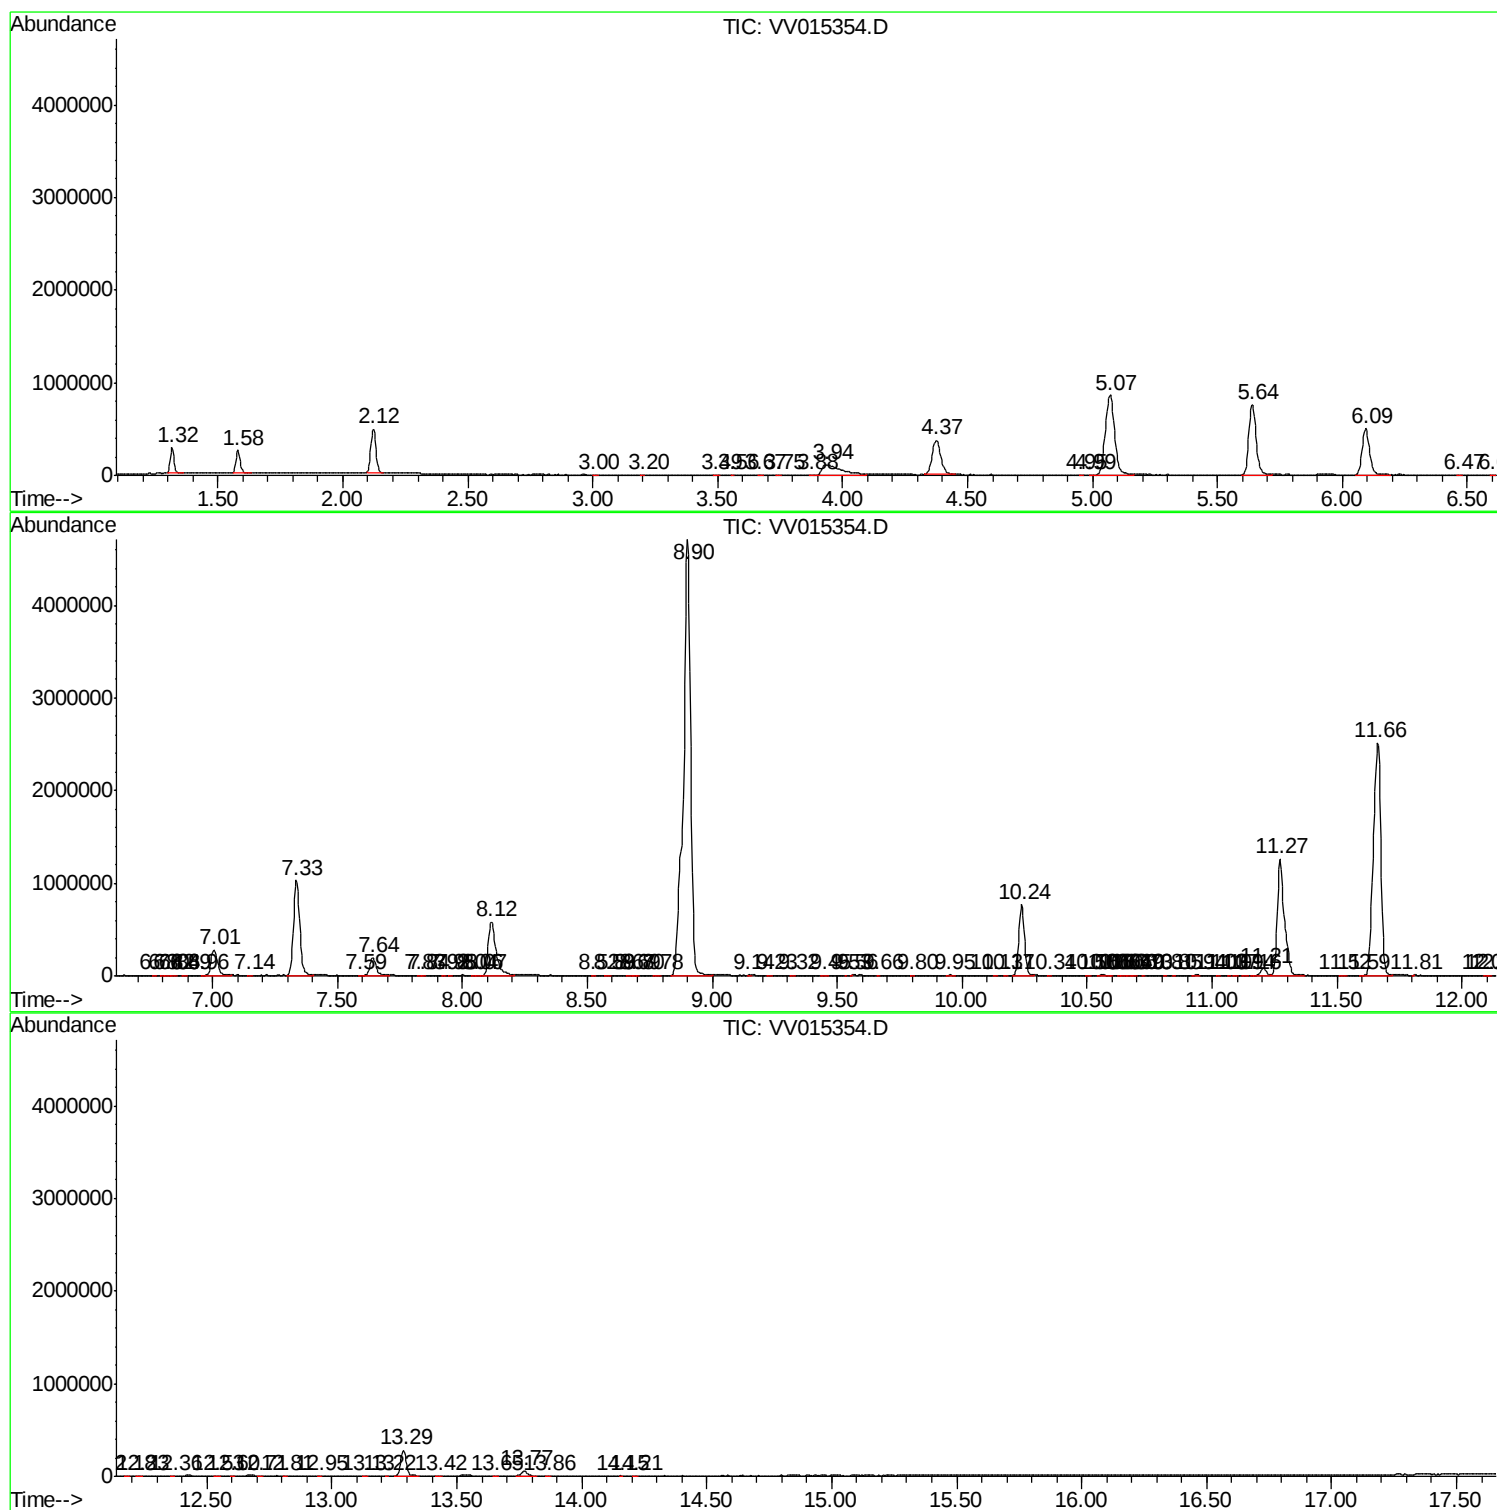

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV040120\
Data File : VV015353.D
Acq On : 02 Apr 2020 03:00
Operator : SY/MD
Sample : L2005-03 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DE4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV040120\
Data File : VV015353.D
Acq On : 02 Apr 2020 03:00
Operator : SY/MD
Sample : L2005-03 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DE4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc