

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015354.D
 Acq On : 02 Apr 2020 03:24
 Operator : SY/MD
 Sample : L2005-04 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

Signal : TIC: VV015355.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	267721	272077	3.09%	0.798%
2	1.579	146	152	167	rVB	245899	291047	3.31%	0.854%
3	2.119	313	320	335	rVB	519521	737286	8.37%	2.164%
4	3.235	666	667	669	rBV2	1315	703	0.01%	0.002%
5	3.405	717	720	721	rBV4	1740	943	0.01%	0.003%
6	3.502	747	750	751	rBV3	1488	808	0.01%	0.002%
7	3.618	784	786	790	rVB5	1157	508	0.01%	0.001%
8	3.663	794	800	802	rBV7	1303	1322	0.02%	0.004%
9	3.891	869	871	874	rBV3	871	641	0.01%	0.002%
10	3.942	874	887	939	rBV2	116414	609758	6.92%	1.789%
11	4.376	1008	1022	1045	rBV	363597	925045	10.51%	2.715%
12	4.679	1114	1116	1121	rBV5	2296	2460	0.03%	0.007%
13	4.743	1134	1136	1138	rBV3	1754	858	0.01%	0.003%
14	4.785	1145	1149	1150	rBV4	1505	950	0.01%	0.003%
15	4.846	1162	1168	1170	rBV7	3404	4081	0.05%	0.012%
16	4.900	1183	1185	1190	rVB4	2217	1393	0.02%	0.004%
17	4.929	1190	1194	1198	rBV7	1586	1562	0.02%	0.005%
18	4.974	1205	1208	1211	rBV4	1977	1366	0.02%	0.004%
19	5.003	1211	1217	1219	rBV6	1290	1003	0.01%	0.003%
20	5.074	1219	1239	1247	rBV2	886010	2181365	24.77%	6.401%
21	5.640	1403	1415	1442	rBV	785440	1575359	17.89%	4.623%
22	5.888	1490	1492	1495	rBV4	1525	1251	0.01%	0.004%
23	6.097	1544	1557	1583	rBV	497881	1021303	11.60%	2.997%
24	6.424	1657	1659	1661	rBV3	1727	965	0.01%	0.003%
25	6.489	1676	1679	1684	rBV6	1421	1390	0.02%	0.004%
26	6.563	1700	1702	1705	rBV3	2515	1535	0.02%	0.005%
27	6.579	1705	1707	1711	rVV4	1707	1405	0.02%	0.004%
28	6.611	1715	1717	1719	rBV3	1042	713	0.01%	0.002%
29	6.836	1785	1787	1789	rBV2	1650	847	0.01%	0.002%
30	6.907	1806	1809	1810	rBV3	1482	907	0.01%	0.003%
31	6.939	1817	1819	1821	rBV3	1585	805	0.01%	0.002%
32	7.006	1829	1840	1861	rBV	269966	485716	5.52%	1.425%
33	7.264	1917	1920	1921	rBV3	1722	1193	0.01%	0.004%
34	7.338	1930	1943	1974	rBV	1082983	1902988	21.61%	5.585%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015354.D
 Acq On : 02 Apr 2020 03:24
 Operator : SY/MD
 Sample : L2005-04 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

35	7.643	2028	2038	2053	rBV	189954	324044	3.68%	0.951%
36	7.891	2113	2115	2116	rBV2	1187	579	0.01%	0.002%
37	7.994	2139	2147	2148	rBV8	3036	2912	0.03%	0.009%
38	8.035	2158	2160	2162	rBV3	957	526	0.01%	0.002%
39	8.077	2170	2173	2174	rBV3	1659	868	0.01%	0.003%
40	8.116	2174	2185	2217	rBV2	612802	1289746	14.65%	3.785%
41	8.521	2308	2311	2312	rBV3	1668	608	0.01%	0.002%
42	8.531	2312	2314	2315	rBV2	1118	481	0.01%	0.001%
43	8.694	2363	2365	2366	rBV2	1475	534	0.01%	0.002%
44	8.752	2381	2383	2386	rBV3	2179	1486	0.02%	0.004%
45	8.788	2390	2394	2397	rBV5	2370	1716	0.02%	0.005%
46	8.804	2397	2399	2400	rBV2	1078	528	0.01%	0.002%
47	8.878	2409	2422	2423	rBV	1315632	1646921	18.70%	4.833%
48	9.129	2498	2500	2505	rBV5	1911	1650	0.02%	0.005%
49	9.164	2505	2511	2514	rBV6	3917	4716	0.05%	0.014%
50	9.344	2564	2567	2570	rBV6	1168	1064	0.01%	0.003%
51	9.473	2604	2607	2608	rBV3	1339	790	0.01%	0.002%
52	9.508	2614	2618	2623	rVB7	2576	2792	0.03%	0.008%
53	9.537	2623	2627	2628	rBV4	1371	863	0.01%	0.003%
54	9.550	2629	2631	2633	rBV3	1321	799	0.01%	0.002%
55	9.624	2652	2654	2655	rBV2	1103	461	0.01%	0.001%
56	9.646	2659	2661	2663	rBV3	1921	1160	0.01%	0.003%
57	9.791	2701	2706	2709	rBV6	1573	1293	0.01%	0.004%
58	9.849	2717	2724	2727	rBV8	2497	2889	0.03%	0.008%
59	9.903	2734	2741	2744	rVB7	2350	2029	0.02%	0.006%
60	9.929	2745	2749	2752	rBV5	2498	1815	0.02%	0.005%
61	9.955	2752	2757	2760	rBV7	2126	2291	0.03%	0.007%
62	10.000	2767	2771	2773	rBV5	939	710	0.01%	0.002%
63	10.058	2787	2789	2792	rVB3	912	450	0.01%	0.001%
64	10.154	2817	2819	2823	rVB4	1221	650	0.01%	0.002%
65	10.174	2823	2825	2826	rBV2	1353	482	0.01%	0.001%
66	10.238	2832	2845	2864	rBV	780871	1231815	13.99%	3.615%
67	10.357	2879	2882	2885	rBV4	2350	1423	0.02%	0.004%
68	10.402	2895	2896	2898	rBV2	1797	741	0.01%	0.002%
69	10.440	2904	2908	2916	rBV10	2943	4737	0.05%	0.014%
70	10.511	2926	2930	2931	rBV3	1213	949	0.01%	0.003%
71	10.563	2938	2946	2947	rBV8	2463	2486	0.03%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015354.D
 Acq On : 02 Apr 2020 03:24
 Operator : SY/MD
 Sample : L2005-04 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

72	10.598	2954	2957	2959	rBV3	1568	931	0.01%	0.003%
73	10.759	3005	3007	3011	rVB5	1467	895	0.01%	0.003%
74	11.006	3080	3084	3086	rBV5	1759	1300	0.01%	0.004%
75	11.064	3099	3102	3106	rBV5	2020	1553	0.02%	0.005%
76	11.122	3115	3120	3124	rVB5	1655	1425	0.02%	0.004%
77	11.151	3124	3129	3131	rBV5	1944	1471	0.02%	0.004%
78	11.202	3134	3145	3156	rBV	527724	815027	9.26%	2.392%
79	11.296	3157	3174	3199	rVB2	3068654	6514646	73.98%	19.118%
80	11.665	3270	3289	3310	rBV2	4767921	8805502	100.00%	25.841%
81	12.000	3391	3393	3395	rBV3	1333	700	0.01%	0.002%
82	12.083	3416	3419	3420	rBV2	2344	1292	0.01%	0.004%
83	12.209	3456	3458	3459	rBV2	1668	640	0.01%	0.002%
84	12.257	3469	3473	3475	rBV4	1011	668	0.01%	0.002%
85	12.347	3498	3501	3504	rBV5	1171	932	0.01%	0.003%
86	12.411	3517	3521	3522	rBV3	3161	2138	0.02%	0.006%
87	12.563	3563	3568	3572	rBV7	1970	1994	0.02%	0.006%
88	12.675	3595	3603	3609	rBV7	7587	10475	0.12%	0.031%
89	12.775	3627	3634	3636	rBV8	5023	5614	0.06%	0.016%
90	12.868	3659	3663	3664	rBV3	1993	1503	0.02%	0.004%
91	12.939	3684	3685	3688	rVB3	1643	501	0.01%	0.001%
92	12.955	3688	3690	3694	rBV4	1867	1427	0.02%	0.004%
93	13.116	3738	3740	3743	rBV3	2022	1249	0.01%	0.004%
94	13.235	3774	3777	3780	rBV5	1368	992	0.01%	0.003%
95	13.286	3780	3793	3816	rVV	1460076	2249220	25.54%	6.601%
96	13.505	3860	3861	3862	rBV	1271	425	0.00%	0.001%
97	13.595	3884	3889	3894	rBV8	2206	3131	0.04%	0.009%
98	13.768	3932	3943	3961	rBV	608978	945593	10.74%	2.775%
99	14.135	4054	4057	4060	rBV2	2168	1788	0.02%	0.005%
100	15.424	4449	4458	4469	rBV2	83367	131516	1.49%	0.386%


Sum of corrected areas: 34076105

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV040120\
Data File : VV015354.D
Acq On : 02 Apr 2020 03:24
Operator : SY/MD
Sample : L2005-04 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CODE6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

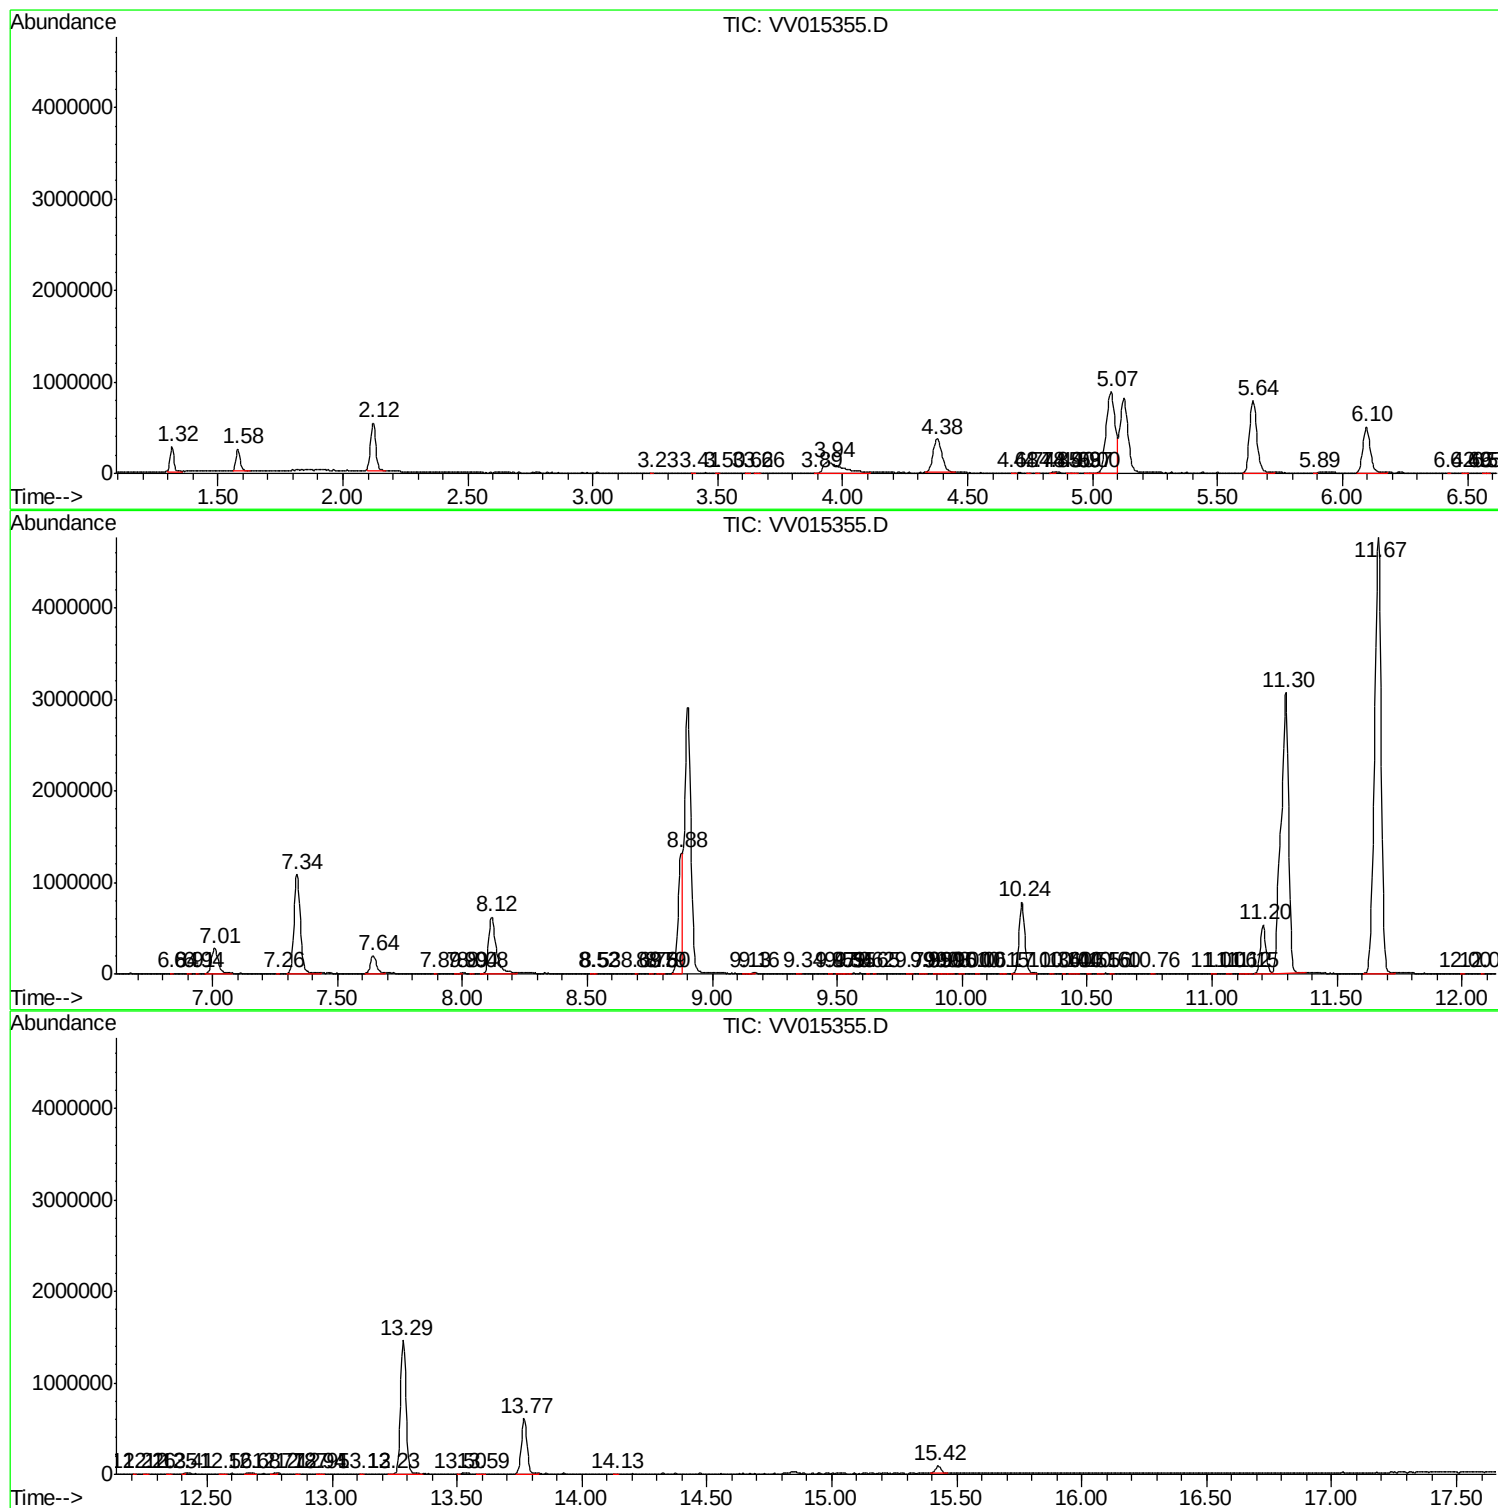

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV040120\
Data File : VV015354.D
Acq On : 02 Apr 2020 03:24
Operator : SY/MD
Sample : L2005-04 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DE6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV040120\
Data File : VV015354.D
Acq On : 02 Apr 2020 03:24
Operator : SY/MD
Sample : L2005-04 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DE6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc