

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015355.D
 Acq On : 02 Apr 2020 03:49
 Operator : SY/MD
 Sample : L2005-07 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

Signal : TIC: VV015356.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	80	rVB	260236	265124	3.27%	0.984%
2	1.576	145	151	165	rVB	241237	284285	3.51%	1.056%
3	2.116	312	319	344	rVB	543909	820626	10.12%	3.047%
4	3.100	623	625	627	rBV2	1270	726	0.01%	0.003%
5	3.171	644	647	651	rVB4	2236	1814	0.02%	0.007%
6	3.196	651	655	661	rBV9	2347	2750	0.03%	0.010%
7	3.306	686	689	691	rBV4	1463	810	0.01%	0.003%
8	3.383	711	713	714	rBV2	1292	407	0.01%	0.002%
9	3.537	759	761	763	rBV3	1385	766	0.01%	0.003%
10	3.627	787	789	791	rVB3	1597	787	0.01%	0.003%
11	3.727	818	820	826	rVB7	1515	1191	0.01%	0.004%
12	3.862	858	862	864	rBV4	1597	1561	0.02%	0.006%
13	3.939	871	886	921	rBV2	115210	512025	6.32%	1.901%
14	4.373	1008	1021	1048	rVB	356032	890543	10.99%	3.307%
15	4.740	1132	1135	1138	rBV5	1700	1243	0.02%	0.005%
16	4.926	1192	1193	1195	rBV2	1052	359	0.00%	0.001%
17	4.981	1208	1210	1214	rBV5	1860	1199	0.01%	0.004%
18	5.071	1221	1238	1247	rBV2	869232	2164684	26.70%	8.038%
19	5.469	1361	1362	1364	rBV2	1349	672	0.01%	0.002%
20	5.640	1401	1415	1439	rBV	791567	1576233	19.45%	5.853%
21	5.849	1478	1480	1484	rVB3	3161	1685	0.02%	0.006%
22	6.093	1544	1556	1583	rVB	481394	981939	12.11%	3.646%
23	6.354	1635	1637	1638	rBV2	1210	512	0.01%	0.002%
24	6.386	1644	1647	1649	rBV4	2159	1053	0.01%	0.004%
25	6.434	1660	1662	1663	rBV2	1450	575	0.01%	0.002%
26	6.524	1687	1690	1693	rBV4	2252	1491	0.02%	0.006%
27	6.556	1696	1700	1704	rVB6	2391	2466	0.03%	0.009%
28	6.582	1704	1708	1709	rBV3	2058	1334	0.02%	0.005%
29	6.621	1717	1720	1722	rBV4	2464	1444	0.02%	0.005%
30	6.926	1813	1815	1816	rBV2	1449	609	0.01%	0.002%
31	6.958	1821	1825	1829	rVV	34424	19426	0.24%	0.072%
32	7.006	1829	1840	1857	rBV2	267369	474897	5.86%	1.763%
33	7.338	1930	1943	1961	rBV	1062980	1848154	22.80%	6.862%
34	7.643	2028	2038	2056	rBV	183406	317409	3.92%	1.179%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015355.D
 Acq On : 02 Apr 2020 03:49
 Operator : SY/MD
 Sample : L2005-07 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DE9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

35	8.116	2174	2185	2222	rBV2	581329	1213669	14.97%	4.506%
36	8.563	2319	2324	2325	rBV4	2019	1475	0.02%	0.005%
37	8.675	2357	2359	2367	rVB9	2156	1785	0.02%	0.007%
38	8.707	2367	2369	2371	rBV2	1344	768	0.01%	0.003%
39	8.903	2407	2430	2452	rBV2	3848387	8106010	100.00%	30.099%
40	9.128	2498	2500	2503	rBV4	2298	1466	0.02%	0.005%
41	9.447	2596	2599	2601	rBV4	1343	843	0.01%	0.003%
42	9.463	2602	2604	2607	rVB4	1522	782	0.01%	0.003%
43	9.543	2626	2629	2631	rBV3	1058	674	0.01%	0.003%
44	10.054	2786	2788	2791	rVB3	923	486	0.01%	0.002%
45	10.090	2797	2799	2801	rBV3	1280	546	0.01%	0.002%
46	10.238	2833	2845	2863	rBV	745931	1175336	14.50%	4.364%
47	10.540	2936	2939	2940	rBV3	1466	614	0.01%	0.002%
48	10.672	2977	2980	2981	rBV3	1214	752	0.01%	0.003%
49	10.698	2985	2988	2991	rBV5	1857	1607	0.02%	0.006%
50	10.755	3001	3006	3008	rBV6	1828	1632	0.02%	0.006%
51	10.823	3023	3027	3031	rBV6	2367	1679	0.02%	0.006%
52	10.862	3037	3039	3041	rBV3	1447	720	0.01%	0.003%
53	10.923	3056	3058	3060	rBV4	1607	1049	0.01%	0.004%
54	11.058	3098	3100	3101	rBV2	1160	464	0.01%	0.002%
55	11.154	3128	3130	3134	rBV4	1229	972	0.01%	0.004%
56	11.206	3134	3146	3155	rBV2	85639	140255	1.73%	0.521%
57	11.276	3156	3168	3169	rBV	1384701	1730462	21.35%	6.425%
58	11.575	3257	3261	3262	rBV4	1164	840	0.01%	0.003%
59	11.662	3270	3288	3312	rBV2	1836213	4181655	51.59%	15.527%
60	11.971	3382	3384	3389	rVB5	1952	1414	0.02%	0.005%
61	11.993	3389	3391	3392	rBV2	768	273	0.00%	0.001%
62	12.022	3397	3400	3403	rBV4	1397	1280	0.02%	0.005%
63	12.067	3412	3414	3416	rBV2	1272	648	0.01%	0.002%
64	12.125	3430	3432	3433	rBV3	1076	437	0.01%	0.002%
65	12.315	3490	3491	3494	rBV3	1568	867	0.01%	0.003%
66	12.469	3536	3539	3541	rBV3	1552	1175	0.01%	0.004%
67	12.521	3551	3555	3559	rBV6	2723	3297	0.04%	0.012%
68	12.559	3565	3567	3570	rBV3	1240	795	0.01%	0.003%
69	12.714	3612	3615	3617	rBV3	3067	1951	0.02%	0.007%
70	12.839	3652	3654	3657	rBV3	1275	822	0.01%	0.003%
71	13.019	3708	3710	3715	rVB5	1348	646	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
Data File : VV015355.D
Acq On : 02 Apr 2020 03:49
Operator : SY/MD
Sample : L2005-07 500X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CODE9

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Title : VOC Analysis

72	13.064	3721	3724	3726	rBV3	1877	1117	0.01%	0.004%
73	13.103	3734	3736	3738	rBV3	1187	598	0.01%	0.002%
74	13.183	3759	3761	3762	rBV2	1134	598	0.01%	0.002%
75	13.238	3777	3778	3782	rBV4	877	706	0.01%	0.003%
76	13.289	3782	3794	3805	rBV2	72541	119974	1.48%	0.445%
77	13.405	3828	3830	3835	rVB3	1669	1212	0.01%	0.005%
78	13.469	3847	3850	3852	rBV3	1946	945	0.01%	0.004%
79	13.620	3891	3897	3901	rBV9	2413	2836	0.03%	0.011%
80	13.771	3937	3944	3956	rVB2	23862	40740	0.50%	0.151%
81	14.762	4249	4252	4255	rBV4	2626	1887	0.02%	0.007%


Sum of corrected areas: 26931558

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV040120\
Data File : VV015355.D
Acq On : 02 Apr 2020 03:49
Operator : SY/MD
Sample : L2005-07 500X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CODE9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

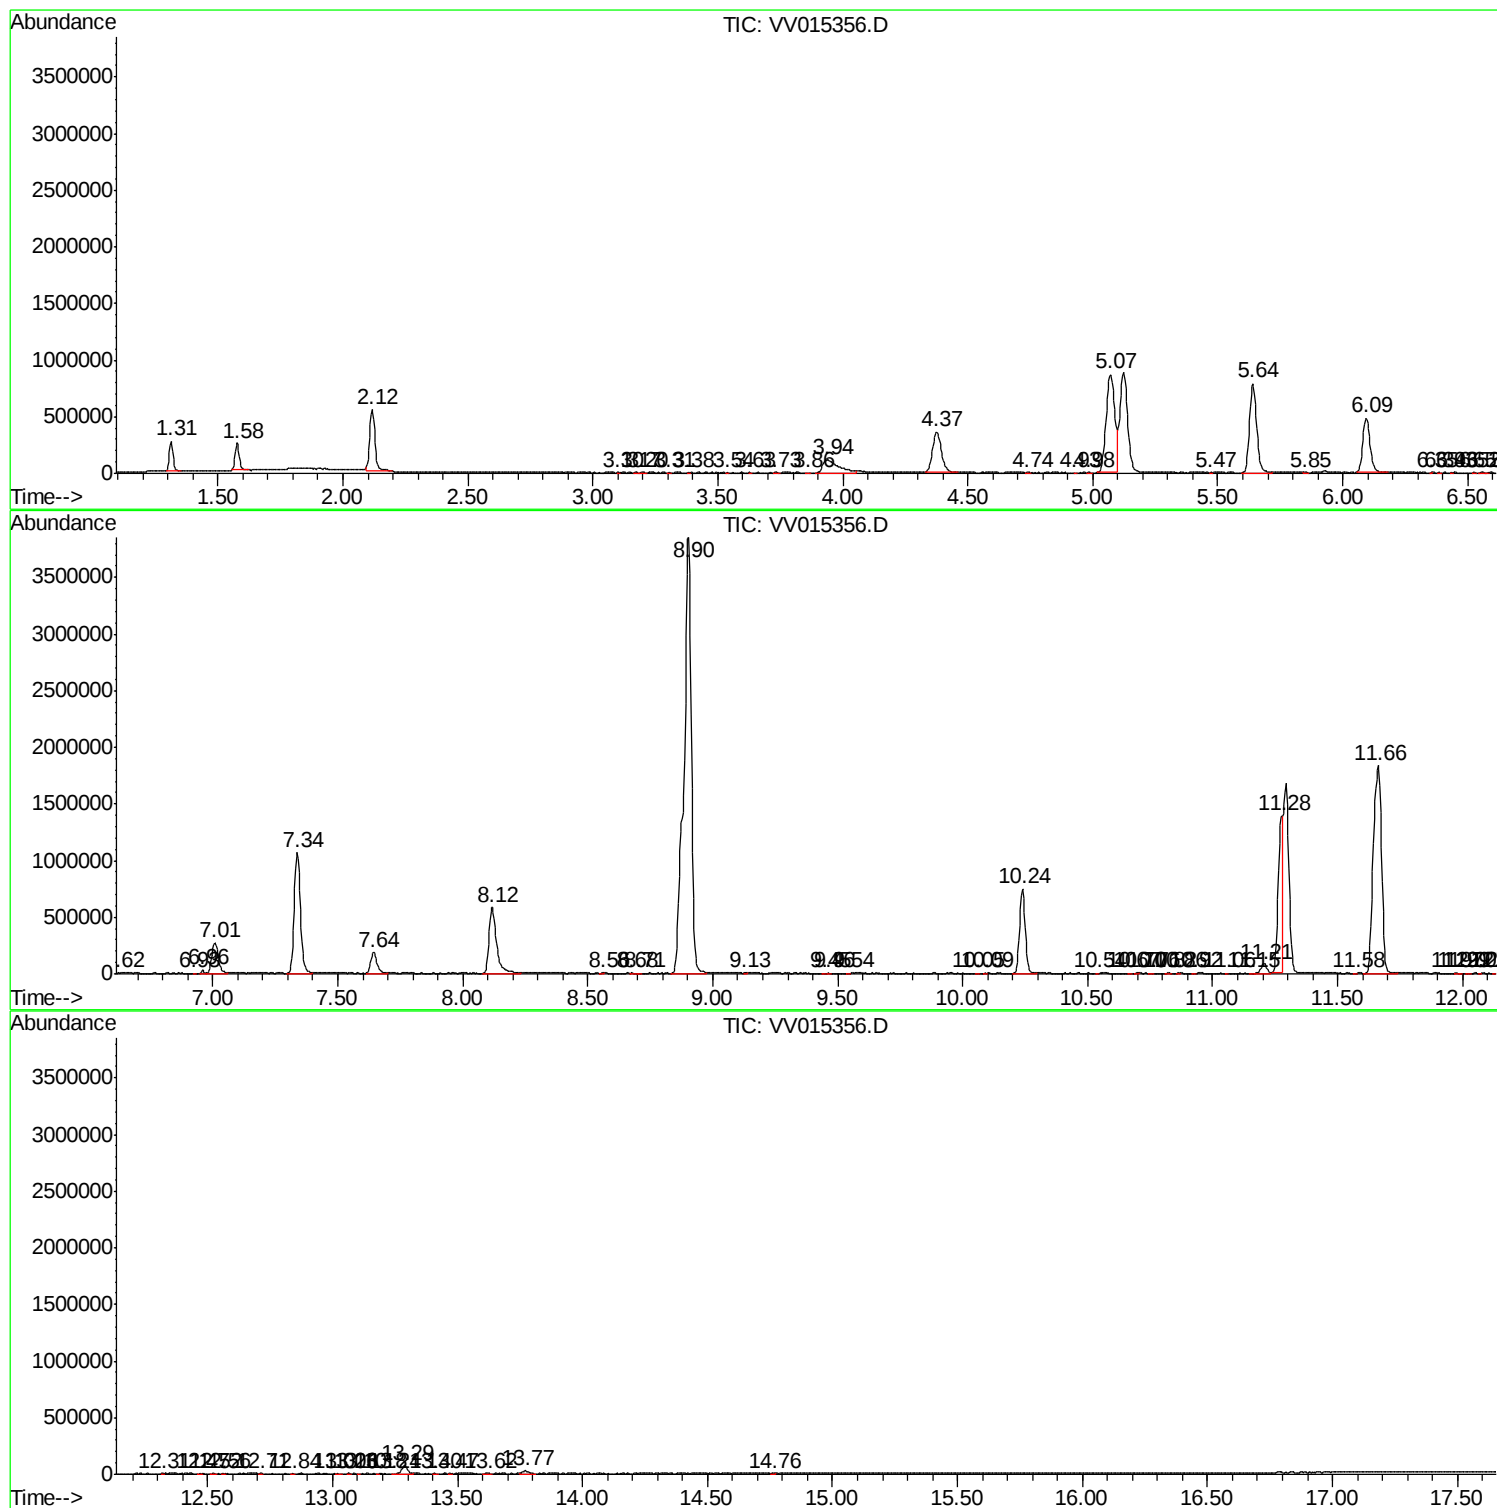

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV040120\
Data File : VV015355.D
Acq On : 02 Apr 2020 03:49
Operator : SY/MD
Sample : L2005-07 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DE9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV040120\
Data File : VV015355.D
Acq On : 02 Apr 2020 03:49
Operator : SY/MD
Sample : L2005-07 500X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DE9

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc