

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015359.D
 Acq On : 02 Apr 2020 05:25
 Operator : SY/MD
 Sample : L2064-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

Signal : TIC: VV015360.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	382175	378051	15.02%	1.748%
2	1.579	145	152	164	rVB	313344	371208	14.75%	1.717%
3	1.762	204	209	220	rVB	196606	250945	9.97%	1.161%
4	2.119	312	320	345	rVB	682892	1029110	40.89%	4.759%
5	3.055	607	611	615	rBV6	2661	2362	0.09%	0.011%
6	3.566	767	770	775	rBV5	2160	1960	0.08%	0.009%
7	3.769	830	833	834	rBV3	1182	642	0.03%	0.003%
8	3.807	842	845	851	rVB8	2203	2008	0.08%	0.009%
9	3.836	851	854	855	rBV3	1157	546	0.02%	0.003%
10	3.868	862	864	866	rBV3	1403	627	0.02%	0.003%
11	3.888	866	870	872	rBV4	1769	1324	0.05%	0.006%
12	3.942	875	887	915	rBV2	115662	468910	18.63%	2.169%
13	4.376	1007	1022	1049	rBV	410212	1018055	40.45%	4.708%
14	4.704	1122	1124	1127	rVB4	1716	863	0.03%	0.004%
15	4.727	1127	1131	1132	rBV4	1381	882	0.04%	0.004%
16	4.765	1141	1143	1145	rBV3	1280	687	0.03%	0.003%
17	4.952	1199	1201	1205	rBV3	1946	1903	0.08%	0.009%
18	5.071	1219	1238	1262	rBV2	1000834	2516533	100.00%	11.638%
19	5.322	1314	1316	1319	rVB4	2304	995	0.04%	0.005%
20	5.553	1383	1388	1393	rBV9	2169	2611	0.10%	0.012%
21	5.640	1402	1415	1439	rBV	751825	1520322	60.41%	7.031%
22	6.096	1542	1557	1583	rBV	560368	1140631	45.33%	5.275%
23	6.293	1616	1618	1625	rVB8	3040	2868	0.11%	0.013%
24	6.502	1680	1683	1685	rBV4	1434	938	0.04%	0.004%
25	6.547	1693	1697	1700	rBV6	995	1005	0.04%	0.005%
26	6.762	1760	1764	1765	rBV3	1199	860	0.03%	0.004%
27	6.778	1767	1769	1771	rBV3	1625	868	0.03%	0.004%
28	6.884	1800	1802	1807	rVB4	1596	1310	0.05%	0.006%
29	6.923	1810	1814	1818	rBV6	1486	1059	0.04%	0.005%
30	7.010	1828	1841	1858	rBV	332598	598516	23.78%	2.768%
31	7.338	1930	1943	1968	rBV	1222972	2143039	85.16%	9.911%
32	7.643	2028	2038	2058	rBV	234378	401831	15.97%	1.858%
33	7.997	2128	2148	2166	rBV	901459	1526630	60.66%	7.060%
34	8.119	2175	2186	2213	rBV2	610394	1290711	51.29%	5.969%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015359.D
 Acq On : 02 Apr 2020 05:25
 Operator : SY/MD
 Sample : L2064-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

35	8.685	2360	2362	2363	rBV2	1152	542	0.02%	0.003%
36	8.791	2393	2395	2399	rBV4	1608	1454	0.06%	0.007%
37	8.874	2407	2421	2444	rBV	1176120	1883626	74.85%	8.711%
38	9.109	2492	2494	2497	rBV4	1483	945	0.04%	0.004%
39	9.135	2497	2502	2504	rVV5	1564	1221	0.05%	0.006%
40	9.206	2523	2524	2528	rBV4	1369	913	0.04%	0.004%
41	9.251	2533	2538	2540	rBV5	2141	1777	0.07%	0.008%
42	9.318	2556	2559	2561	rBV3	1078	919	0.04%	0.004%
43	9.350	2566	2569	2571	rBV3	1663	1231	0.05%	0.006%
44	9.444	2597	2598	2601	rBV3	1365	776	0.03%	0.004%
45	9.463	2601	2604	2607	rBV5	1824	1473	0.06%	0.007%
46	9.518	2616	2621	2624	rBV7	1924	1759	0.07%	0.008%
47	9.540	2626	2628	2632	rBV4	1734	1141	0.05%	0.005%
48	9.559	2632	2634	2636	rBV2	1469	695	0.03%	0.003%
49	9.656	2663	2664	2666	rBV2	975	540	0.02%	0.002%
50	9.688	2672	2674	2676	rVB3	984	263	0.01%	0.001%
51	9.772	2694	2700	2706	rBV10	2210	2724	0.11%	0.013%
52	9.797	2706	2708	2711	rVB3	1378	718	0.03%	0.003%
53	9.826	2713	2717	2720	rBV5	1746	1567	0.06%	0.007%
54	9.907	2739	2742	2745	rVB4	1715	1032	0.04%	0.005%
55	9.919	2745	2746	2748	rBV2	733	216	0.01%	0.001%
56	9.974	2761	2763	2766	rVB2	1819	931	0.04%	0.004%
57	10.016	2773	2776	2779	rBV4	2131	1469	0.06%	0.007%
58	10.128	2809	2811	2814	rBV4	1161	713	0.03%	0.003%
59	10.238	2834	2845	2863	rBV	815304	1273212	50.59%	5.888%
60	10.492	2922	2924	2927	rBV3	979	536	0.02%	0.002%
61	10.553	2940	2943	2944	rBV3	2116	1182	0.05%	0.005%
62	10.662	2973	2977	2979	rBV4	1299	1082	0.04%	0.005%
63	10.739	2998	3001	3004	rBV4	1517	1359	0.05%	0.006%
64	10.768	3008	3010	3014	rVB4	1671	1059	0.04%	0.005%
65	10.791	3014	3017	3019	rBV4	1791	991	0.04%	0.005%
66	10.820	3024	3026	3028	rVB3	1564	601	0.02%	0.003%
67	10.833	3028	3030	3031	rBV2	1086	473	0.02%	0.002%
68	10.842	3031	3033	3035	rVB2	2015	940	0.04%	0.004%
69	10.926	3055	3059	3060	rBV3	1639	959	0.04%	0.004%
70	10.974	3072	3074	3075	rBV3	720	239	0.01%	0.001%
71	11.003	3081	3083	3084	rBV2	1113	351	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015359.D
 Acq On : 02 Apr 2020 05:25
 Operator : SY/MD
 Sample : L2064-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

72	11.042	3093	3095	3098	rBV3	822	477	0.02%	0.002%
73	11.061	3098	3101	3103	rBV4	1184	765	0.03%	0.004%
74	11.141	3123	3126	3128	rBV4	1687	785	0.03%	0.004%
75	11.161	3128	3132	3134	rBV6	1371	1147	0.05%	0.005%
76	11.209	3143	3147	3149	rBV4	2139	1849	0.07%	0.009%
77	11.270	3154	3166	3192	rBV	1146931	1789459	71.11%	8.276%
78	11.514	3241	3242	3244	rBV2	1145	491	0.02%	0.002%
79	11.646	3271	3283	3302	rBV	1229873	1938186	77.02%	8.964%
80	11.816	3332	3336	3339	rBV5	2774	2661	0.11%	0.012%
81	12.064	3411	3413	3414	rBV2	792	246	0.01%	0.001%
82	12.376	3507	3510	3512	rBV3	1665	858	0.03%	0.004%
83	12.508	3549	3551	3552	rBV2	1506	557	0.02%	0.003%
84	12.533	3557	3559	3562	rVV4	881	455	0.02%	0.002%
85	12.643	3591	3593	3594	rBV2	1394	550	0.02%	0.003%
86	12.823	3647	3649	3650	rBV2	1128	494	0.02%	0.002%
87	12.935	3680	3684	3687	rBV6	1371	1070	0.04%	0.005%
88	13.022	3707	3711	3713	rBV5	1269	924	0.04%	0.004%
89	13.231	3773	3776	3780	rVB5	1450	1097	0.04%	0.005%
90	13.260	3783	3785	3787	rBV3	1293	727	0.03%	0.003%
91	13.411	3830	3832	3834	rBV3	1778	667	0.03%	0.003%
92	13.469	3848	3850	3853	rVB3	2226	1211	0.05%	0.006%
93	13.485	3853	3855	3860	rBV4	1176	898	0.04%	0.004%
94	13.524	3865	3867	3869	rBV2	1468	808	0.03%	0.004%
95	13.585	3883	3886	3888	rBV4	1617	1059	0.04%	0.005%
96	13.614	3893	3895	3897	rBV3	1331	871	0.03%	0.004%
97	14.035	4024	4026	4027	rBV	1396	629	0.02%	0.003%
98	14.453	4154	4156	4159	rBV5	1896	1188	0.05%	0.005%


Sum of corrected areas: 21622568

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV040120\
Data File : VV015359.D
Acq On : 02 Apr 2020 05:25
Operator : SY/MD
Sample : L2064-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0Y03

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

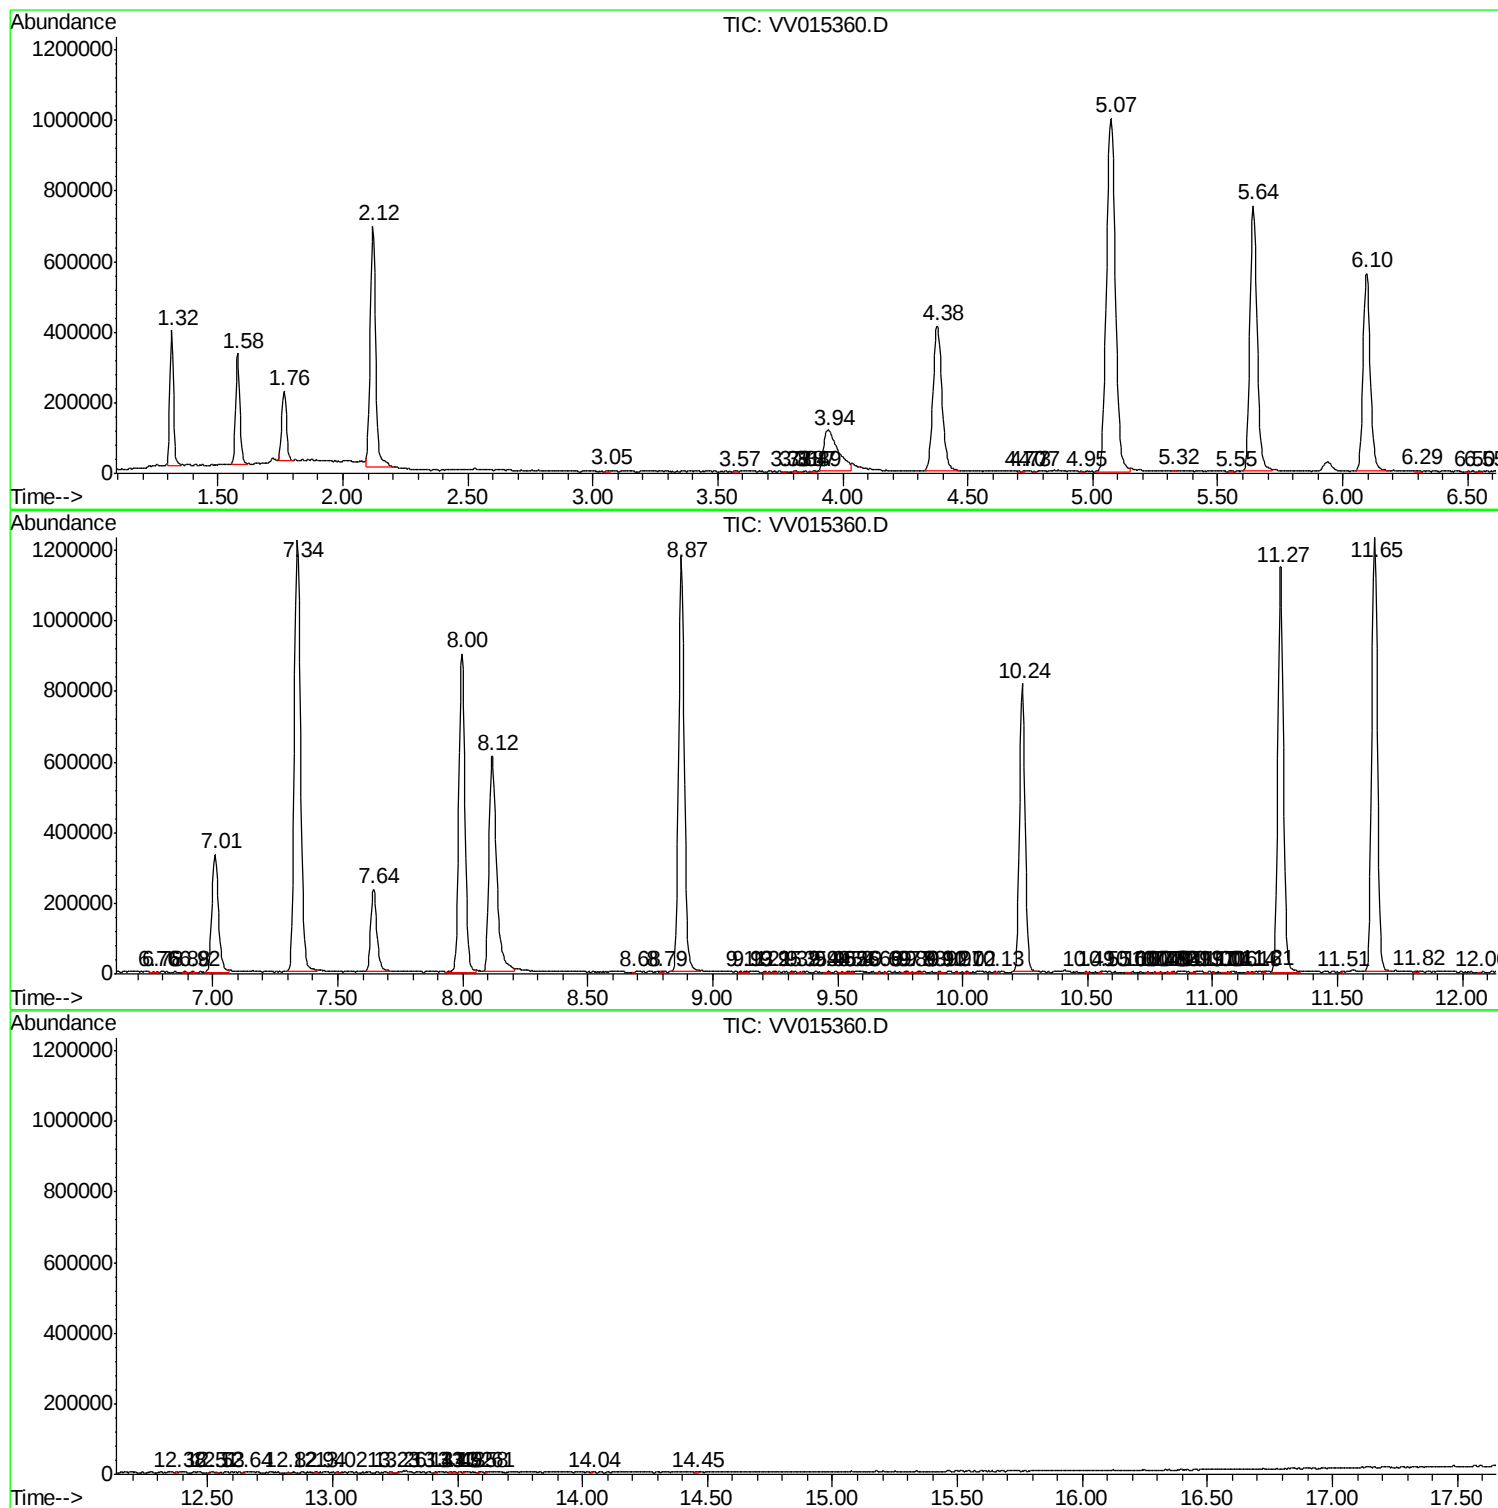

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV040120\
Data File : VV015359.D
Acq On : 02 Apr 2020 05:25
Operator : SY/MD
Sample : L2064-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0Y03

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV040120\
Data File : VV015359.D
Acq On : 02 Apr 2020 05:25
Operator : SY/MD
Sample : L2064-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0Y03

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc