

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015361.D
 Acq On : 02 Apr 2020 06:14
 Operator : SY/MD
 Sample : L2064-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

Signal : TIC: VV015362.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	84	rVB	388948	385909	15.09%	1.732%
2	1.579	146	152	167	rVB	313925	374117	14.63%	1.679%
3	1.766	204	210	219	rVB	195720	247292	9.67%	1.110%
4	2.119	312	320	342	rVB	695476	1044683	40.84%	4.688%
5	3.049	606	609	612	rBV4	1997	1226	0.05%	0.006%
6	3.203	652	657	661	rBV6	2672	2452	0.10%	0.011%
7	3.386	709	714	715	rBV4	1291	1153	0.05%	0.005%
8	3.425	722	726	728	rBV5	1404	853	0.03%	0.004%
9	3.463	736	738	739	rBV2	1284	407	0.02%	0.002%
10	3.566	768	770	774	rVB4	1736	1086	0.04%	0.005%
11	3.589	774	777	778	rBV3	1720	1015	0.04%	0.005%
12	3.682	804	806	810	rBV5	2043	1858	0.07%	0.008%
13	3.727	817	820	825	rVB6	1923	1878	0.07%	0.008%
14	3.769	828	833	839	rBV9	2463	3447	0.13%	0.015%
15	3.862	860	862	868	rBV6	1810	1694	0.07%	0.008%
16	3.939	874	886	924	rBV2	121334	526297	20.57%	2.362%
17	4.376	1003	1022	1045	rBV	416374	1047888	40.96%	4.702%
18	4.553	1073	1077	1080	rBV5	1626	1776	0.07%	0.008%
19	5.074	1222	1239	1266	rBV2	1020867	2558033	100.00%	11.479%
20	5.428	1346	1349	1355	rBV7	2778	3208	0.13%	0.014%
21	5.640	1403	1415	1442	rBV	782608	1579117	61.73%	7.086%
22	5.942	1498	1509	1528	rVB5	36840	84717	3.31%	0.380%
23	6.093	1540	1556	1578	rBV	560238	1147781	44.87%	5.151%
24	6.482	1672	1677	1679	rBV4	1643	1211	0.05%	0.005%
25	6.492	1679	1680	1683	rBV3	1495	805	0.03%	0.004%
26	6.608	1711	1716	1722	rBV10	2793	3997	0.16%	0.018%
27	6.720	1748	1751	1752	rBV3	1168	717	0.03%	0.003%
28	6.810	1775	1779	1783	rBV4	1783	1851	0.07%	0.008%
29	6.865	1792	1796	1800	rBV5	1938	1887	0.07%	0.008%
30	7.007	1829	1840	1864	rBV	333547	603563	23.59%	2.709%
31	7.338	1931	1943	1976	rBV	1302939	2251594	88.02%	10.104%
32	7.643	2028	2038	2058	rBV	234022	395415	15.46%	1.774%
33	7.810	2087	2090	2094	rBV6	1990	1685	0.07%	0.008%
34	7.997	2136	2148	2166	rVB	896605	1492569	58.35%	6.698%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015361.D
 Acq On : 02 Apr 2020 06:14
 Operator : SY/MD
 Sample : L2064-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

35	8.116	2175	2185	2219	rBV2	627021	1295886	50.66%	5.815%
36	8.511	2306	2308	2309	rBV2	1507	733	0.03%	0.003%
37	8.714	2369	2371	2372	rBV2	1375	508	0.02%	0.002%
38	8.804	2396	2399	2403	rBV6	1939	1624	0.06%	0.007%
39	8.875	2409	2421	2445	rBV	1198481	1955461	76.44%	8.775%
40	9.228	2529	2531	2536	rBV5	1874	1394	0.05%	0.006%
41	9.289	2547	2550	2552	rVB3	2047	1098	0.04%	0.005%
42	9.444	2594	2598	2601	rVB6	1699	1197	0.05%	0.005%
43	9.457	2601	2602	2603	rBV	701	225	0.01%	0.001%
44	9.514	2618	2620	2623	rBV3	901	685	0.03%	0.003%
45	9.672	2665	2669	2671	rVB5	1493	1025	0.04%	0.005%
46	9.801	2707	2709	2710	rBV2	841	251	0.01%	0.001%
47	9.949	2751	2755	2756	rBV4	1607	945	0.04%	0.004%
48	10.064	2789	2791	2799	rVB7	2536	1988	0.08%	0.009%
49	10.135	2812	2813	2816	rBV3	1211	712	0.03%	0.003%
50	10.164	2820	2822	2826	rBV4	1553	987	0.04%	0.004%
51	10.238	2832	2845	2863	rBV	829431	1294574	50.61%	5.810%
52	10.383	2888	2890	2891	rBV2	1927	824	0.03%	0.004%
53	10.572	2945	2949	2952	rBV5	2219	2229	0.09%	0.010%
54	10.646	2970	2972	2975	rBV3	2017	1260	0.05%	0.006%
55	10.794	3016	3018	3019	rBV2	1100	500	0.02%	0.002%
56	10.836	3029	3031	3033	rBV4	1170	611	0.02%	0.003%
57	10.871	3038	3042	3043	rBV4	2174	1589	0.06%	0.007%
58	10.929	3058	3060	3062	rBV2	1320	702	0.03%	0.003%
59	10.977	3073	3075	3079	rBV4	1754	1104	0.04%	0.005%
60	10.997	3079	3081	3082	rBV2	1475	474	0.02%	0.002%
61	11.090	3108	3110	3114	rBV4	1635	1069	0.04%	0.005%
62	11.190	3137	3141	3143	rBV3	1979	1379	0.05%	0.006%
63	11.270	3155	3166	3187	rBV	1229939	1898690	74.22%	8.521%
64	11.646	3271	3283	3302	rBV	1283846	2016373	78.83%	9.049%
65	11.804	3329	3332	3334	rBV4	2470	1673	0.07%	0.008%
66	11.945	3374	3376	3378	rBV3	1349	571	0.02%	0.003%
67	12.106	3423	3426	3429	rBV4	1010	783	0.03%	0.004%
68	12.148	3436	3439	3441	rVB4	2266	1245	0.05%	0.006%
69	12.170	3441	3446	3447	rBV5	1582	1400	0.05%	0.006%
70	12.321	3490	3493	3494	rBV3	1325	789	0.03%	0.004%
71	12.402	3515	3518	3520	rBV4	1770	909	0.04%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015361.D
 Acq On : 02 Apr 2020 06:14
 Operator : SY/MD
 Sample : L2064-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

72	12.424	3523	3525	3531	rVB7	1474	885	0.03%	0.004%
73	12.547	3560	3563	3566	rBV4	1511	1080	0.04%	0.005%
74	12.778	3634	3635	3637	rBV2	601	245	0.01%	0.001%
75	12.794	3637	3640	3643	rBV4	2073	1650	0.06%	0.007%
76	13.141	3745	3748	3750	rBV4	1755	1025	0.04%	0.005%
77	13.225	3772	3774	3775	rBV2	1489	577	0.02%	0.003%
78	13.286	3789	3793	3794	rBV4	3474	2568	0.10%	0.012%
79	13.350	3811	3813	3816	rBV4	1483	985	0.04%	0.004%
80	13.392	3823	3826	3827	rBV3	2042	902	0.04%	0.004%
81	13.453	3841	3845	3847	rVB4	2490	1451	0.06%	0.007%
82	13.479	3850	3853	3854	rBV3	1514	905	0.04%	0.004%
83	13.701	3919	3922	3924	rBV4	1585	1140	0.04%	0.005%
84	13.749	3935	3937	3939	rBV2	1100	486	0.02%	0.002%
85	13.772	3941	3944	3945	rBV2	2384	1396	0.05%	0.006%
86	14.173	4067	4069	4073	rBV5	1618	1056	0.04%	0.005%
87	14.263	4095	4097	4099	rBV2	1472	658	0.03%	0.003%


Sum of corrected areas: 22283657

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV040120\
Data File : VV015361.D
Acq On : 02 Apr 2020 06:14
Operator : SY/MD
Sample : L2064-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0Y05

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

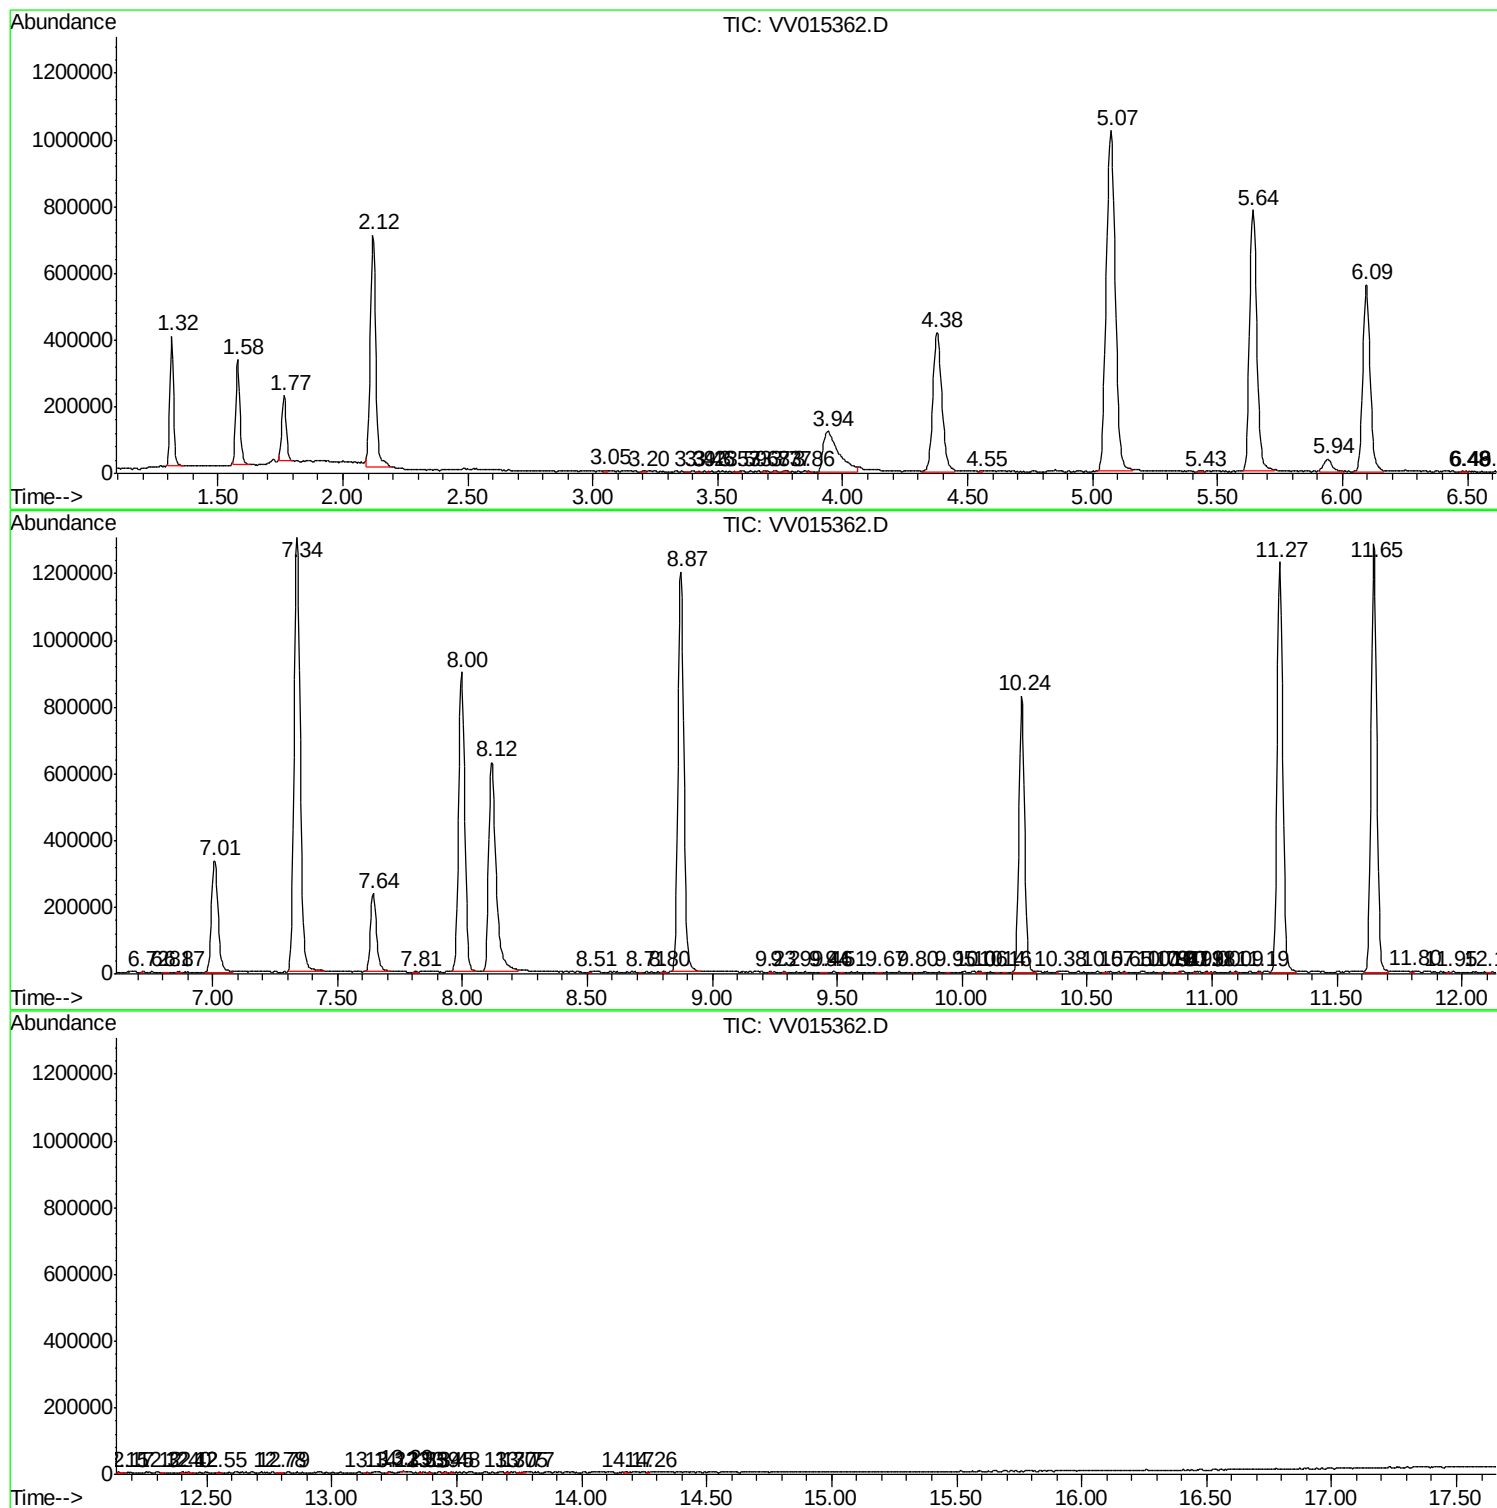

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV040120\
Data File : VV015361.D
Acq On : 02 Apr 2020 06:14
Operator : SY/MD
Sample : L2064-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0Y05

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV040120\
Data File : VV015361.D
Acq On : 02 Apr 2020 06:14
Operator : SY/MD
Sample : L2064-09
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0Y05

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc