


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040120\
 Data File : VV015325.D
 Acq On : 01 Apr 2020 08:39
 Operator : SY/MD
 Sample : BFB76
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB76

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis
 Last Update : Mon Feb 24 10:07:06 2020

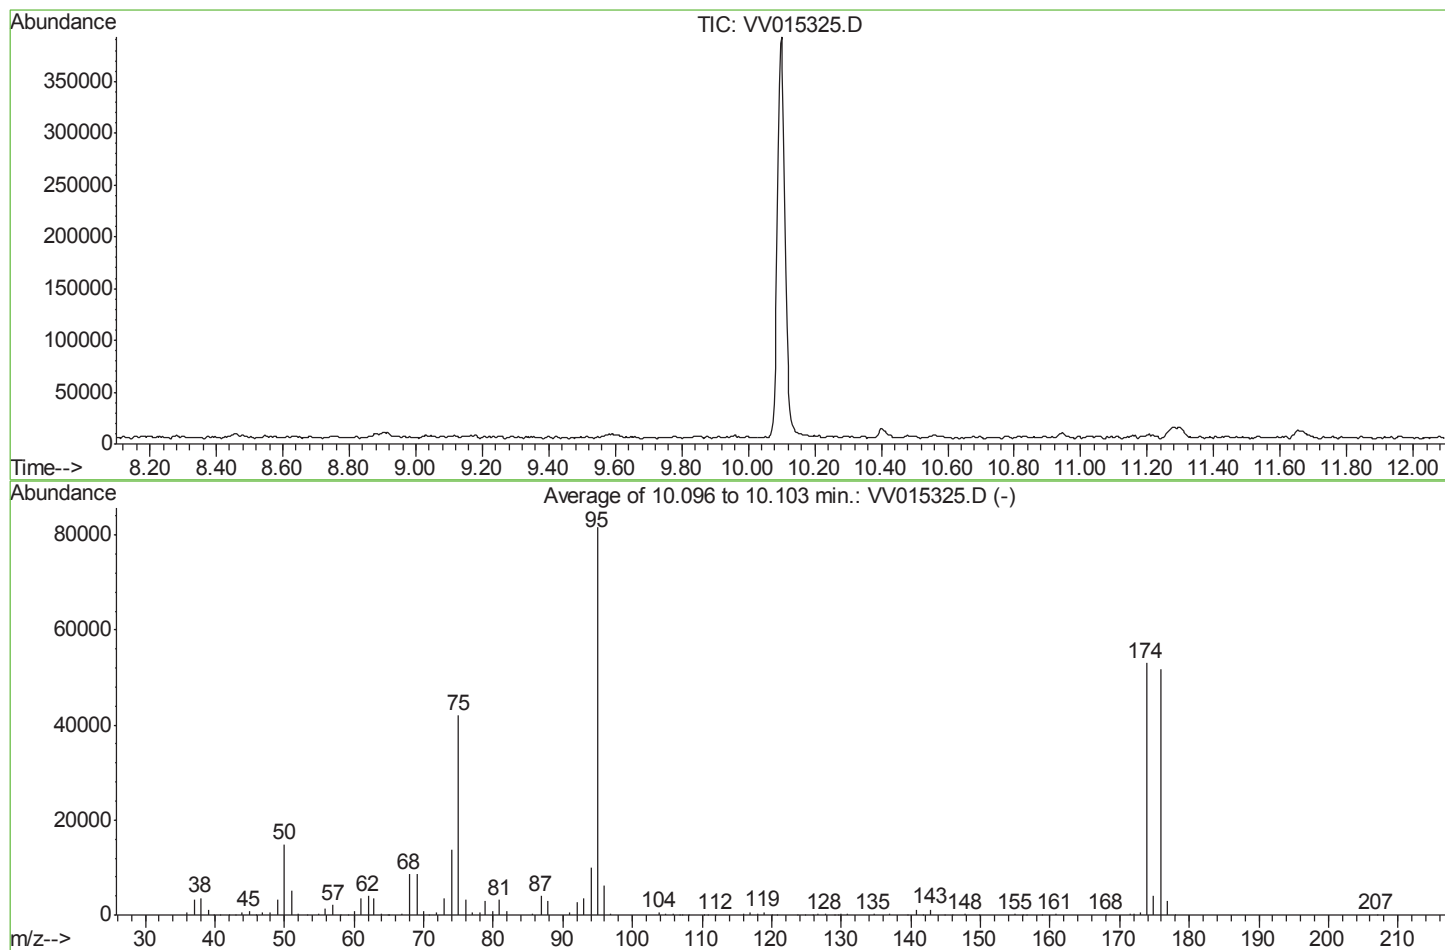

AutoFind: Scans 2801, 2802, 2803; Background Corrected with Scan 2787

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	14788	PASS
75	95	30	80	51.5	42010	PASS
95	95	100	100	100.0	81637	PASS
96	95	5	9	7.6	6199	PASS
173	174	0.00	2	1.3	673	PASS
174	95	50	120	65.0	53096	PASS
175	174	5	9	7.9	4181	PASS
176	174	95	105	97.4	51704	PASS
177	176	5	10	5.5	2867	PASS

m/z	Abundance
35.00	121.0
36.00	191.0
37.10	146.0
37.90	137.0
39.10	241.0
39.90	680.0
41.00	226.0
42.00	156.0
43.00	236.0
44.00	1012.0
45.00	160.0
45.20	157.0
46.20	123.0
46.90	108.0
48.90	121.0
52.30	117.0
52.70	141.0
54.00	157.0
54.90	122.0
55.90	147.0
56.90	162.0
58.10	147.0
58.60	143.0
60.00	137.0
60.80	175.0
66.00	126.0
67.20	106.0
67.80	156.0
69.20	151.0
69.80	161.0
73.00	121.0
76.10	105.0
77.70	145.0
91.20	143.0
94.10	126.0
97.20	185.0
98.40	115.0
102.90	122.0
105.80	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
35.90	821.0
37.00	3178.0
38.00	3879.0
39.00	1480.0
39.90	774.0
40.80	155.0
40.90	152.0
42.00	260.0
43.10	354.0
43.90	1560.0
44.90	854.0
47.00	843.0
48.00	689.0
49.00	3444.0
50.00	15328.0
51.00	5193.0
51.90	289.0
53.30	168.0
54.90	605.0
56.00	1650.0
57.00	2368.0
58.10	253.0
59.20	119.0
60.00	962.0
61.00	3901.0
62.00	4094.0
62.90	3614.0
63.90	308.0
64.80	128.0
67.00	207.0
68.00	8863.0
69.00	9087.0
70.00	867.0
71.90	634.0
73.00	3865.0
74.00	14204.0
75.00	42624.0
76.00	3651.0
77.00	439.0
78.00	346.0
78.90	3151.0
79.90	1005.0
80.90	3110.0
82.00	663.0
85.60	167.0
86.90	4143.0
87.90	2962.0
91.00	546.0
92.00	2882.0
93.00	3449.0
94.00	10472.0
95.00	83288.0
96.00	6611.0
96.90	294.0
103.80	479.0
104.70	358.0
105.90	483.0
106.70	143.0
107.10	126.0
110.20	163.0
111.90	147.0
115.90	363.0
116.90	526.0
117.90	274.0
118.90	565.0
120.00	108.0
120.70	103.0
123.80	118.0
124.70	110.0
125.90	125.0
126.70	153.0
127.70	216.0
129.00	132.0
129.60	329.0
130.80	169.0
134.70	254.0
136.90	220.0
139.60	115.0
140.80	1179.0
141.80	181.0
142.80	1269.0
145.90	139.0
147.80	230.0
155.10	234.0
156.10	136.0
156.70	113.0
158.90	106.0
160.80	120.0
168.10	122.0
172.00	400.0
172.90	683.0
173.90	52528.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

174.90	4159.0
175.90	51440.0
176.90	2962.0
177.90	105.0
206.90	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
35.90	798.0
37.00	3382.0
38.00	3919.0
39.00	1493.0
39.90	776.0
40.90	160.0
42.00	207.0
43.10	354.0
43.90	1698.0
44.90	923.0
45.90	114.0
47.00	750.0
48.00	696.0
49.00	3658.0
50.00	15227.0
51.00	5306.0
51.90	276.0
53.30	111.0
54.90	475.0
56.00	1620.0
57.00	2246.0
58.10	266.0
59.20	128.0
60.00	1136.0
61.00	3885.0
62.00	4113.0
62.90	3603.0
63.90	319.0
65.00	183.0
67.00	155.0
68.00	9071.0
69.00	8900.0
70.00	957.0
70.80	131.0
71.90	598.0
73.00	3777.0
74.00	14163.0
75.00	43112.0
76.00	3472.0
77.00	410.0
78.10	411.0
78.90	3149.0
79.80	940.0
80.90	3235.0
81.90	760.0
85.70	192.0
86.90	4285.0
87.90	3095.0
90.90	528.0
92.00	2718.0
93.00	3718.0
94.00	10320.0
95.00	83824.0
96.00	6380.0
96.90	245.0
103.80	425.0
104.70	262.0
105.90	487.0
107.10	144.0
108.00	135.0
110.20	115.0
110.80	175.0
112.00	140.0
115.90	347.0
116.80	425.0
117.90	324.0
118.80	664.0
120.10	118.0
120.70	109.0
123.70	123.0
124.70	134.0
125.90	104.0
126.70	167.0
127.70	220.0
129.00	125.0
130.00	343.0
130.90	170.0
134.70	287.0
136.90	220.0
139.60	134.0
140.80	1075.0
141.80	149.0
142.80	1105.0
145.90	122.0
147.80	250.0
149.80	125.0
155.10	281.0
160.90	165.0
168.10	113.0
171.60	330.0
172.00	313.0
173.00	683.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

173.90	55040.0
174.90	4365.0
175.90	53384.0
176.90	2919.0
177.90	140.0
207.00	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76

m/z	Abundance
35.90	740.0
37.00	3380.0
38.00	3484.0
39.00	1323.0
39.90	721.0
40.90	162.0
42.00	166.0
43.00	244.0
43.90	1657.0
44.90	908.0
45.90	128.0
46.90	624.0
47.90	566.0
49.00	3335.0
50.00	13811.0
51.00	4641.0
51.90	285.0
54.90	371.0
55.90	1458.0
57.00	2013.0
58.10	198.0
59.20	128.0
60.00	1017.0
61.00	3454.0
62.00	3678.0
62.90	3269.0
63.90	295.0
64.90	217.0
66.90	177.0
68.00	8274.0
69.00	8042.0
70.00	889.0
70.70	139.0
71.90	475.0
72.90	3287.0
74.00	12865.0
75.00	40296.0
76.00	2958.0
76.90	449.0
78.10	506.0
78.90	2936.0
79.80	815.0
80.90	3127.0
81.90	777.0
85.70	170.0
86.90	3534.0
87.90	2924.0
90.90	468.0
92.00	2294.0
93.00	3620.0
94.00	9258.0
95.00	77800.0
96.00	5607.0
96.90	230.0
103.90	347.0
104.80	165.0
106.00	436.0
107.10	140.0
108.00	138.0
110.90	199.0
112.10	116.0
115.90	293.0
116.80	446.0
117.90	382.0
118.80	614.0
124.80	106.0
126.70	113.0
127.70	236.0
129.00	159.0
130.00	335.0
131.00	221.0
134.70	260.0
136.90	198.0
139.60	109.0
140.90	980.0
142.90	874.0
144.90	108.0
147.80	259.0
149.80	147.0
155.00	233.0
160.90	160.0
171.50	245.0
173.00	655.0
173.90	51720.0
174.90	4021.0
175.90	50288.0
176.90	2721.0
177.90	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB76