

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020838.D
 Acq On : 01 Apr 2021 14:39
 Operator : SY/MD
 Sample : M1845-01RE
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B1RE

Quant Time: Apr 02 07:18:00 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 02 07:14:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	488748	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	476429	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	231487	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	173172	49.91	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	99.82%		
7) Chloroethane-d5	1.571	69	149281	56.91	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	113.82%		
11) 1,1-Dichloroethene-d2	2.108	63	290395	44.36	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	88.72%		
21) 2-Butanone-d5	3.896	46	256163	113.47	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	113.47%		
24) Chloroform-d	4.352	84	441515	64.02	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	128.04%#		
26) 1,2-Dichloroethane-d4	5.037	65	299804	65.99	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	131.98%#		
32) Benzene-d6	5.053	84	806171	63.48	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	126.96%#		
36) 1,2-Dichloropropane-d6	6.072	67	235975	60.53	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	121.06%#		
41) Toluene-d8	7.320	98	738675	62.49	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	124.98%#		
43) trans-1,3-Dichloroprop...	7.625	79	124037	59.79	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	119.58%		
47) 2-Hexanone-d5	8.092	63	184377	112.80	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	112.80%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	329425	58.01	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	116.02%		
64) 1,2-Dichlorobenzene-d4	11.632	152	301536	67.12	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	134.24%#		
Target Compounds						
20) cis-1,2-Dichloroethene	3.921	96	3432	0.98	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020838.D
Acq On : 01 Apr 2021 14:39
Operator : SY/MD
Sample : M1845-01RE
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B1RE

Quant Time: Apr 02 07:18:00 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 02 07:14:26 2021
Response via : Initial Calibration

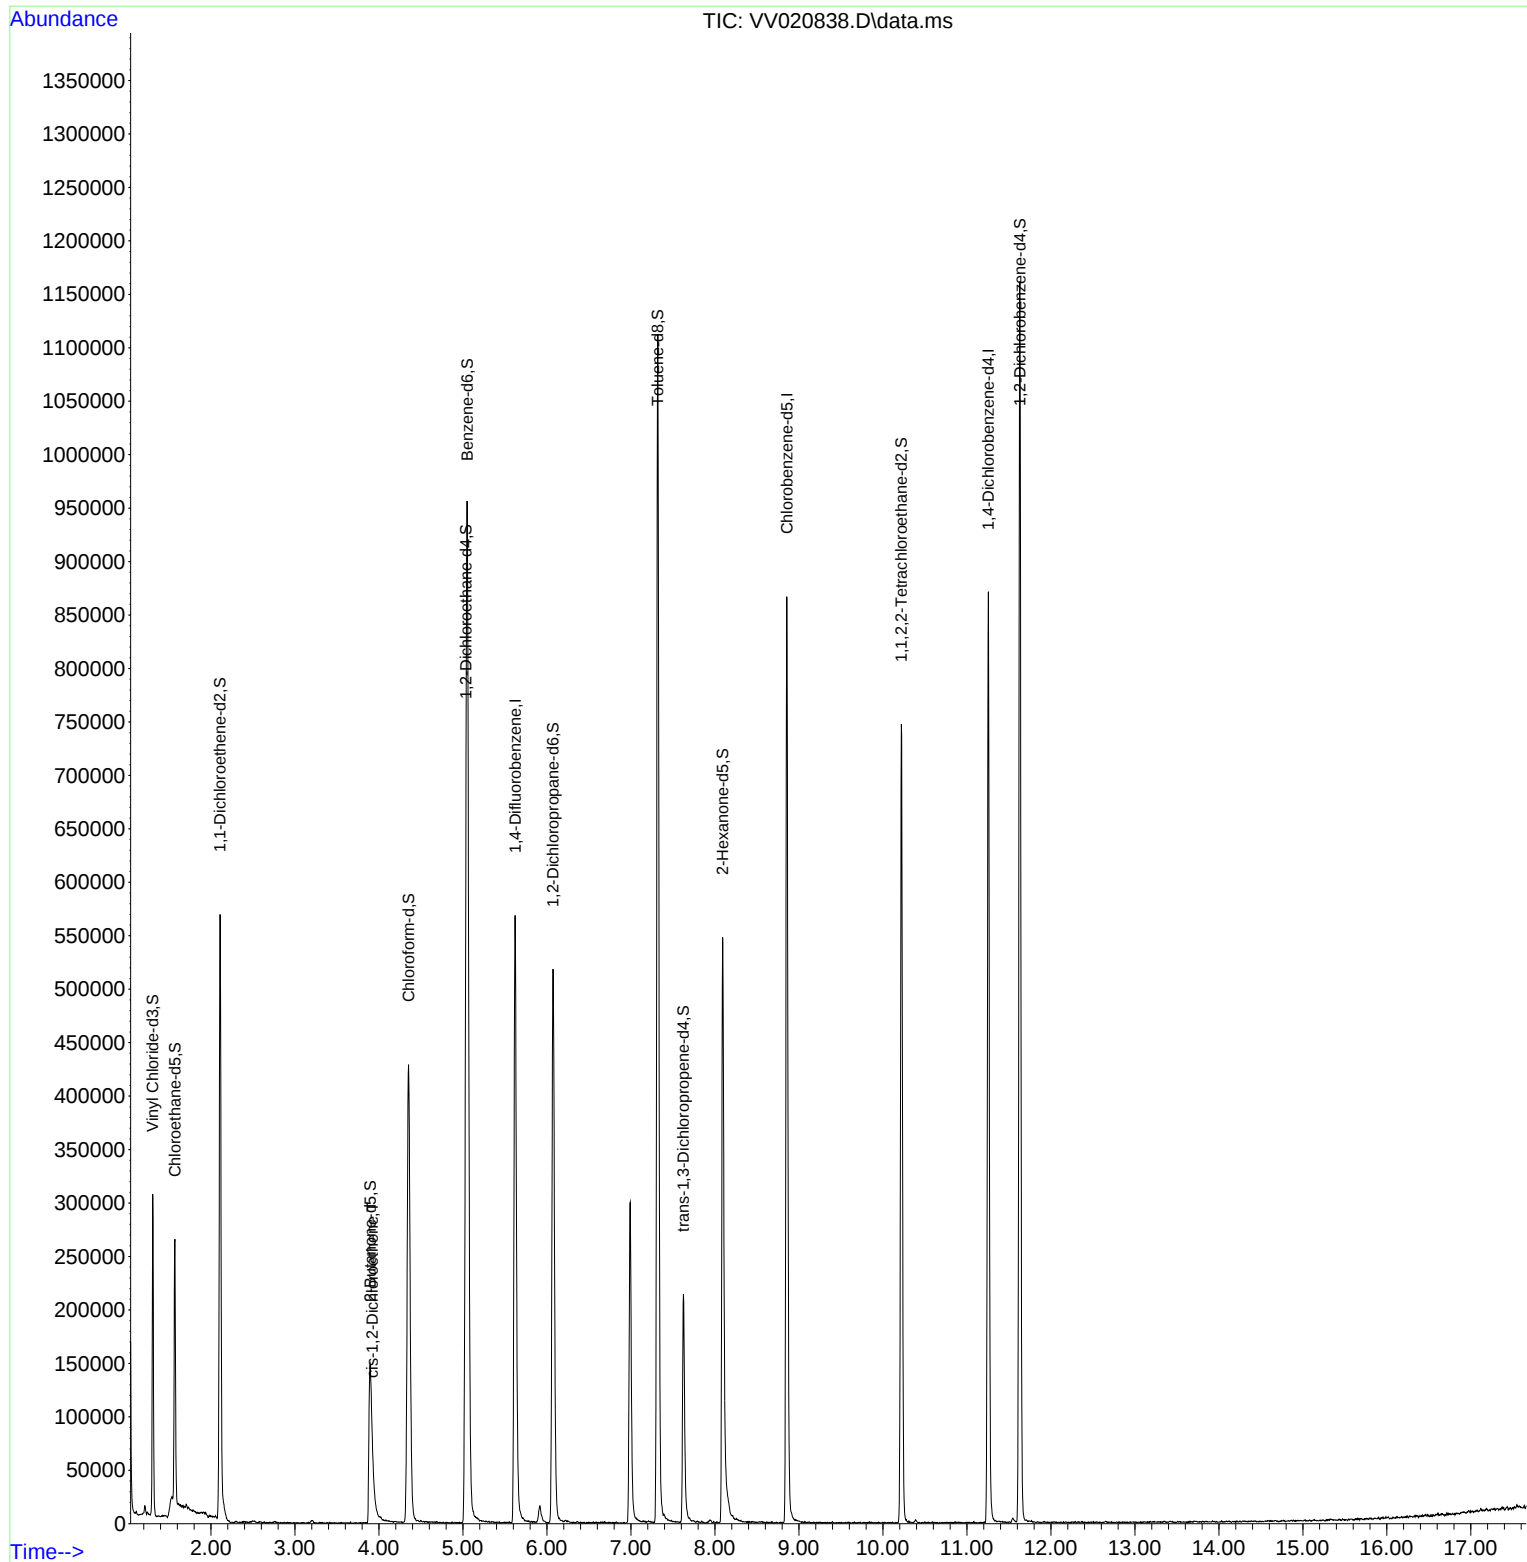

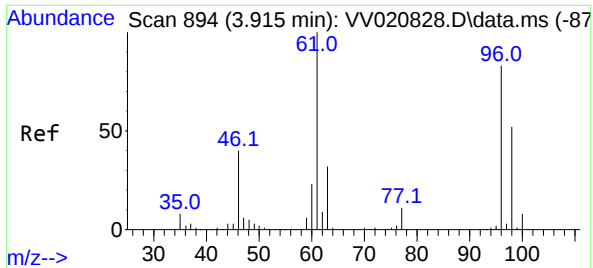

#20
 cis-1,2-Dichloroethene
 Concen: 0.98 ug/L
 RT: 3.921 min Scan# 896
 Delta R.T. 0.007 min
 Lab File: VV020838.D
 Acq: 01 Apr 2021 14:39

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B1RE

Tgt Ion: 96 Resp: 3432

Ion	Ratio	Lower	Upper
96	100		
61	120.3	89.9	167.0
68	0.0	0.0	0.0

