

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020831.D
 Acq On : 01 Apr 2021 11:54
 Operator : SY/MD
 Sample : M1845-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020822.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	95	rVB	361346	358181	12.33%	1.739%
2	1.568	157	164	175	rBV	305497	335496	11.55%	1.629%
3	2.108	321	332	356	rVB	692264	1028613	35.41%	4.995%
4	2.352	406	408	410	rBV	499	240	0.01%	0.001%
5	2.568	474	475	477	rBV	611	200	0.01%	0.001%
6	2.616	486	490	491	rBV2	1482	1044	0.04%	0.005%
7	2.709	516	519	522	rBV2	626	453	0.02%	0.002%
8	2.815	550	552	554	rVB2	416	167	0.01%	0.001%
9	2.847	559	562	567	rVB3	761	600	0.02%	0.003%
10	2.892	574	576	578	rBV	440	237	0.01%	0.001%
11	2.950	591	594	597	rBV3	724	421	0.01%	0.002%
12	3.047	621	624	630	rVB4	729	665	0.02%	0.003%
13	3.079	630	634	636	rBV2	379	283	0.01%	0.001%
14	3.137	650	652	653	rBV	460	214	0.01%	0.001%
15	3.249	685	687	691	rBV3	518	382	0.01%	0.002%
16	3.307	702	705	708	rBV2	461	304	0.01%	0.001%
17	3.359	718	721	722	rBV	577	269	0.01%	0.001%
18	3.603	795	797	798	rBV2	458	179	0.01%	0.001%
19	3.661	813	815	817	rBV	315	140	0.00%	0.001%
20	3.677	817	820	822	rBV3	675	346	0.01%	0.002%
21	3.699	825	827	829	rBV3	365	182	0.01%	0.001%
22	3.744	838	841	845	rBV	717	464	0.02%	0.002%
23	3.764	845	847	850	rBV	546	268	0.01%	0.001%
24	3.796	853	857	860	rBV4	924	770	0.03%	0.004%
25	3.838	868	870	871	rBV	551	237	0.01%	0.001%
26	3.883	874	884	914	rBV	170931	505120	17.39%	2.453%
27	4.349	1013	1029	1055	rBV	509599	1249339	43.01%	6.067%
28	4.834	1178	1180	1181	rBV	411	156	0.01%	0.001%
29	4.902	1199	1201	1202	rBV	451	146	0.01%	0.001%
30	4.912	1202	1204	1206	rVB3	675	285	0.01%	0.001%
31	4.982	1223	1226	1229	rBV3	561	504	0.02%	0.002%
32	5.047	1229	1246	1272	rBV3	1128716	2904759	100.00%	14.106%
33	5.481	1378	1381	1382	rBV2	587	229	0.01%	0.001%
34	5.490	1382	1384	1388	rBV2	835	624	0.02%	0.003%
35	5.551	1401	1403	1408	rVB4	985	437	0.02%	0.002%
36	5.619	1410	1424	1455	rBV	660763	1342488	46.22%	6.519%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020831.D
 Acq On : 01 Apr 2021 11:54
 Operator : SY/MD
 Sample : M1845-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.912	1505	1515	1528	rBV2	22268	45817	1.58%	0.222%
38	6.072	1551	1565	1589	rBV	639622	1275324	43.90%	6.193%
39	6.378	1658	1660	1663	rBV4	881	482	0.02%	0.002%
40	6.423	1672	1674	1676	rBV	912	382	0.01%	0.002%
41	6.471	1686	1689	1692	rVB2	965	643	0.02%	0.003%
42	6.497	1692	1697	1698	rBV2	501	300	0.01%	0.001%
43	6.516	1701	1703	1704	rBV	574	181	0.01%	0.001%
44	6.583	1721	1724	1725	rBV	632	343	0.01%	0.002%
45	6.876	1814	1815	1817	rVB2	429	143	0.00%	0.001%
46	6.889	1817	1819	1821	rBV	867	335	0.01%	0.002%
47	6.937	1830	1834	1837	rBV2	413	356	0.01%	0.002%
48	6.989	1837	1850	1876	rBV	364666	656207	22.59%	3.187%
49	7.223	1920	1923	1925	rBV3	1014	627	0.02%	0.003%
50	7.320	1940	1953	1975	rBV	1353859	2353471	81.02%	11.429%
51	7.625	2037	2048	2071	rBV	252213	445685	15.34%	2.164%
52	7.825	2107	2110	2113	rBV3	993	751	0.03%	0.004%
53	7.947	2139	2148	2159	rVB3	17367	29771	1.02%	0.145%
54	8.046	2177	2179	2181	rBV2	404	190	0.01%	0.001%
55	8.091	2183	2193	2225	rBV	604986	1139989	39.25%	5.536%
56	8.680	2371	2376	2377	rBV4	851	718	0.02%	0.003%
57	8.773	2402	2405	2408	rBV3	626	543	0.02%	0.003%
58	8.857	2419	2431	2461	rBV	999524	1658672	57.10%	8.055%
59	9.329	2575	2578	2580	rBV2	710	469	0.02%	0.002%
60	9.464	2618	2620	2623	rBV2	601	351	0.01%	0.002%
61	9.654	2677	2679	2681	rBV	881	437	0.02%	0.002%
62	9.715	2696	2698	2701	rBV3	525	302	0.01%	0.001%
63	9.786	2715	2720	2721	rBV2	353	221	0.01%	0.001%
64	10.014	2789	2791	2796	rBV3	626	572	0.02%	0.003%
65	10.072	2806	2809	2810	rBV	534	315	0.01%	0.002%
66	10.220	2841	2855	2880	rBV	872357	1364230	46.97%	6.625%
67	10.387	2896	2907	2923	rVB3	20304	35206	1.21%	0.171%
68	10.641	2983	2986	2988	rBV3	774	460	0.02%	0.002%
69	10.786	3028	3031	3034	rBV2	708	564	0.02%	0.003%
70	10.902	3065	3067	3068	rBV2	681	321	0.01%	0.002%
71	10.956	3082	3084	3088	rBV2	779	445	0.02%	0.002%
72	11.072	3116	3120	3125	rVB4	663	678	0.02%	0.003%
73	11.098	3126	3128	3130	rBV4	544	306	0.01%	0.001%
74	11.255	3165	3177	3198	rBV	1039379	1612312	55.51%	7.830%
75	11.545	3260	3267	3273	rBV7	5037	7504	0.26%	0.036%
76	11.632	3281	3294	3319	rBV	1419289	2220805	76.45%	10.785%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020831.D
Acq On : 01 Apr 2021 11:54
Operator : SY/MD
Sample : M1845-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Title : VOC Analysis

77	12.320	3506	3508	3513	rBV2	674	406	0.01%	0.002%
78	13.066	3738	3740	3742	rBV	819	428	0.01%	0.002%
79	13.329	3820	3822	3826	rBV4	1041	625	0.02%	0.003%




Sum of corrected areas: 20592329

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020831.D
Acq On : 01 Apr 2021 11:54
Operator : SY/MD
Sample : M1845-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

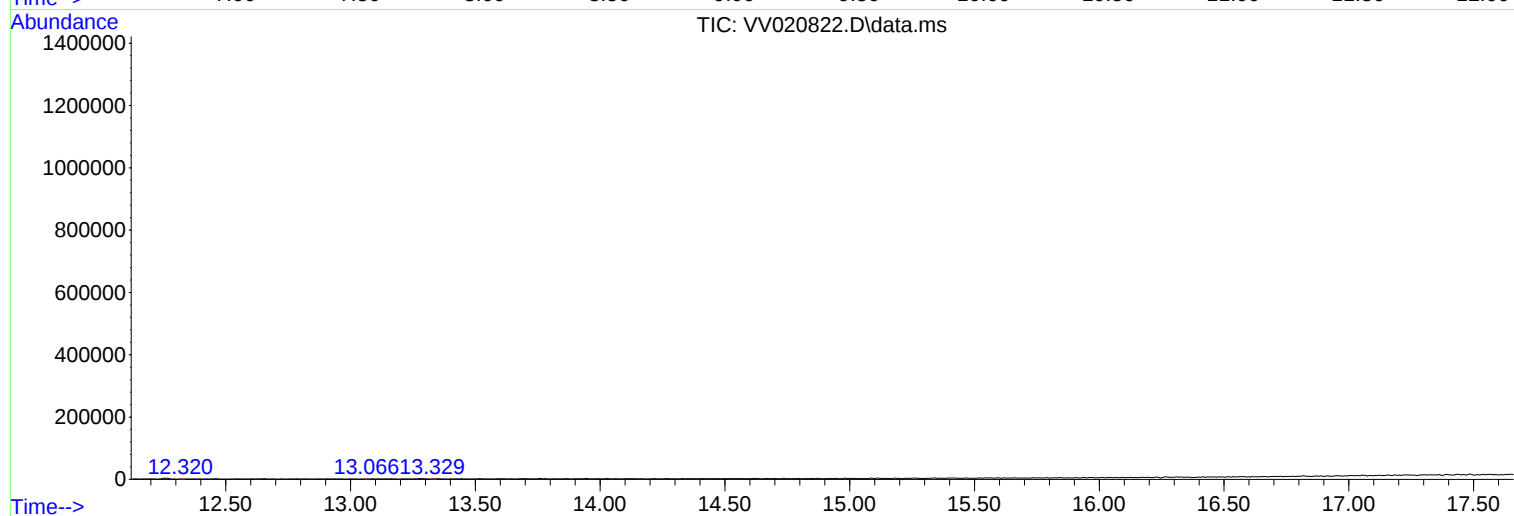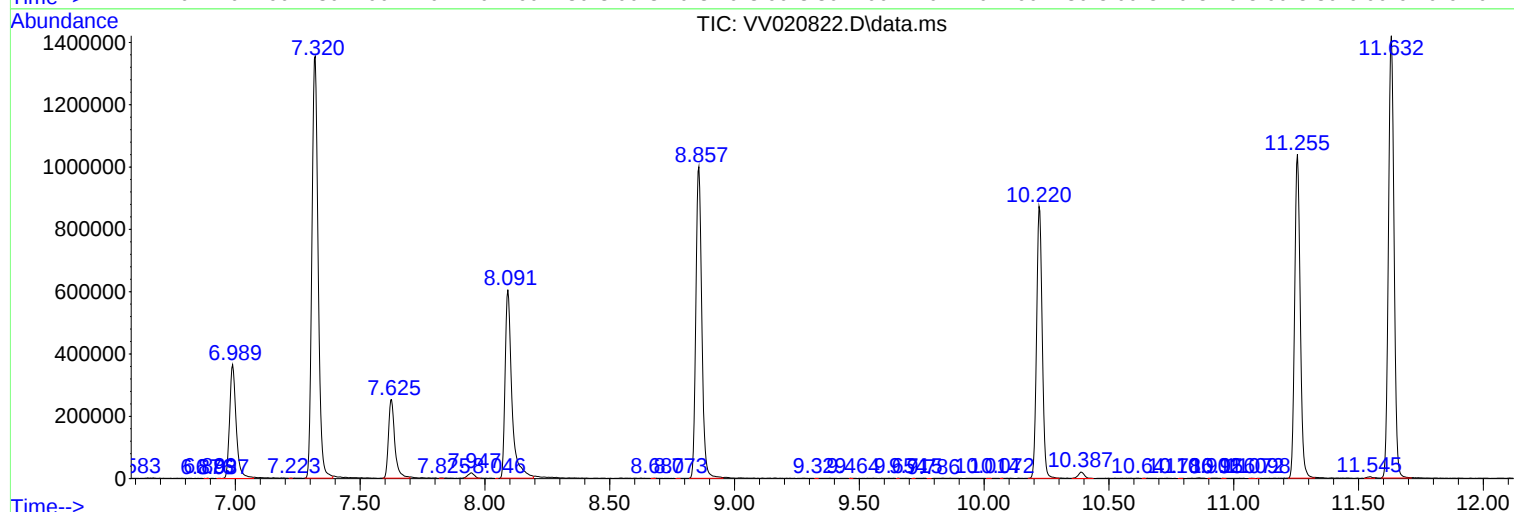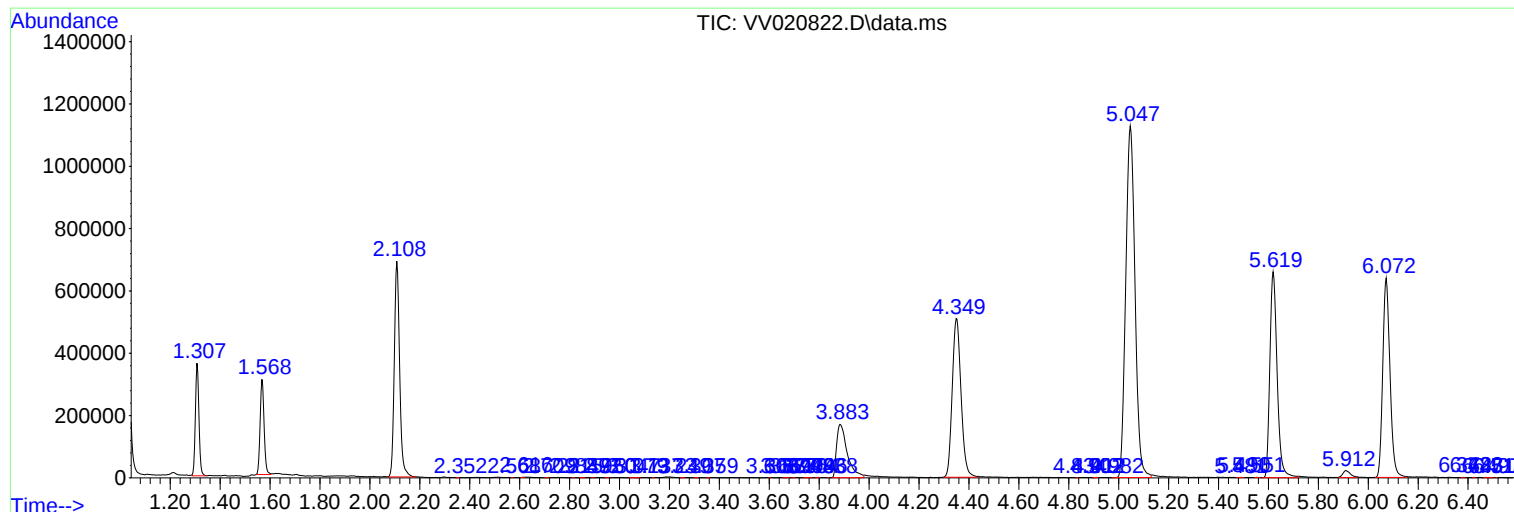

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020831.D
Acq On : 01 Apr 2021 11:54
Operator : SY/MD
Sample : M1845-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020831.D
Acq On : 01 Apr 2021 11:54
Operator : SY/MD
Sample : M1845-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
