

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020838.D
 Acq On : 01 Apr 2021 14:39
 Operator : SY/MD
 Sample : M1845-01RE
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B1RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020829.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	94	rVB	300894	297444	12.18%	1.726%
2	1.571	159	165	175	rVB	247800	281886	11.55%	1.636%
3	2.108	322	332	362	rVB	566990	863267	35.36%	5.009%
4	2.423	427	430	432	rBV2	835	618	0.03%	0.004%
5	2.458	439	441	442	rBV2	889	404	0.02%	0.002%
6	2.638	490	497	502	rVB3	1013	1050	0.04%	0.006%
7	2.909	578	581	586	rBV5	792	713	0.03%	0.004%
8	2.937	588	590	595	rVB3	725	617	0.03%	0.004%
9	2.963	596	598	601	rBV2	455	290	0.01%	0.002%
10	3.076	629	633	635	rBV2	629	342	0.01%	0.002%
11	3.191	664	669	671	rBV4	2025	1746	0.07%	0.010%
12	3.281	695	697	699	rBV4	643	369	0.02%	0.002%
13	3.391	728	731	736	rVB2	620	394	0.02%	0.002%
14	3.436	743	745	748	rBV2	530	333	0.01%	0.002%
15	3.471	754	756	759	rBV	614	375	0.02%	0.002%
16	3.661	813	815	818	rBV2	1086	491	0.02%	0.003%
17	3.728	834	836	841	rVB2	659	431	0.02%	0.003%
18	3.761	841	846	849	rBV2	526	558	0.02%	0.003%
19	3.790	852	855	857	rBV	609	395	0.02%	0.002%
20	3.812	859	862	864	rBV2	534	286	0.01%	0.002%
21	3.844	870	872	874	rBV	500	254	0.01%	0.001%
22	3.896	877	888	921	rBV2	148340	450896	18.47%	2.616%
23	4.352	1015	1030	1059	rBV	427095	1042975	42.72%	6.052%
24	4.690	1131	1135	1140	rBV3	1195	1108	0.05%	0.006%
25	4.767	1156	1159	1164	rVB2	962	713	0.03%	0.004%
26	4.789	1164	1166	1168	rBV2	477	310	0.01%	0.002%
27	4.802	1168	1170	1176	rVB3	598	600	0.02%	0.003%
28	4.870	1188	1191	1194	rBV2	1321	908	0.04%	0.005%
29	5.050	1229	1247	1277	rBV2	955936	2441254	100.00%	14.165%
30	5.622	1412	1425	1452	rBV	568260	1146248	46.95%	6.651%
31	6.072	1549	1565	1587	rBV	518225	1065527	43.65%	6.183%
32	6.310	1638	1639	1641	rBV	832	339	0.01%	0.002%
33	6.346	1648	1650	1651	rBV2	556	285	0.01%	0.002%
34	6.404	1666	1668	1672	rVB3	978	537	0.02%	0.003%
35	6.439	1676	1679	1684	rVB3	888	851	0.03%	0.005%
36	6.468	1684	1688	1689	rBV2	593	337	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020838.D
 Acq On : 01 Apr 2021 14:39
 Operator : SY/MD
 Sample : M1845-01RE
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B1RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	6.500	1696	1698	1702	rBV3	887	575	0.02%	0.003%
38	6.551	1712	1714	1717	rVB4	968	505	0.02%	0.003%
39	6.587	1720	1725	1727	rBV5	930	615	0.03%	0.004%
40	6.616	1732	1734	1737	rVB2	704	341	0.01%	0.002%
41	6.641	1740	1742	1745	rBV3	762	400	0.02%	0.002%
42	6.744	1772	1774	1778	rVB4	713	456	0.02%	0.003%
43	6.783	1785	1786	1790	rVB2	712	407	0.02%	0.002%
44	6.812	1793	1795	1796	rBV	681	246	0.01%	0.001%
45	6.828	1796	1800	1804	rBV5	1068	833	0.03%	0.005%
46	6.879	1813	1816	1822	rBV3	371	384	0.02%	0.002%
47	6.918	1827	1828	1833	rVB2	579	275	0.01%	0.002%
48	6.992	1835	1851	1871	rBV	300249	541010	22.16%	3.139%
49	7.320	1940	1953	1973	rBV	1111533	1933026	79.18%	11.216%
50	7.625	2038	2048	2067	rBV2	213432	371920	15.23%	2.158%
51	7.908	2129	2136	2139	rBV5	1139	1274	0.05%	0.007%
52	7.928	2139	2142	2143	rBV3	1468	861	0.04%	0.005%
53	7.985	2158	2160	2164	rVB5	913	412	0.02%	0.002%
54	8.092	2184	2193	2226	rBV	546494	1018729	41.73%	5.911%
55	8.407	2289	2291	2292	rBV	1196	478	0.02%	0.003%
56	8.484	2313	2315	2319	rBV3	576	430	0.02%	0.002%
57	8.629	2358	2360	2363	rVB2	808	421	0.02%	0.002%
58	8.645	2363	2365	2367	rBV2	631	337	0.01%	0.002%
59	8.709	2382	2385	2387	rBV2	558	406	0.02%	0.002%
60	8.857	2419	2431	2453	rBV	866141	1399665	57.33%	8.122%
61	9.040	2486	2488	2493	rVB5	927	775	0.03%	0.004%
62	9.063	2493	2495	2497	rBV2	883	378	0.02%	0.002%
63	9.149	2519	2522	2524	rBV3	484	270	0.01%	0.002%
64	9.214	2539	2542	2546	rVB2	927	684	0.03%	0.004%
65	9.236	2546	2549	2552	rBV2	686	512	0.02%	0.003%
66	9.252	2552	2554	2559	rVB4	796	676	0.03%	0.004%
67	9.339	2577	2581	2583	rBV2	828	548	0.02%	0.003%
68	9.400	2597	2600	2603	rVB3	1093	584	0.02%	0.003%
69	9.535	2638	2642	2645	rBV3	311	338	0.01%	0.002%
70	9.577	2653	2655	2658	rBV2	544	381	0.02%	0.002%
71	9.635	2669	2673	2674	rBV	554	373	0.02%	0.002%
72	9.661	2680	2681	2685	rVB2	823	342	0.01%	0.002%
73	9.809	2724	2727	2729	rBV2	544	311	0.01%	0.002%
74	9.825	2729	2732	2734	rBV2	804	457	0.02%	0.003%
75	9.841	2734	2737	2739	rVV3	996	568	0.02%	0.003%
76	9.866	2743	2745	2749	rVB2	692	419	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020838.D
 Acq On : 01 Apr 2021 14:39
 Operator : SY/MD
 Sample : M1845-01RE
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B1RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.024	2792	2794	2799	rBV2	616	384	0.02%	0.002%
78	10.114	2820	2822	2827	rVB3	831	610	0.02%	0.004%
79	10.149	2830	2833	2836	rBV	605	453	0.02%	0.003%
80	10.220	2843	2855	2871	rBV	746727	1176908	48.21%	6.829%
81	10.310	2880	2883	2885	rVB2	1473	842	0.03%	0.005%
82	10.673	2993	2996	3000	rBV2	778	538	0.02%	0.003%
83	10.860	3049	3054	3058	rVV3	1318	1273	0.05%	0.007%
84	11.024	3102	3105	3111	rVB2	815	678	0.03%	0.004%
85	11.053	3111	3114	3117	rBV	554	408	0.02%	0.002%
86	11.082	3120	3123	3127	rVB3	1266	842	0.03%	0.005%
87	11.146	3140	3143	3145	rBV	426	294	0.01%	0.002%
88	11.207	3158	3162	3165	rVB2	854	554	0.02%	0.003%
89	11.255	3165	3177	3196	rBV	870908	1333033	54.60%	7.735%
90	11.545	3260	3267	3276	rBV7	4277	7548	0.31%	0.044%
91	11.632	3282	3294	3314	rBV	1159759	1818578	74.49%	10.552%
92	12.011	3410	3412	3413	rBV	690	256	0.01%	0.001%
93	12.149	3452	3455	3458	rBV3	1196	673	0.03%	0.004%
94	12.252	3484	3487	3492	rBV4	842	891	0.04%	0.005%
95	12.448	3546	3548	3551	rBV3	734	376	0.02%	0.002%
96	12.583	3589	3590	3595	rVB3	666	410	0.02%	0.002%
97	12.686	3620	3622	3624	rBV2	659	342	0.01%	0.002%
98	12.808	3658	3660	3662	rBV2	680	274	0.01%	0.002%
99	13.072	3740	3742	3745	rBV3	809	393	0.02%	0.002%
100	13.966	4018	4020	4023	rBV2	954	577	0.02%	0.003%




Sum of corrected areas: 17233908

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020838.D
Acq On : 01 Apr 2021 14:39
Operator : SY/MD
Sample : M1845-01RE
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B1RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

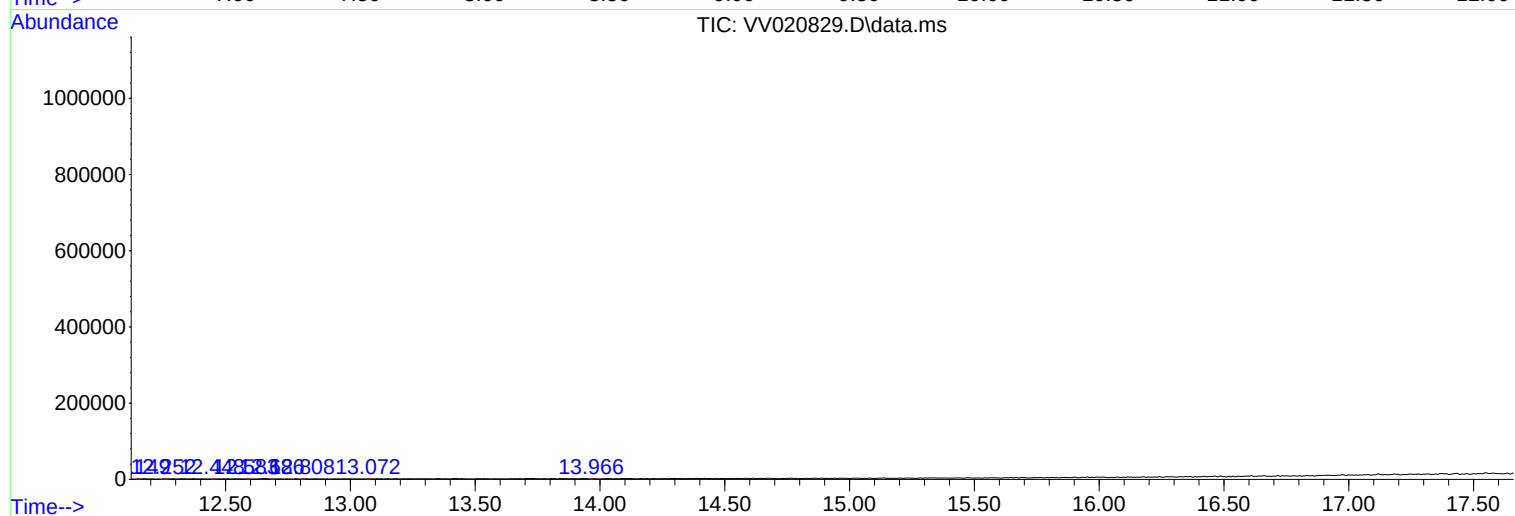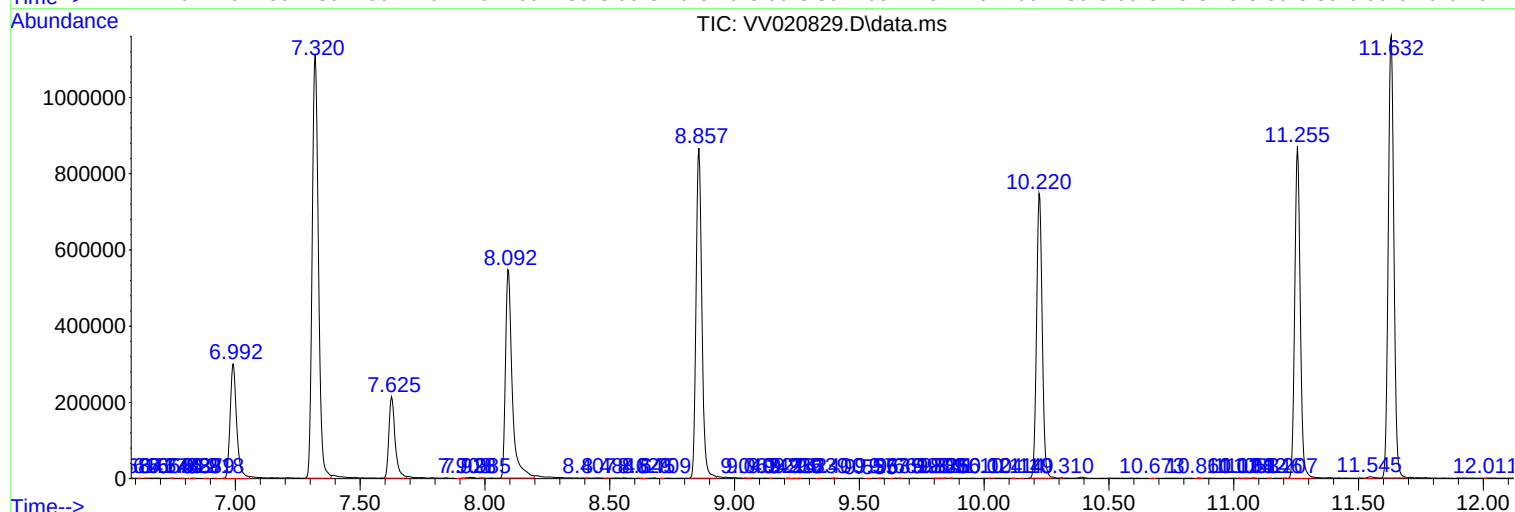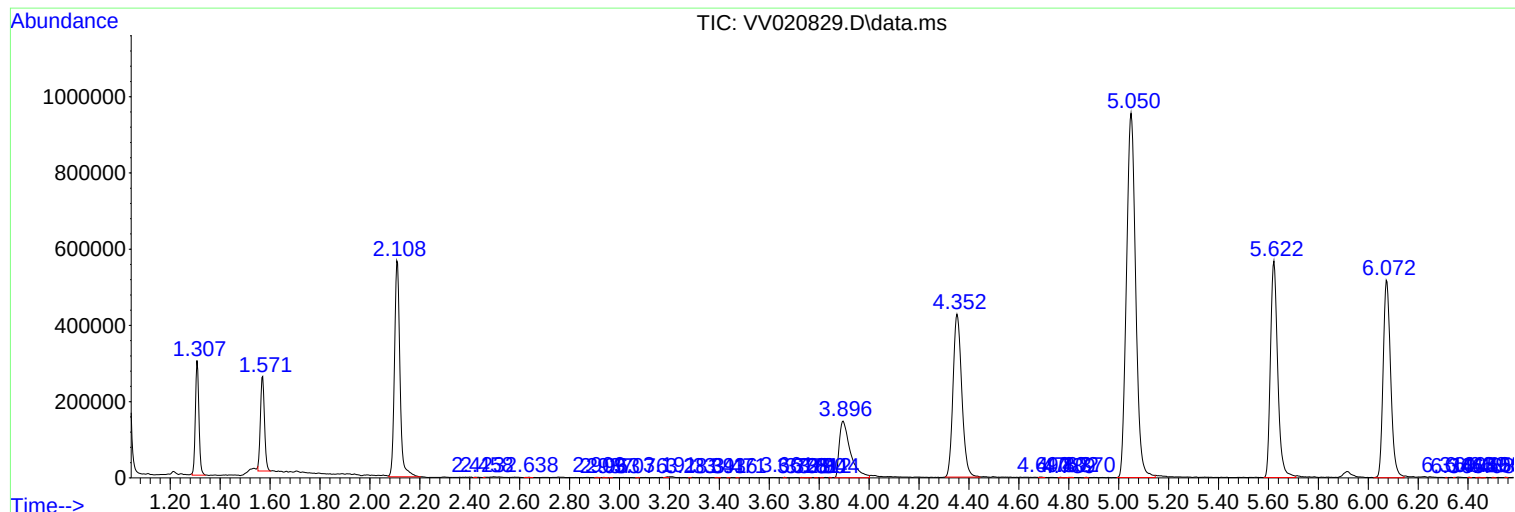

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020838.D
Acq On : 01 Apr 2021 14:39
Operator : SY/MD
Sample : M1845-01RE
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B1RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020838.D
Acq On : 01 Apr 2021 14:39
Operator : SY/MD
Sample : M1845-01RE
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B1RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
