

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW040121\
 Data File : VW020840.D
 Acq On : 01 Apr 2021 15:27
 Operator : SY/MD
 Sample : M1879-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW198

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VW020831.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	77	84	103	rBV	3634965	3770437	21.11%	9.604%
2	1.571	158	165	178	rVB	237311	264272	1.48%	0.673%
3	2.108	322	332	361	rVB	553477	838514	4.69%	2.136%
4	2.362	406	411	412	rBV3	731	534	0.00%	0.001%
5	2.410	425	426	429	rBV2	534	315	0.00%	0.001%
6	2.574	474	477	479	rBV2	631	351	0.00%	0.001%
7	2.587	479	481	485	rVB2	569	363	0.00%	0.001%
8	2.610	485	488	490	rBV2	828	533	0.00%	0.001%
9	2.635	493	496	499	rBV3	852	615	0.00%	0.002%
10	2.767	529	537	552	rVB3	10582	20163	0.11%	0.051%
11	2.847	559	562	565	rBV3	524	424	0.00%	0.001%
12	2.918	583	584	586	rBV	419	208	0.00%	0.001%
13	2.992	605	607	610	rVB2	670	353	0.00%	0.001%
14	3.018	610	615	617	rBV2	745	652	0.00%	0.002%
15	3.082	632	635	641	rBV4	701	471	0.00%	0.001%
16	3.140	652	653	657	rBV	323	248	0.00%	0.001%
17	3.156	657	658	660	rVB2	507	186	0.00%	0.000%
18	3.211	672	675	679	rVB2	997	642	0.00%	0.002%
19	3.233	679	682	683	rBV2	316	168	0.00%	0.000%
20	3.243	683	685	688	rVB3	658	325	0.00%	0.001%
21	3.317	706	708	710	rBV	195	70	0.00%	0.000%
22	3.330	710	712	715	rBV	352	247	0.00%	0.001%
23	3.378	725	727	730	rBV	479	212	0.00%	0.001%
24	3.439	744	746	751	rBV2	979	810	0.00%	0.002%
25	3.465	751	754	755	rVV	362	205	0.00%	0.001%
26	3.507	763	767	769	rBV2	366	253	0.00%	0.001%
27	3.545	775	779	780	rBV2	594	455	0.00%	0.001%
28	3.600	794	796	798	rBV	484	257	0.00%	0.001%
29	3.613	798	800	804	rVB2	535	334	0.00%	0.001%
30	3.632	804	806	807	rBV2	302	127	0.00%	0.000%
31	3.680	818	821	825	rBV2	696	404	0.00%	0.001%
32	3.722	829	834	842	rVB4	427	487	0.00%	0.001%
33	3.754	842	844	846	rBV	267	166	0.00%	0.000%
34	3.799	856	858	860	rBV	448	273	0.00%	0.001%
35	3.912	875	893	935	rBV	7422437	17863788	100.00%	45.504%
36	4.352	1016	1030	1057	rVB	425488	1038890	5.82%	2.646%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW040121\
 Data File : VW020840.D
 Acq On : 01 Apr 2021 15:27
 Operator : SY/MD
 Sample : M1879-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW198

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	4.934	1206	1211	1215	rBV3	826	812	0.00%	0.002%
38	4.976	1222	1224	1226	rBV2	606	365	0.00%	0.001%
39	5.050	1230	1247	1276	rVV2	945372	2420041	13.55%	6.165%
40	5.388	1349	1352	1356	rBV	766	744	0.00%	0.002%
41	5.449	1369	1371	1374	rBV3	781	602	0.00%	0.002%
42	5.542	1396	1400	1404	rVB5	1467	1329	0.01%	0.003%
43	5.619	1412	1424	1451	rBV	740268	1489836	8.34%	3.795%
44	5.912	1503	1515	1530	rBV3	19292	42812	0.24%	0.109%
45	6.072	1552	1565	1584	rBV2	509681	1049299	5.87%	2.673%
46	6.433	1671	1677	1681	rBV5	770	995	0.01%	0.003%
47	6.487	1692	1694	1698	rBV3	488	283	0.00%	0.001%
48	6.613	1730	1733	1734	rBV2	507	240	0.00%	0.001%
49	6.661	1745	1748	1757	rVB6	1863	1899	0.01%	0.005%
50	6.796	1788	1790	1792	rBV2	804	442	0.00%	0.001%
51	6.834	1800	1802	1803	rBV2	471	215	0.00%	0.001%
52	6.924	1826	1830	1831	rBV2	539	330	0.00%	0.001%
53	6.989	1839	1850	1872	rBV	297779	539362	3.02%	1.374%
54	7.275	1935	1939	1940	rBV2	715	377	0.00%	0.001%
55	7.320	1941	1953	1973	rBV	1102531	1902212	10.65%	4.845%
56	7.625	2038	2048	2071	rBV	217369	376720	2.11%	0.960%
57	7.809	2103	2105	2107	rBV	674	339	0.00%	0.001%
58	7.844	2114	2116	2117	rBV2	794	276	0.00%	0.001%
59	7.931	2140	2143	2145	rBV3	1121	785	0.00%	0.002%
60	8.095	2181	2194	2234	rBV	542646	1055720	5.91%	2.689%
61	8.587	2344	2347	2349	rBV2	974	555	0.00%	0.001%
62	8.629	2358	2360	2362	rBV2	800	310	0.00%	0.001%
63	8.641	2362	2364	2369	rVB3	920	599	0.00%	0.002%
64	8.664	2369	2371	2375	rBV4	1103	736	0.00%	0.002%
65	8.751	2394	2398	2400	rBV2	407	291	0.00%	0.001%
66	8.857	2420	2431	2454	rBV	1127364	1819806	10.19%	4.636%
67	9.143	2517	2520	2524	rVB4	1380	982	0.01%	0.003%
68	9.262	2553	2557	2559	rBV2	859	636	0.00%	0.002%
69	9.349	2579	2584	2585	rBV3	922	743	0.00%	0.002%
70	9.403	2599	2601	2605	rBV2	860	547	0.00%	0.001%
71	9.442	2611	2613	2615	rBV	613	261	0.00%	0.001%
72	9.481	2624	2625	2627	rBV	523	217	0.00%	0.001%
73	9.609	2663	2665	2670	rVB2	994	594	0.00%	0.002%
74	10.223	2843	2856	2879	rBV	749898	1183430	6.62%	3.015%
75	10.346	2891	2894	2895	rBV	770	355	0.00%	0.001%
76	10.419	2915	2917	2919	rBV	630	321	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020840.D
 Acq On : 01 Apr 2021 15:27
 Operator : SY/MD
 Sample : M1879-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW198

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.452	2925	2927	2932	rBV3	951	764	0.00%	0.002%
78	10.638	2982	2985	2986	rBV	607	297	0.00%	0.001%
79	10.706	3003	3006	3008	rBV	511	290	0.00%	0.001%
80	10.760	3022	3023	3025	rBV	413	172	0.00%	0.000%
81	10.776	3025	3028	3030	rVV	681	379	0.00%	0.001%
82	10.960	3080	3085	3087	rBV2	964	1001	0.01%	0.003%
83	11.255	3166	3177	3197	rBV	1102946	1714567	9.60%	4.368%
84	11.632	3281	3294	3312	rBV	1181502	1831230	10.25%	4.665%
85	11.831	3354	3356	3362	rVB4	1898	1760	0.01%	0.004%
86	11.857	3362	3364	3369	rBV2	775	590	0.00%	0.002%
87	12.165	3456	3460	3463	rBV3	1072	755	0.00%	0.002%
88	12.368	3520	3523	3528	rBV3	864	809	0.00%	0.002%
89	12.435	3542	3544	3546	rBV3	913	393	0.00%	0.001%
90	12.545	3576	3578	3580	rBV	794	405	0.00%	0.001%
91	12.776	3648	3650	3654	rBV2	833	773	0.00%	0.002%




Sum of corrected areas: 39257355

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020840.D
Acq On : 01 Apr 2021 15:27
Operator : SY/MD
Sample : M1879-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW198

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

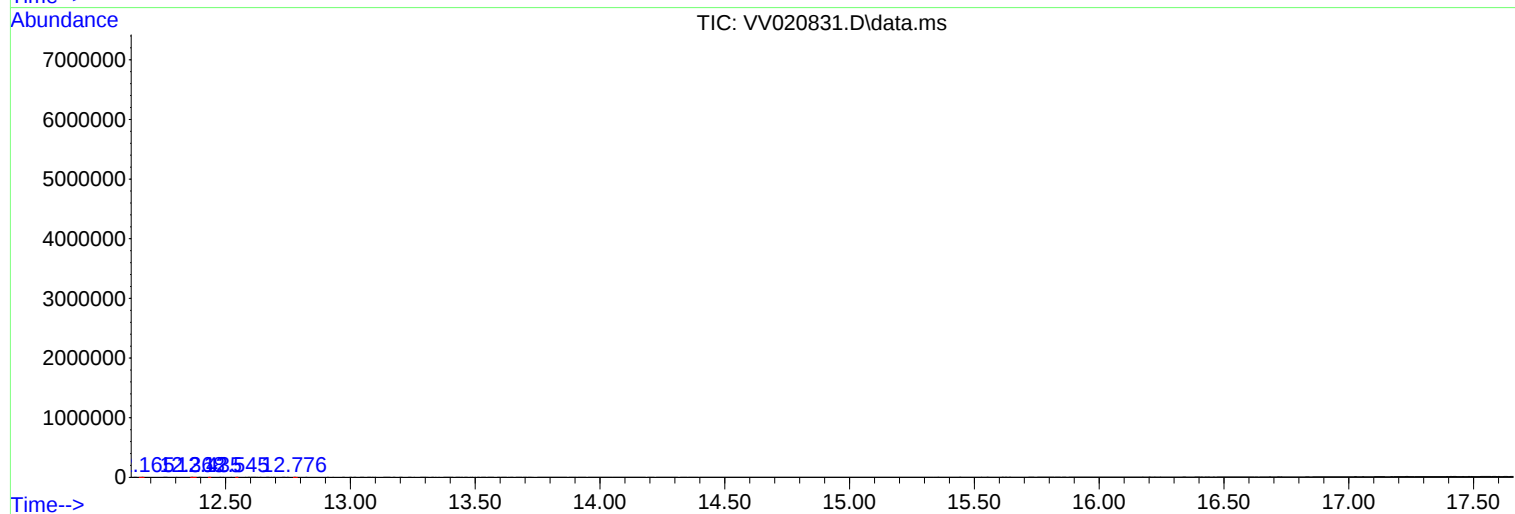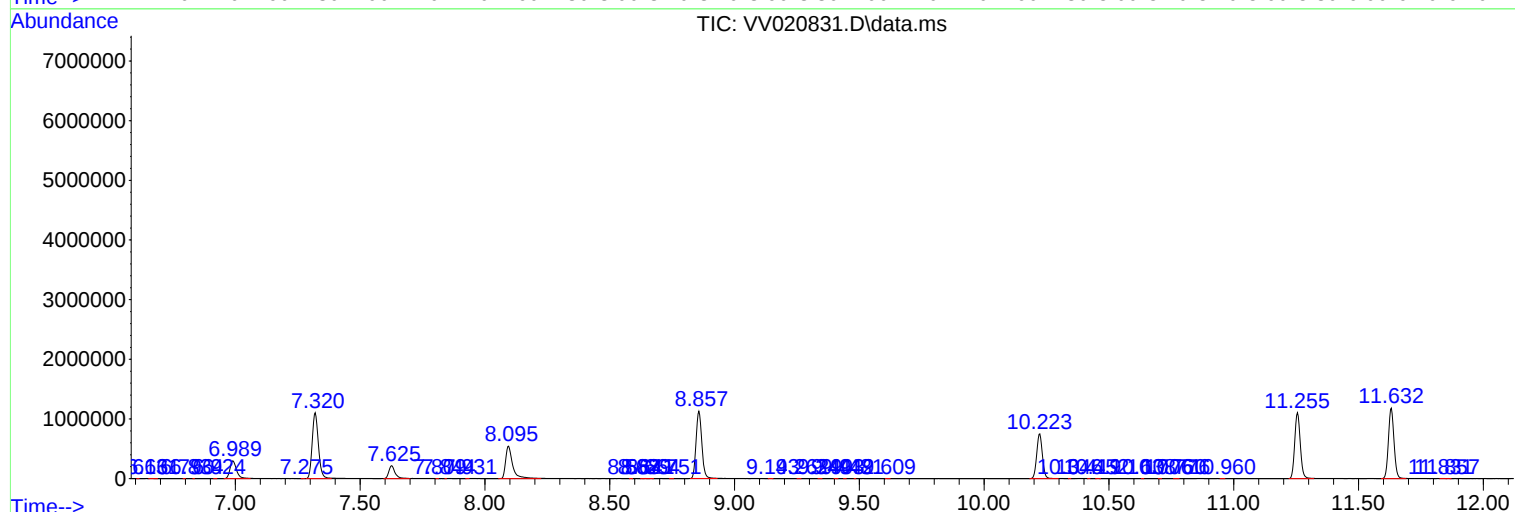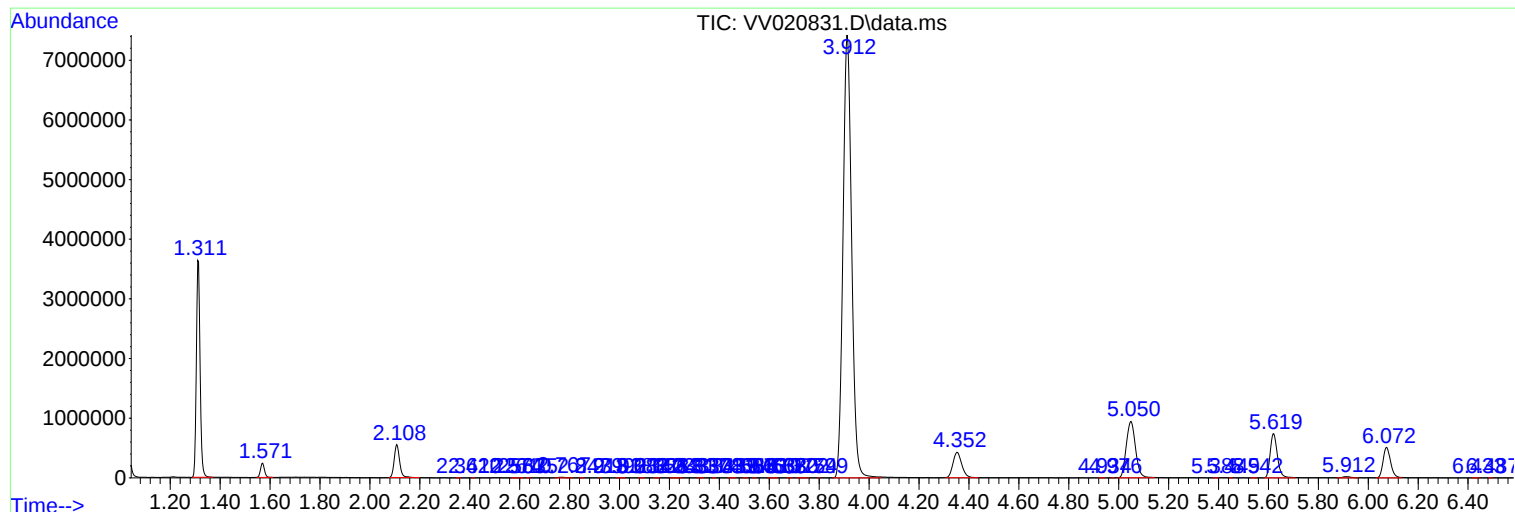

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020840.D
Acq On : 01 Apr 2021 15:27
Operator : SY/MD
Sample : M1879-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW198

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020840.D
Acq On : 01 Apr 2021 15:27
Operator : SY/MD
Sample : M1879-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW198

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------