

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020841.D
 Acq On : 01 Apr 2021 15:51
 Operator : SY/MD
 Sample : M1879-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW199

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020832.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	99	rVB	304916	324970	13.35%	1.795%
2	1.571	157	165	178	rBV	243455	276569	11.36%	1.528%
3	2.108	322	332	366	rVB	565003	850202	34.92%	4.697%
4	2.301	386	392	400	rVB5	1215	1798	0.07%	0.010%
5	2.375	413	415	417	rVB3	784	214	0.01%	0.001%
6	2.484	446	449	451	rBV	829	414	0.02%	0.002%
7	2.513	453	458	464	rVV3	1534	1585	0.07%	0.009%
8	2.606	485	487	491	rVB2	790	557	0.02%	0.003%
9	2.639	494	497	500	rBV2	561	340	0.01%	0.002%
10	2.696	513	515	517	rBV2	341	207	0.01%	0.001%
11	2.783	539	542	544	rBV3	615	310	0.01%	0.002%
12	2.835	556	558	559	rBV	329	143	0.01%	0.001%
13	2.844	559	561	563	rVV	331	167	0.01%	0.001%
14	2.925	582	586	588	rBV	464	361	0.01%	0.002%
15	2.995	607	608	611	rBV2	379	184	0.01%	0.001%
16	3.011	611	613	615	rVB3	426	197	0.01%	0.001%
17	3.021	615	616	619	rBV2	438	263	0.01%	0.001%
18	3.069	629	631	632	rBV2	198	55	0.00%	0.000%
19	3.082	633	635	640	rVB2	618	349	0.01%	0.002%
20	3.105	640	642	644	rBV2	616	349	0.01%	0.002%
21	3.169	660	662	664	rBV	548	190	0.01%	0.001%
22	3.243	682	685	690	rVB3	681	593	0.02%	0.003%
23	3.359	718	721	723	rBV2	334	205	0.01%	0.001%
24	3.384	727	729	732	rVV	711	355	0.01%	0.002%
25	3.410	735	737	738	rBV	239	103	0.00%	0.001%
26	3.433	742	744	746	rBV	388	145	0.01%	0.001%
27	3.446	746	748	750	rBV	472	216	0.01%	0.001%
28	3.465	752	754	756	rBV2	509	183	0.01%	0.001%
29	3.526	772	773	774	rBV	239	61	0.00%	0.000%
30	3.545	777	779	784	rBV2	551	402	0.02%	0.002%
31	3.581	787	790	791	rBV	346	158	0.01%	0.001%
32	3.677	818	820	823	rBV	297	150	0.01%	0.001%
33	3.693	823	825	826	rBV	249	138	0.01%	0.001%
34	3.712	826	831	835	rVB3	476	551	0.02%	0.003%
35	3.806	858	860	862	rVB	706	290	0.01%	0.002%
36	3.822	862	865	868	rBV2	725	533	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020841.D
 Acq On : 01 Apr 2021 15:51
 Operator : SY/MD
 Sample : M1879-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW199

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	3.841	868	871	873	rVB	539	296	0.01%	0.002%
38	3.854	873	875	877	rVB	209	88	0.00%	0.000%
39	3.899	877	889	922	rBV	141913	480954	19.75%	2.657%
40	4.352	1016	1030	1055	rVB	417510	1020905	41.93%	5.640%
41	4.767	1157	1159	1162	rBV3	565	360	0.01%	0.002%
42	4.867	1186	1190	1193	rBV3	719	531	0.02%	0.003%
43	4.899	1196	1200	1203	rBV3	688	500	0.02%	0.003%
44	4.915	1203	1205	1207	rBV	482	244	0.01%	0.001%
45	4.950	1213	1216	1218	rBV2	712	364	0.01%	0.002%
46	4.986	1225	1227	1229	rBV	479	222	0.01%	0.001%
47	5.050	1230	1247	1273	rBV2	957859	2435062	100.00%	13.453%
48	5.426	1362	1364	1366	rVB2	924	366	0.02%	0.002%
49	5.478	1378	1380	1384	rBV2	860	751	0.03%	0.004%
50	5.622	1412	1425	1452	rBV	691497	1389578	57.07%	7.677%
51	5.912	1506	1515	1533	rVB3	21205	47076	1.93%	0.260%
52	6.002	1541	1543	1544	rBV	502	184	0.01%	0.001%
53	6.072	1552	1565	1588	rBV	529130	1063838	43.69%	5.877%
54	6.368	1655	1657	1660	rBV3	680	387	0.02%	0.002%
55	6.433	1675	1677	1681	rVB2	569	349	0.01%	0.002%
56	6.458	1681	1685	1690	rBV2	1113	993	0.04%	0.005%
57	6.503	1696	1699	1702	rBV	509	245	0.01%	0.001%
58	6.519	1702	1704	1705	rBV	579	208	0.01%	0.001%
59	6.609	1730	1732	1734	rBV3	513	249	0.01%	0.001%
60	6.664	1747	1749	1752	rBV2	690	363	0.01%	0.002%
61	6.699	1758	1760	1762	rVB	722	294	0.01%	0.002%
62	6.719	1762	1766	1767	rBV2	801	486	0.02%	0.003%
63	6.770	1780	1782	1787	rBV4	609	423	0.02%	0.002%
64	6.789	1787	1788	1790	rBV2	353	148	0.01%	0.001%
65	6.844	1802	1805	1806	rBV	867	458	0.02%	0.003%
66	6.931	1829	1832	1835	rBV3	448	325	0.01%	0.002%
67	6.989	1839	1850	1874	rBV	300363	540433	22.19%	2.986%
68	7.320	1939	1953	1980	rBV	1118720	1937324	79.56%	10.703%
69	7.625	2037	2048	2068	rBV	211984	367455	15.09%	2.030%
70	7.873	2123	2125	2130	rBV4	985	826	0.03%	0.005%
71	8.092	2183	2193	2230	rBV	547250	1033738	42.45%	5.711%
72	8.535	2327	2331	2334	rVB2	1291	1057	0.04%	0.006%
73	8.696	2380	2381	2385	rBV	700	494	0.02%	0.003%
74	8.857	2419	2431	2456	rBV	1059816	1700069	69.82%	9.392%
75	9.153	2520	2523	2526	rBV3	730	481	0.02%	0.003%
76	9.371	2586	2591	2593	rBV2	786	670	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020841.D
 Acq On : 01 Apr 2021 15:51
 Operator : SY/MD
 Sample : M1879-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW199

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	9.426	2607	2608	2610	rBV	271	72	0.00%	0.000%
78	9.494	2626	2629	2630	rBV2	651	442	0.02%	0.002%
79	9.725	2699	2701	2703	rBV	404	226	0.01%	0.001%
80	9.767	2711	2714	2717	rBV2	794	460	0.02%	0.003%
81	9.821	2729	2731	2732	rBV2	562	187	0.01%	0.001%
82	9.847	2737	2739	2743	rBV4	628	446	0.02%	0.002%
83	10.082	2810	2812	2815	rBV	686	283	0.01%	0.002%
84	10.101	2815	2818	2821	rBV3	937	641	0.03%	0.004%
85	10.220	2842	2855	2872	rBV	742653	1176203	48.30%	6.498%
86	10.352	2893	2896	2897	rBV3	628	320	0.01%	0.002%
87	10.535	2951	2953	2955	rBV2	426	220	0.01%	0.001%
88	11.059	3114	3116	3119	rVB	614	320	0.01%	0.002%
89	11.085	3122	3124	3126	rBV	519	302	0.01%	0.002%
90	11.153	3143	3145	3147	rBV3	685	254	0.01%	0.001%
91	11.256	3165	3177	3199	rBV	1038043	1603264	65.84%	8.858%
92	11.548	3259	3268	3280	rBV8	3262	6186	0.25%	0.034%
93	11.632	3282	3294	3319	rVV	1157177	1815037	74.54%	10.028%
94	12.165	3457	3460	3464	rVB2	959	397	0.02%	0.002%
95	12.374	3521	3525	3529	rBV2	935	808	0.03%	0.004%
96	12.493	3558	3562	3564	rBV3	1254	1005	0.04%	0.006%
97	12.783	3650	3652	3654	rVB2	952	398	0.02%	0.002%
98	12.802	3654	3658	3661	rBV3	653	540	0.02%	0.003%




Sum of corrected areas: 18100312

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020841.D
Acq On : 01 Apr 2021 15:51
Operator : SY/MD
Sample : M1879-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW199

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

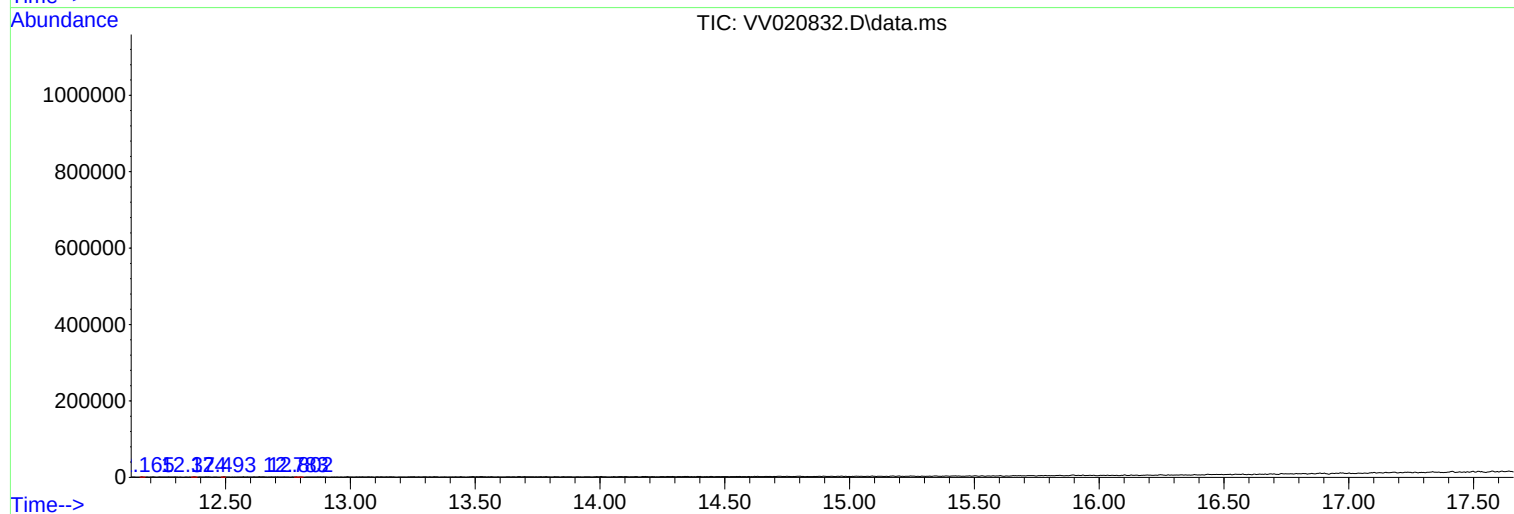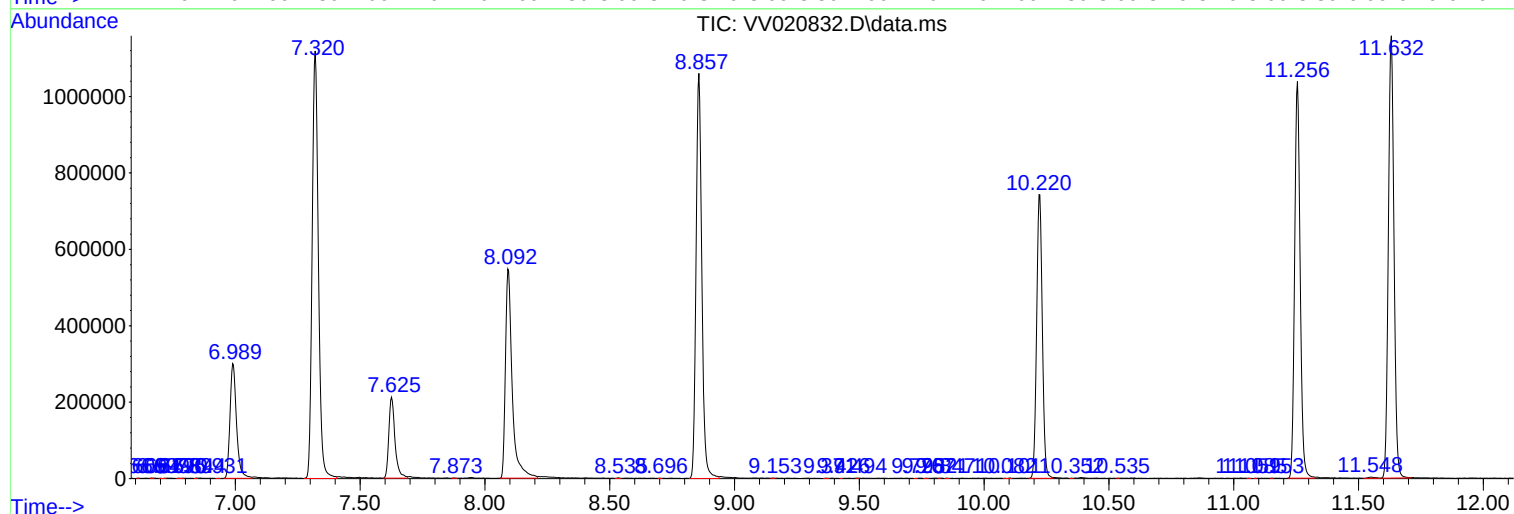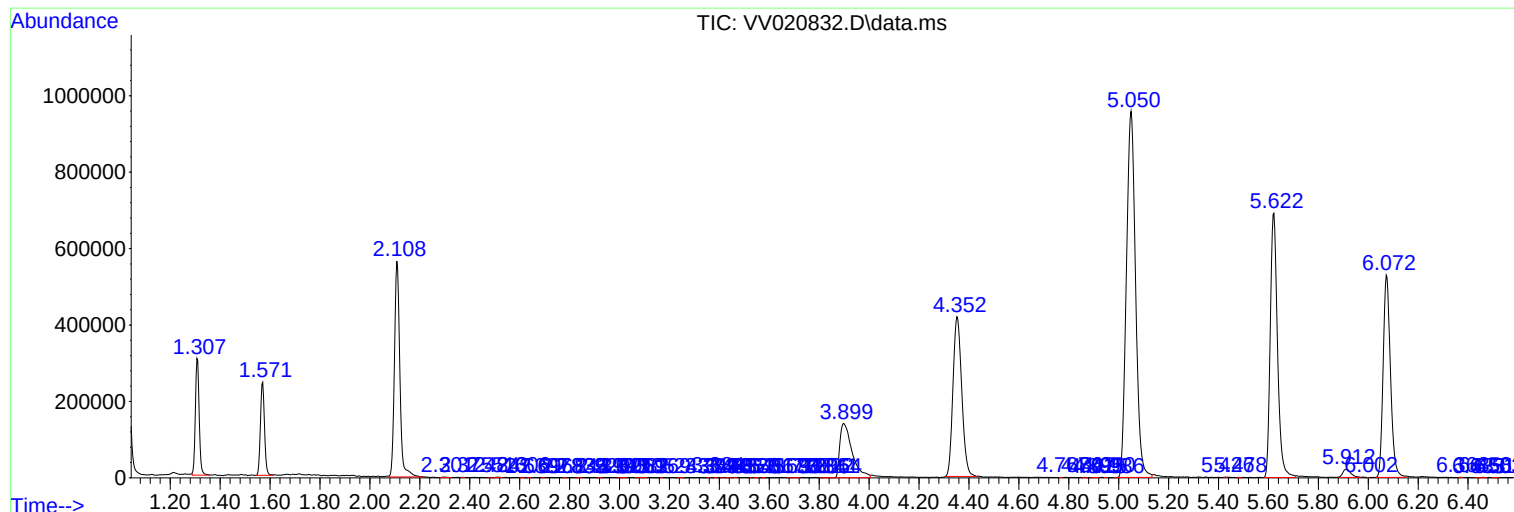

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020841.D
Acq On : 01 Apr 2021 15:51
Operator : SY/MD
Sample : M1879-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW199

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020841.D
Acq On : 01 Apr 2021 15:51
Operator : SY/MD
Sample : M1879-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW199

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
