

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020849.D
 Acq On : 01 Apr 2021 19:01
 Operator : SY/MD
 Sample : M1879-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020840.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	95	rVB2	534948	560388	23.28%	2.823%
2	1.571	158	165	177	rVB	237653	267449	11.11%	1.347%
3	2.108	322	332	359	rVB	536515	806094	33.49%	4.061%
4	2.236	370	372	374	rBV	758	288	0.01%	0.001%
5	2.468	442	444	446	rBV	672	432	0.02%	0.002%
6	2.564	471	474	476	rBV3	605	423	0.02%	0.002%
7	2.622	490	492	496	rVB2	514	326	0.01%	0.002%
8	2.683	508	511	514	rBV3	669	519	0.02%	0.003%
9	2.828	553	556	561	rVB5	548	551	0.02%	0.003%
10	2.886	571	574	580	rVB2	518	320	0.01%	0.002%
11	3.076	626	633	635	rBV2	676	694	0.03%	0.003%
12	3.201	659	672	682	rBV4	4313	9408	0.39%	0.047%
13	3.239	682	684	690	rVB4	1059	852	0.04%	0.004%
14	3.275	690	695	697	rBV2	429	368	0.02%	0.002%
15	3.291	697	700	704	rVB2	743	460	0.02%	0.002%
16	3.333	709	713	716	rBV2	482	432	0.02%	0.002%
17	3.420	736	740	742	rBV3	635	560	0.02%	0.003%
18	3.445	746	748	752	rVB	866	357	0.01%	0.002%
19	3.487	758	761	763	rBV2	570	359	0.01%	0.002%
20	3.590	789	793	795	rBV3	552	311	0.01%	0.002%
21	3.625	802	804	807	rBV2	516	274	0.01%	0.001%
22	3.667	812	817	819	rBV2	636	370	0.02%	0.002%
23	3.731	835	837	842	rBV2	367	290	0.01%	0.001%
24	3.793	852	856	858	rBV2	473	282	0.01%	0.001%
25	3.809	858	861	862	rBV2	817	445	0.02%	0.002%
26	3.911	877	893	921	rBV3	496874	1412256	58.68%	7.114%
27	4.352	1013	1030	1056	rBV	423821	1038299	43.14%	5.230%
28	4.580	1098	1101	1105	rBV4	992	825	0.03%	0.004%
29	4.783	1159	1164	1172	rBV4	800	963	0.04%	0.005%
30	4.889	1194	1197	1200	rBV3	825	489	0.02%	0.002%
31	4.915	1202	1205	1207	rVV2	818	378	0.02%	0.002%
32	5.050	1229	1247	1275	rBV2	934093	2406688	100.00%	12.124%
33	5.464	1374	1376	1380	rVB3	965	471	0.02%	0.002%
34	5.497	1383	1386	1388	rBV3	623	421	0.02%	0.002%
35	5.526	1392	1395	1397	rVB4	865	401	0.02%	0.002%
36	5.548	1400	1402	1407	rVB3	551	398	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020849.D
 Acq On : 01 Apr 2021 19:01
 Operator : SY/MD
 Sample : M1879-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.622	1410	1425	1451	rBV	792668	1611350	66.95%	8.117%
38	5.911	1502	1515	1530	rBV4	17677	37272	1.55%	0.188%
39	6.024	1546	1550	1551	rBV2	586	396	0.02%	0.002%
40	6.072	1552	1565	1587	rBV	515461	1042365	43.31%	5.251%
41	6.339	1646	1648	1650	rBV3	664	281	0.01%	0.001%
42	6.439	1676	1679	1682	rBV3	557	402	0.02%	0.002%
43	6.580	1721	1723	1726	rBV3	534	399	0.02%	0.002%
44	6.616	1731	1734	1738	rBV2	651	539	0.02%	0.003%
45	6.654	1743	1746	1750	rBV5	953	1002	0.04%	0.005%
46	6.693	1755	1758	1759	rBV	908	495	0.02%	0.002%
47	6.757	1771	1778	1779	rBV4	1175	977	0.04%	0.005%
48	6.767	1779	1781	1783	rVB	904	399	0.02%	0.002%
49	6.783	1783	1786	1788	rBV3	900	555	0.02%	0.003%
50	6.808	1792	1794	1797	rBV3	447	333	0.01%	0.002%
51	6.882	1812	1817	1820	rBV2	661	659	0.03%	0.003%
52	6.989	1839	1850	1873	rBV	294120	527114	21.90%	2.655%
53	7.185	1909	1911	1914	rBV3	813	643	0.03%	0.003%
54	7.320	1941	1953	1984	rBV	1102312	1921014	79.82%	9.677%
55	7.625	2038	2048	2068	rBV	207627	359325	14.93%	1.810%
56	8.011	2163	2168	2172	rVB5	943	745	0.03%	0.004%
57	8.040	2172	2177	2179	rBV4	804	757	0.03%	0.004%
58	8.095	2183	2194	2221	rBV	539780	999523	41.53%	5.035%
59	8.535	2329	2331	2333	rBV	624	261	0.01%	0.001%
60	8.551	2334	2336	2338	rVB3	713	288	0.01%	0.001%
61	8.587	2344	2347	2354	rVB4	868	761	0.03%	0.004%
62	8.625	2356	2359	2364	rVB4	725	669	0.03%	0.003%
63	8.702	2380	2383	2386	rBV5	1304	868	0.04%	0.004%
64	8.773	2401	2405	2413	rVB3	1175	1214	0.05%	0.006%
65	8.857	2419	2431	2454	rBV	1205474	1949338	81.00%	9.820%
66	9.371	2589	2591	2596	rVB3	855	564	0.02%	0.003%
67	9.468	2619	2621	2624	rVB	809	421	0.02%	0.002%
68	9.506	2625	2633	2636	rBV3	711	833	0.03%	0.004%
69	9.532	2636	2641	2645	rBV2	883	929	0.04%	0.005%
70	9.554	2646	2648	2650	rVB	1048	351	0.01%	0.002%
71	9.574	2650	2654	2658	rBV4	1408	1254	0.05%	0.006%
72	9.654	2677	2679	2682	rBV3	438	302	0.01%	0.002%
73	9.882	2746	2750	2752	rBV3	644	446	0.02%	0.002%
74	10.027	2790	2795	2806	rVB6	4329	6309	0.26%	0.032%
75	10.220	2842	2855	2874	rBV	747994	1174270	48.79%	5.915%
76	10.339	2889	2892	2896	rBV3	903	789	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020849.D
 Acq On : 01 Apr 2021 19:01
 Operator : SY/MD
 Sample : M1879-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.381	2901	2905	2906	rBV3	1641	1080	0.04%	0.005%
78	10.451	2925	2927	2930	rVB2	557	285	0.01%	0.001%
79	10.535	2951	2953	2957	rVB2	695	309	0.01%	0.002%
80	10.696	3001	3003	3006	rVB2	896	485	0.02%	0.002%
81	10.750	3017	3020	3023	rVB3	742	390	0.02%	0.002%
82	10.847	3046	3050	3052	rBV3	849	666	0.03%	0.003%
83	10.876	3057	3059	3064	rVV3	1346	1008	0.04%	0.005%
84	11.185	3153	3155	3160	rVB3	672	410	0.02%	0.002%
85	11.255	3164	3177	3202	rBV	1214520	1877408	78.01%	9.458%
86	11.545	3258	3267	3268	rBV5	3791	4441	0.18%	0.022%
87	11.631	3281	3294	3312	rBV	1153599	1797652	74.69%	9.056%
88	11.959	3394	3396	3397	rBV	803	351	0.01%	0.002%
89	11.988	3402	3405	3409	rVV2	882	568	0.02%	0.003%
90	12.210	3472	3474	3477	rBV2	769	534	0.02%	0.003%
91	12.239	3480	3483	3485	rVV3	856	494	0.02%	0.002%
92	12.291	3496	3499	3502	rVB2	986	515	0.02%	0.003%
93	12.323	3508	3509	3511	rBV	643	293	0.01%	0.001%
94	12.477	3553	3557	3561	rBV3	796	808	0.03%	0.004%
95	12.612	3598	3599	3603	rVB	657	331	0.01%	0.002%
96	12.641	3606	3608	3611	rBV3	829	578	0.02%	0.003%
97	12.699	3623	3626	3630	rVB2	733	624	0.03%	0.003%
98	12.776	3648	3650	3653	rBV	687	338	0.01%	0.002%
99	12.799	3653	3657	3658	rBV2	780	435	0.02%	0.002%
100	14.033	4038	4041	4043	rBV2	1237	731	0.03%	0.004%




Sum of corrected areas: 19850987

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020849.D
Acq On : 01 Apr 2021 19:01
Operator : SY/MD
Sample : M1879-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

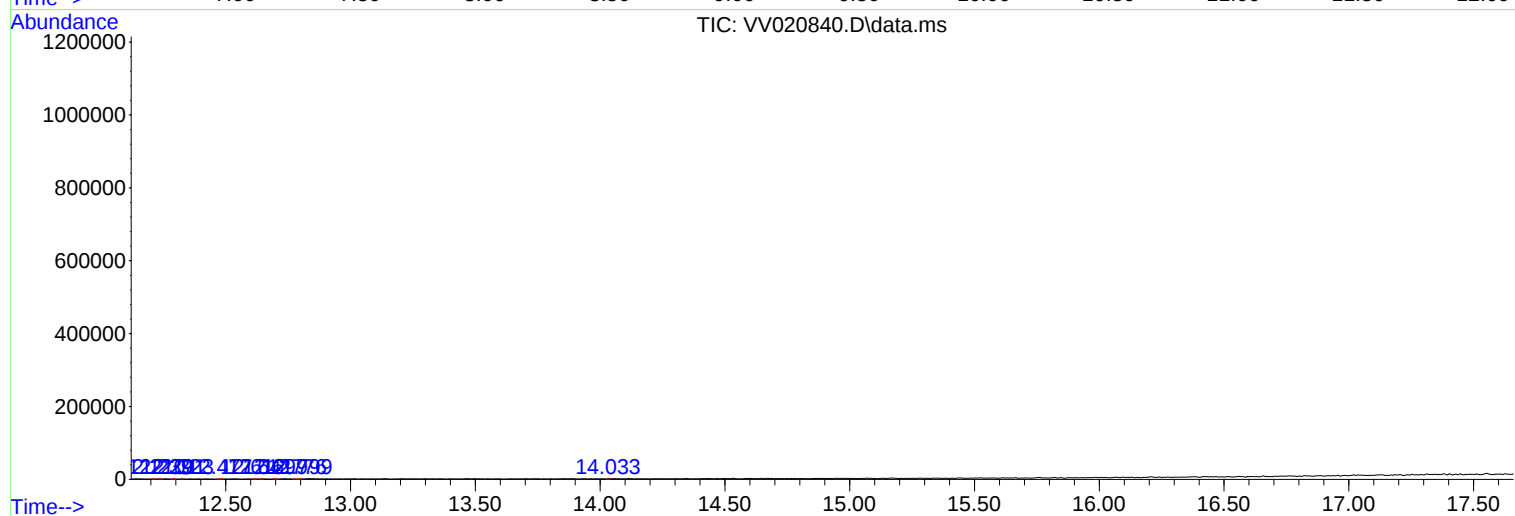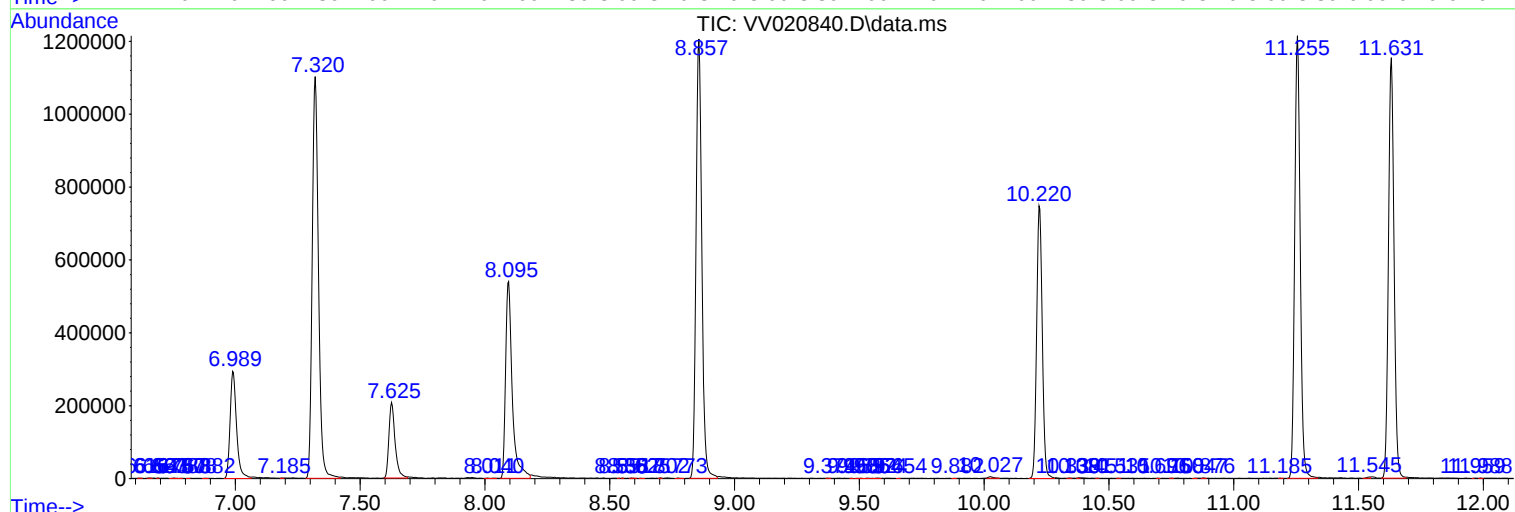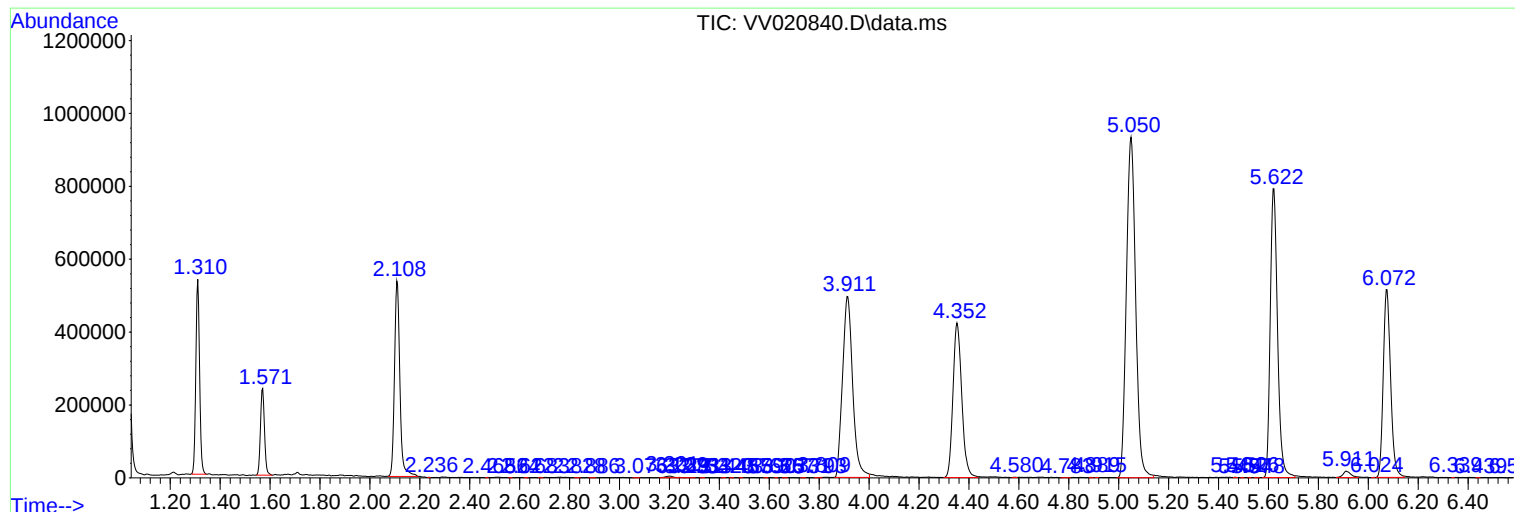

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020849.D
Acq On : 01 Apr 2021 19:01
Operator : SY/MD
Sample : M1879-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020849.D
Acq On : 01 Apr 2021 19:01
Operator : SY/MD
Sample : M1879-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
