

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020851.D
 Acq On : 01 Apr 2021 19:49
 Operator : SY/MD
 Sample : M1879-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1C3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020842.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	77	84	97	rVB2	458607	486693	19.30%	2.231%
2	1.571	158	165	178	rVB	245461	282043	11.19%	1.293%
3	2.108	323	332	361	rVB	567974	848069	33.64%	3.888%
4	2.429	426	432	434	rBV5	1219	1198	0.05%	0.005%
5	2.867	565	568	572	rBV3	902	631	0.03%	0.003%
6	3.002	607	610	612	rVB	951	528	0.02%	0.002%
7	3.024	612	617	622	rBV4	947	952	0.04%	0.004%
8	3.150	652	656	658	rBV3	806	654	0.03%	0.003%
9	3.182	664	666	671	rVB3	701	474	0.02%	0.002%
10	3.204	671	673	676	rBV	605	250	0.01%	0.001%
11	3.246	684	686	690	rBV3	555	372	0.01%	0.002%
12	3.285	695	698	702	rBV2	681	606	0.02%	0.003%
13	3.307	702	705	706	rBV	615	318	0.01%	0.001%
14	3.352	715	719	722	rVB3	1062	736	0.03%	0.003%
15	3.484	758	760	762	rVB2	796	304	0.01%	0.001%
16	3.510	762	768	771	rBV3	844	1047	0.04%	0.005%
17	3.581	787	790	791	rBV3	600	323	0.01%	0.001%
18	3.629	801	805	809	rBV4	1041	1078	0.04%	0.005%
19	3.674	817	819	823	rBV2	591	334	0.01%	0.002%
20	3.751	836	843	845	rBV3	740	763	0.03%	0.003%
21	3.783	852	853	855	rBV2	394	185	0.01%	0.001%
22	3.799	857	858	859	rBV	388	103	0.00%	0.000%
23	3.835	866	869	872	rBV2	517	347	0.01%	0.002%
24	3.915	878	894	926	rBV3	854908	2281189	90.48%	10.457%
25	4.352	1015	1030	1060	rVB	439546	1077833	42.75%	4.941%
26	4.915	1203	1205	1206	rBV	533	188	0.01%	0.001%
27	4.986	1224	1227	1229	rBV4	816	497	0.02%	0.002%
28	5.050	1230	1247	1275	rBV2	989544	2521086	100.00%	11.557%
29	5.339	1335	1337	1339	rBV2	868	431	0.02%	0.002%
30	5.619	1410	1424	1447	rBV	830703	1659655	65.83%	7.608%
31	5.918	1504	1517	1539	rBV3	242520	505582	20.05%	2.318%
32	6.076	1553	1566	1594	rVB	534795	1094880	43.43%	5.019%
33	6.484	1690	1693	1697	rBV4	520	418	0.02%	0.002%
34	6.506	1697	1700	1703	rBV2	819	509	0.02%	0.002%
35	6.545	1710	1712	1714	rBV2	502	250	0.01%	0.001%
36	6.596	1723	1728	1730	rBV3	755	537	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020851.D
 Acq On : 01 Apr 2021 19:49
 Operator : SY/MD
 Sample : M1879-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1C3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	6.609	1730	1732	1734	rVB2	502	150	0.01%	0.001%
38	6.748	1773	1775	1778	rVB2	1365	673	0.03%	0.003%
39	6.764	1778	1780	1783	rBV2	906	652	0.03%	0.003%
40	6.809	1790	1794	1800	rBV5	869	992	0.04%	0.005%
41	6.857	1807	1809	1811	rBV2	676	423	0.02%	0.002%
42	6.931	1829	1832	1834	rBV2	693	452	0.02%	0.002%
43	6.989	1839	1850	1874	rBV	308060	556768	22.08%	2.552%
44	7.320	1941	1953	1971	rBV	1168138	1999781	79.32%	9.167%
45	7.625	2038	2048	2065	rBV	219774	383899	15.23%	1.760%
46	7.870	2122	2124	2125	rBV2	588	247	0.01%	0.001%
47	7.989	2159	2161	2167	rVB5	1341	897	0.04%	0.004%
48	8.092	2183	2193	2230	rBV	554303	1064333	42.22%	4.879%
49	8.609	2350	2354	2357	rBV3	648	570	0.02%	0.003%
50	8.789	2403	2410	2414	rBV6	1227	1385	0.05%	0.006%
51	8.857	2419	2431	2453	rBV	1242807	1999742	79.32%	9.167%
52	9.133	2514	2517	2523	rBV6	1544	1359	0.05%	0.006%
53	9.394	2595	2598	2600	rBV2	851	580	0.02%	0.003%
54	9.432	2608	2610	2612	rBV	635	323	0.01%	0.001%
55	9.458	2617	2618	2621	rBV2	592	403	0.02%	0.002%
56	9.506	2630	2633	2636	rBV2	753	442	0.02%	0.002%
57	9.577	2653	2655	2659	rVB2	795	394	0.02%	0.002%
58	9.600	2659	2662	2664	rBV3	809	496	0.02%	0.002%
59	9.680	2683	2687	2690	rBV5	691	678	0.03%	0.003%
60	9.844	2736	2738	2741	rBV	583	450	0.02%	0.002%
61	10.014	2789	2791	2793	rBV3	327	121	0.00%	0.001%
62	10.220	2842	2855	2877	rBV	776319	1239274	49.16%	5.681%
63	10.387	2895	2907	2910	rBV8	3384	4835	0.19%	0.022%
64	10.513	2944	2946	2951	rBV3	953	818	0.03%	0.004%
65	10.535	2951	2953	2955	rVB2	1155	397	0.02%	0.002%
66	10.731	3011	3014	3016	rVB2	831	414	0.02%	0.002%
67	10.825	3040	3043	3046	rVB5	844	513	0.02%	0.002%
68	10.841	3046	3048	3050	rBV2	855	470	0.02%	0.002%
69	10.927	3072	3075	3081	rBV3	1065	942	0.04%	0.004%
70	11.008	3098	3100	3103	rBV2	615	493	0.02%	0.002%
71	11.034	3106	3108	3111	rVB2	854	486	0.02%	0.002%
72	11.255	3165	3177	3201	rBV	1238623	1897276	75.26%	8.697%
73	11.535	3262	3264	3265	rBV2	952	443	0.02%	0.002%
74	11.632	3280	3294	3318	rBV	1189036	1874966	74.37%	8.595%
75	12.127	3444	3448	3453	rBV4	1315	1410	0.06%	0.006%
76	12.149	3453	3455	3456	rVV	550	143	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020851.D
Acq On : 01 Apr 2021 19:49
Operator : SY/MD
Sample : M1879-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Title : VOC Analysis

77	12.207	3470	3473	3474	rBV	624	372	0.01%	0.002%
78	12.407	3533	3535	3538	rBV3	1143	610	0.02%	0.003%
79	12.484	3557	3559	3563	rBV3	704	564	0.02%	0.003%
80	12.931	3695	3698	3699	rBV	699	330	0.01%	0.002%
81	13.046	3731	3734	3737	rBV2	775	412	0.02%	0.002%
82	13.191	3777	3779	3782	rVB3	1450	790	0.03%	0.004%
83	14.204	4089	4094	4096	rBV3	1170	1039	0.04%	0.005%




Sum of corrected areas: 21814270

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020851.D
Acq On : 01 Apr 2021 19:49
Operator : SY/MD
Sample : M1879-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

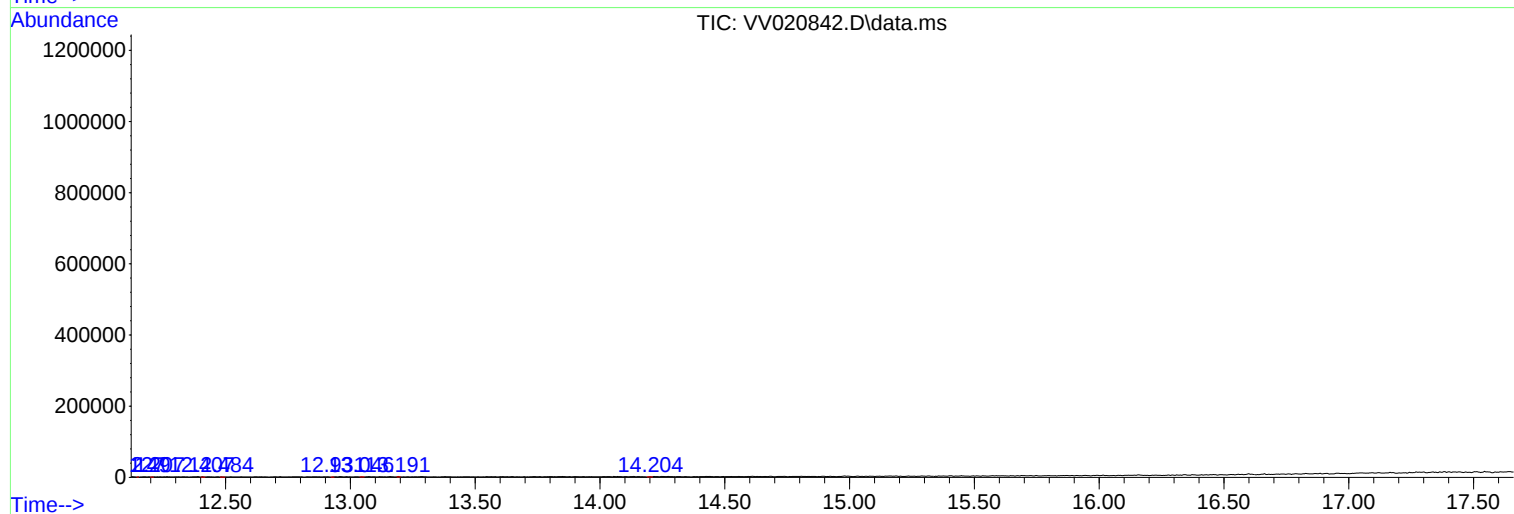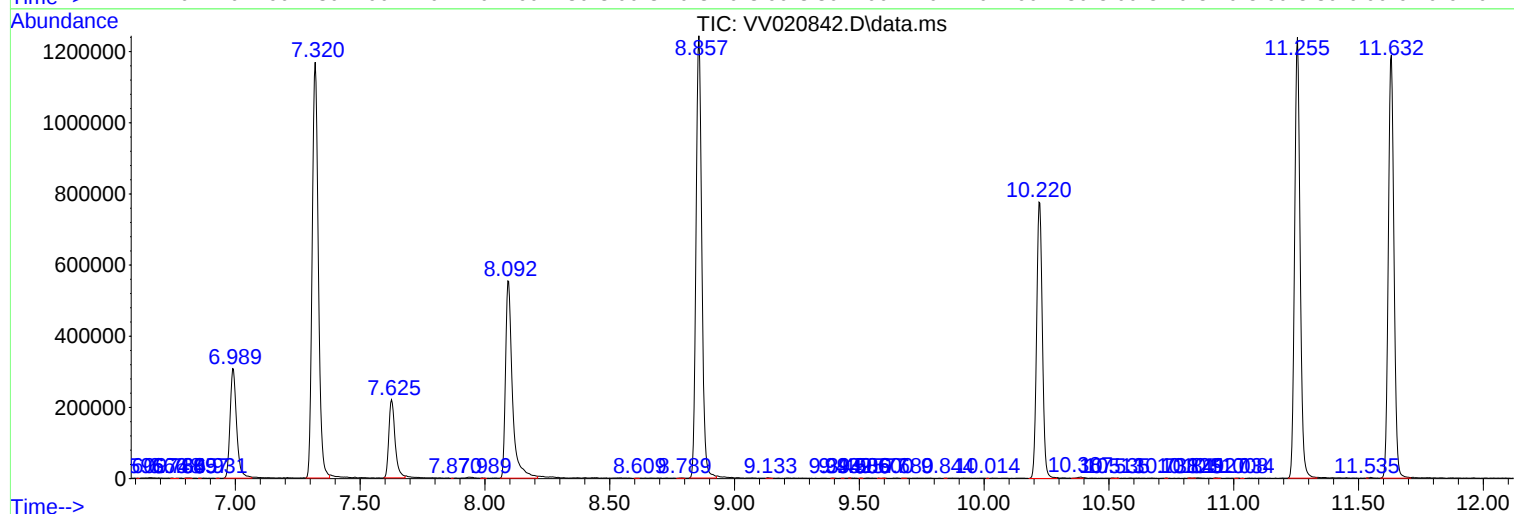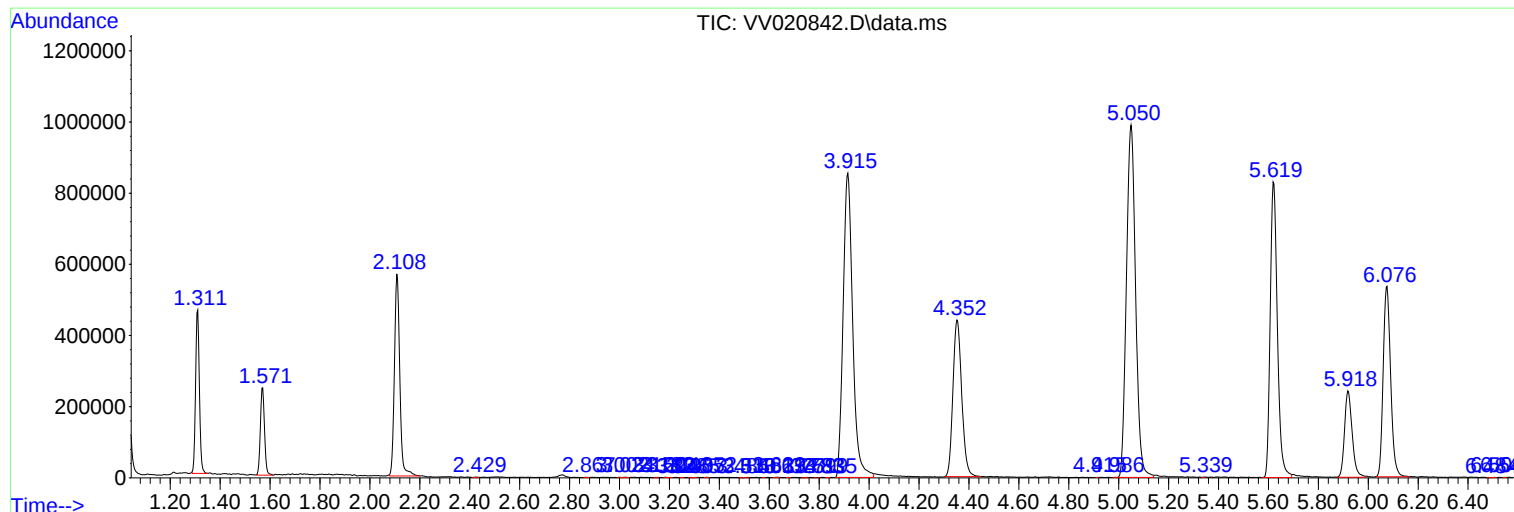

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020851.D
Acq On : 01 Apr 2021 19:49
Operator : SY/MD
Sample : M1879-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020851.D
Acq On : 01 Apr 2021 19:49
Operator : SY/MD
Sample : M1879-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
