

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020854.D
 Acq On : 01 Apr 2021 21:55
 Operator : SY/MD
 Sample : VV0401WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK99

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020845.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	313785	314558	12.04%	1.617%
2	1.571	157	165	176	rBV	266161	300283	11.49%	1.544%
3	2.108	323	332	348	rBV	602409	870585	33.31%	4.477%
4	2.433	429	433	435	rBV3	568	536	0.02%	0.003%
5	2.699	514	516	518	rBV2	447	238	0.01%	0.001%
6	2.738	526	528	530	rBV2	828	340	0.01%	0.002%
7	2.831	555	557	559	rVB	710	289	0.01%	0.001%
8	2.966	597	599	601	rVB	594	306	0.01%	0.002%
9	3.066	624	630	632	rBV2	653	516	0.02%	0.003%
10	3.130	645	650	653	rBV3	931	778	0.03%	0.004%
11	3.223	678	679	682	rVV2	632	252	0.01%	0.001%
12	3.249	686	687	691	rVB3	448	254	0.01%	0.001%
13	3.310	702	706	708	rBV2	346	255	0.01%	0.001%
14	3.326	708	711	716	rVB2	428	312	0.01%	0.002%
15	3.400	731	734	736	rVB	606	300	0.01%	0.002%
16	3.416	736	739	743	rBV3	537	381	0.01%	0.002%
17	3.436	743	745	749	rVV2	770	453	0.02%	0.002%
18	3.458	749	752	754	rVV2	725	546	0.02%	0.003%
19	3.484	758	760	765	rVB2	828	487	0.02%	0.003%
20	3.661	812	815	816	rBV2	408	261	0.01%	0.001%
21	3.796	854	857	861	rBV3	550	372	0.01%	0.002%
22	3.828	864	867	869	rBV2	502	259	0.01%	0.001%
23	3.860	872	877	878	rBV2	420	244	0.01%	0.001%
24	3.908	878	892	921	rBV2	164044	575138	22.01%	2.957%
25	4.352	1014	1030	1054	rBV	464405	1126073	43.09%	5.790%
26	4.780	1160	1163	1165	rVB2	1036	589	0.02%	0.003%
27	4.812	1170	1173	1175	rBV	828	435	0.02%	0.002%
28	4.857	1185	1187	1190	rBV4	783	481	0.02%	0.002%
29	5.050	1229	1247	1278	rBV2	1029677	2613472	100.00%	13.439%
30	5.558	1403	1405	1407	rBV3	591	353	0.01%	0.002%
31	5.622	1412	1425	1448	rBV	759334	1516830	58.04%	7.800%
32	5.854	1495	1497	1501	rBV4	644	343	0.01%	0.002%
33	5.915	1506	1516	1535	rVB5	35951	82594	3.16%	0.425%
34	6.075	1552	1566	1595	rBV	551414	1132088	43.32%	5.821%
35	6.294	1632	1634	1635	rBV2	836	372	0.01%	0.002%
36	6.304	1635	1637	1645	rVB4	1809	1591	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020854.D
 Acq On : 01 Apr 2021 21:55
 Operator : SY/MD
 Sample : VV0401WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK99

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	6.384	1658	1662	1664	rBV2	779	679	0.03%	0.003%
38	6.429	1674	1676	1680	rVB3	881	413	0.02%	0.002%
39	6.474	1687	1690	1692	rBV	658	308	0.01%	0.002%
40	6.577	1720	1722	1724	rBV	537	318	0.01%	0.002%
41	6.924	1825	1830	1831	rBV	695	394	0.02%	0.002%
42	6.989	1839	1850	1874	rBV2	309538	566059	21.66%	2.911%
43	7.320	1941	1953	1977	rBV	1197477	2063819	78.97%	10.612%
44	7.625	2035	2048	2070	rBV	221619	384162	14.70%	1.975%
45	7.882	2126	2128	2132	rBV3	703	409	0.02%	0.002%
46	8.050	2177	2180	2182	rVB2	891	485	0.02%	0.002%
47	8.095	2182	2194	2230	rBV	612881	1171822	44.84%	6.026%
48	8.500	2319	2320	2322	rBV	623	250	0.01%	0.001%
49	8.754	2395	2399	2400	rBV3	611	324	0.01%	0.002%
50	8.808	2414	2416	2418	rBV	631	359	0.01%	0.002%
51	8.857	2419	2431	2457	rVV	1134762	1843863	70.55%	9.481%
52	9.050	2488	2491	2495	rVB5	1114	737	0.03%	0.004%
53	9.069	2495	2497	2499	rVB3	715	248	0.01%	0.001%
54	9.120	2511	2513	2515	rBV3	473	247	0.01%	0.001%
55	9.146	2519	2521	2527	rVB3	1305	936	0.04%	0.005%
56	9.172	2527	2529	2532	rBV2	910	661	0.03%	0.003%
57	9.297	2566	2568	2570	rBV3	726	351	0.01%	0.002%
58	9.342	2580	2582	2584	rVB2	666	261	0.01%	0.001%
59	9.355	2584	2586	2592	rBV4	627	516	0.02%	0.003%
60	9.381	2592	2594	2599	rVV3	609	479	0.02%	0.002%
61	9.464	2618	2620	2623	rBV	747	481	0.02%	0.002%
62	9.561	2642	2650	2653	rBV4	1045	1196	0.05%	0.006%
63	9.612	2662	2666	2670	rBV5	831	784	0.03%	0.004%
64	9.632	2670	2672	2674	rVB2	920	439	0.02%	0.002%
65	9.738	2701	2705	2708	rBV	460	398	0.02%	0.002%
66	9.789	2718	2721	2723	rBV2	641	405	0.02%	0.002%
67	9.966	2774	2776	2780	rBV2	474	309	0.01%	0.002%
68	10.046	2798	2801	2803	rBV3	936	565	0.02%	0.003%
69	10.220	2843	2855	2881	rBV	799429	1271525	48.65%	6.538%
70	10.387	2905	2907	2912	rVB2	993	642	0.02%	0.003%
71	10.416	2912	2916	2919	rVB	581	483	0.02%	0.002%
72	10.435	2919	2922	2925	rBV	956	661	0.03%	0.003%
73	10.625	2977	2981	2984	rBV4	477	399	0.02%	0.002%
74	10.744	3015	3018	3021	rBV2	497	317	0.01%	0.002%
75	10.767	3024	3025	3028	rBV	617	340	0.01%	0.002%
76	10.844	3046	3049	3050	rBV	492	285	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020854.D
 Acq On : 01 Apr 2021 21:55
 Operator : SY/MD
 Sample : VV0401WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK99

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.857	3050	3053	3056	rVB2	1386	868	0.03%	0.004%
78	10.976	3083	3090	3093	rBV3	767	909	0.03%	0.005%
79	11.033	3105	3108	3112	rBV2	801	598	0.02%	0.003%
80	11.255	3165	3177	3200	rBV	1101205	1687014	64.55%	8.675%
81	11.493	3248	3251	3255	rBV	902	648	0.02%	0.003%
82	11.631	3282	3294	3312	rBV	1220345	1887047	72.20%	9.703%
83	11.950	3391	3393	3399	rVB6	1047	647	0.02%	0.003%
84	11.988	3403	3405	3406	rBV	572	237	0.01%	0.001%
85	12.059	3424	3427	3430	rVB3	1043	619	0.02%	0.003%
86	12.168	3458	3461	3465	rBV2	1055	697	0.03%	0.004%
87	12.249	3484	3486	3488	rBV	611	306	0.01%	0.002%
88	12.474	3552	3556	3558	rBV3	688	643	0.02%	0.003%
89	12.548	3577	3579	3581	rBV2	620	258	0.01%	0.001%
90	12.603	3594	3596	3599	rVB2	1012	398	0.02%	0.002%
91	12.773	3647	3649	3651	rBV2	546	339	0.01%	0.002%
92	12.818	3660	3663	3666	rBV2	619	446	0.02%	0.002%
93	12.866	3676	3678	3681	rBV3	915	613	0.02%	0.003%
94	12.921	3693	3695	3699	rBV3	852	533	0.02%	0.003%
95	13.139	3761	3763	3767	rBV4	778	556	0.02%	0.003%
96	13.217	3782	3787	3789	rBV3	716	708	0.03%	0.004%
97	13.323	3818	3820	3822	rBV2	1125	540	0.02%	0.003%
98	13.374	3833	3836	3837	rBV	711	394	0.02%	0.002%
99	13.413	3844	3848	3850	rBV2	1040	728	0.03%	0.004%
100	13.921	4001	4006	4008	rBV3	1318	1306	0.05%	0.007%




Sum of corrected areas: 19447545

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020854.D
Acq On : 01 Apr 2021 21:55
Operator : SY/MD
Sample : VV0401WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

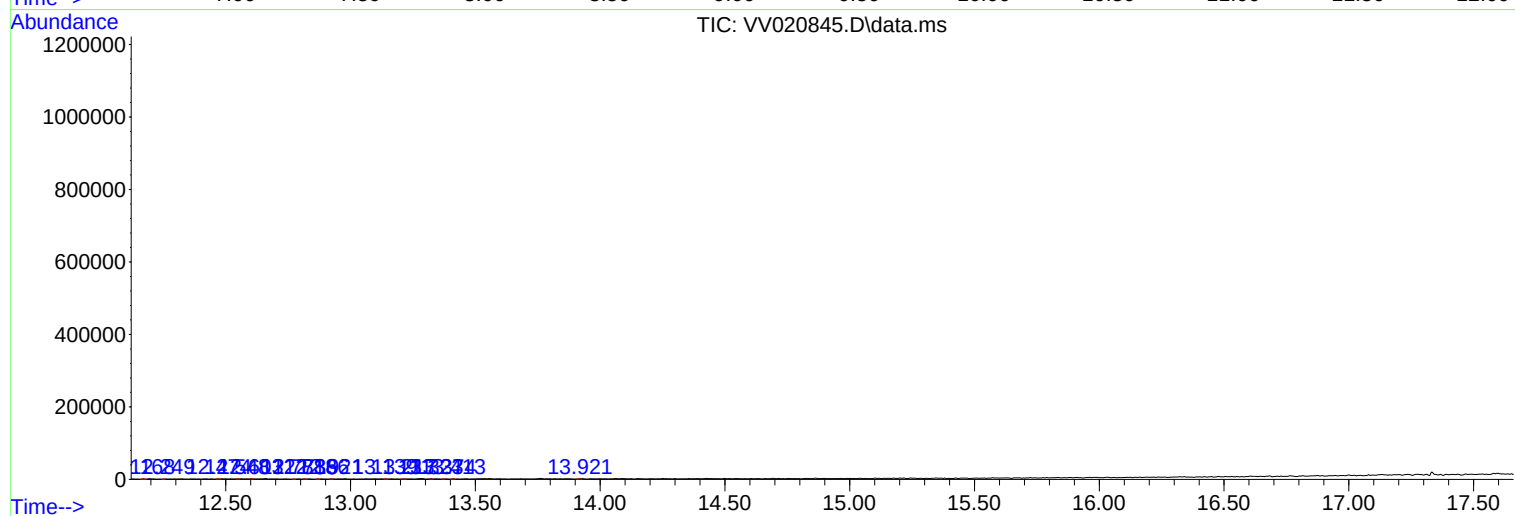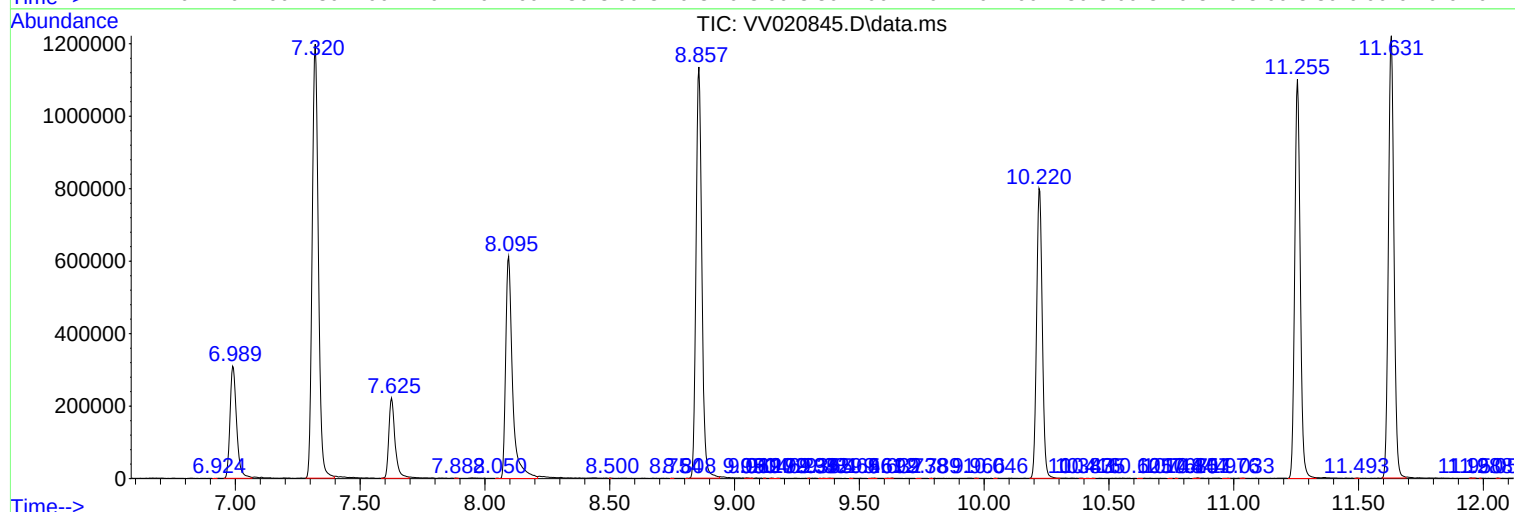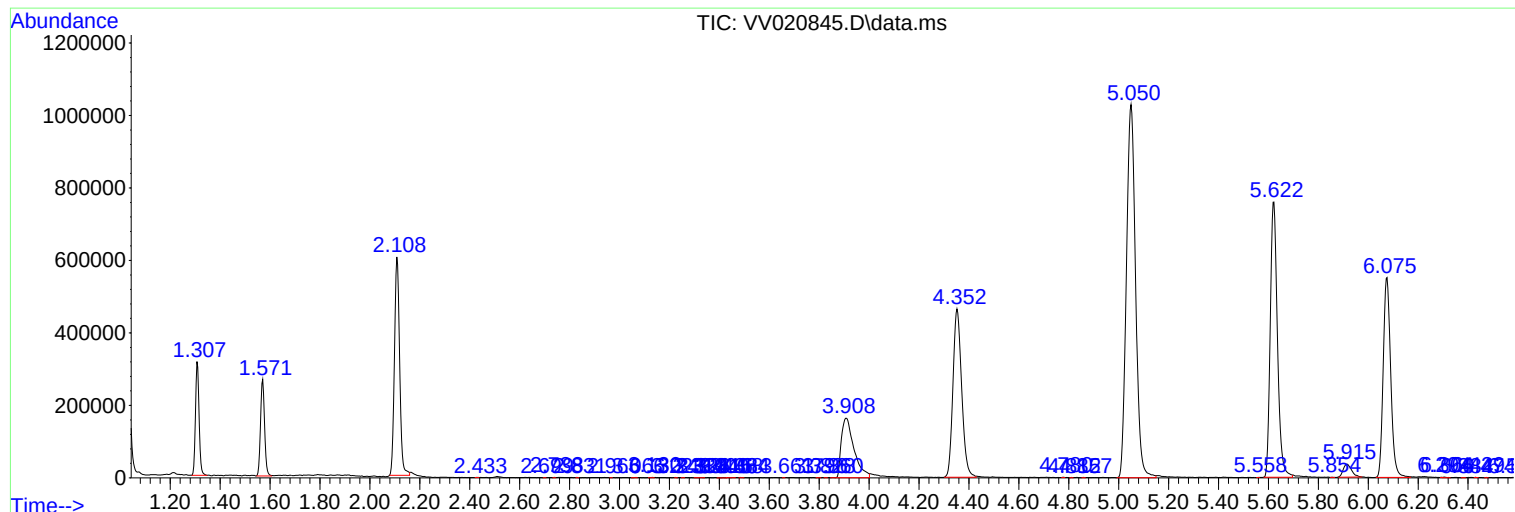

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020854.D
Acq On : 01 Apr 2021 21:55
Operator : SY/MD
Sample : VV0401WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020854.D
Acq On : 01 Apr 2021 21:55
Operator : SY/MD
Sample : VV0401WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
