

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW040121\
 Data File : VW020856.D
 Acq On : 01 Apr 2021 22:46
 Operator : SY/MD
 Sample : M1845-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1A4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VW020847.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	260184	264412	11.46%	1.527%
2	1.571	158	165	174	rVB	224215	247394	10.73%	1.429%
3	2.108	322	332	356	rVB	519060	763231	33.09%	4.408%
4	2.259	376	379	382	rBV4	809	477	0.02%	0.003%
5	2.285	382	387	388	rBV3	757	589	0.03%	0.003%
6	2.381	413	417	420	rBV4	561	399	0.02%	0.002%
7	2.445	434	437	438	rBV	807	348	0.02%	0.002%
8	2.471	442	445	448	rBV3	477	364	0.02%	0.002%
9	2.677	506	509	514	rVB2	845	707	0.03%	0.004%
10	2.783	539	542	544	rBV	477	339	0.01%	0.002%
11	2.805	545	549	551	rVB2	811	518	0.02%	0.003%
12	2.998	607	609	612	rVB3	776	326	0.01%	0.002%
13	3.021	612	616	619	rBV3	492	367	0.02%	0.002%
14	3.114	641	645	646	rBV2	441	283	0.01%	0.002%
15	3.297	699	702	705	rBV2	499	381	0.02%	0.002%
16	3.326	707	711	714	rVV	461	285	0.01%	0.002%
17	3.378	724	727	733	rBV2	541	677	0.03%	0.004%
18	3.452	747	750	754	rBV3	523	302	0.01%	0.002%
19	3.616	797	801	804	rVB3	537	448	0.02%	0.003%
20	3.658	812	814	819	rBV3	516	362	0.02%	0.002%
21	3.693	819	825	827	rBV2	474	476	0.02%	0.003%
22	3.815	861	863	867	rBV	463	320	0.01%	0.002%
23	3.902	877	890	918	rBV2	142177	479106	20.77%	2.767%
24	4.352	1014	1030	1056	rBV	406726	997034	43.22%	5.759%
25	4.574	1097	1099	1104	rBV5	963	729	0.03%	0.004%
26	4.786	1163	1165	1169	rBV3	714	392	0.02%	0.002%
27	4.805	1169	1171	1176	rVB4	931	635	0.03%	0.004%
28	4.854	1183	1186	1187	rBV4	530	267	0.01%	0.002%
29	4.931	1204	1210	1214	rVB5	968	779	0.03%	0.004%
30	4.950	1214	1216	1217	rBV	757	340	0.01%	0.002%
31	5.050	1230	1247	1275	rBV2	895491	2306642	100.00%	13.323%
32	5.391	1351	1353	1356	rBV3	887	420	0.02%	0.002%
33	5.445	1367	1370	1371	rBV3	711	351	0.02%	0.002%
34	5.465	1374	1376	1379	rVB2	634	308	0.01%	0.002%
35	5.487	1379	1383	1388	rBV4	958	1008	0.04%	0.006%
36	5.510	1388	1390	1394	rVV3	798	489	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW040121\
 Data File : VW020856.D
 Acq On : 01 Apr 2021 22:46
 Operator : SY/MD
 Sample : M1845-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1A4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.622	1412	1425	1460	rBV	694294	1416861	61.43%	8.183%
38	5.915	1506	1516	1536	rVB7	26960	64619	2.80%	0.373%
39	6.014	1542	1547	1550	rBV4	1039	941	0.04%	0.005%
40	6.072	1552	1565	1596	rVV	491199	1002997	43.48%	5.793%
41	6.317	1637	1641	1644	rVB2	900	675	0.03%	0.004%
42	6.333	1644	1646	1648	rBV	969	628	0.03%	0.004%
43	6.384	1660	1662	1663	rBV	656	272	0.01%	0.002%
44	6.538	1708	1710	1713	rVB2	736	368	0.02%	0.002%
45	6.612	1730	1733	1736	rVV	403	275	0.01%	0.002%
46	6.645	1741	1743	1745	rBV3	799	454	0.02%	0.003%
47	6.931	1830	1832	1836	rBV2	525	370	0.02%	0.002%
48	6.989	1839	1850	1875	rBV	266763	497617	21.57%	2.874%
49	7.320	1941	1953	1973	rBV	1053339	1804634	78.24%	10.423%
50	7.625	2037	2048	2070	rBV	196946	345372	14.97%	1.995%
51	7.899	2129	2133	2136	rBV4	787	659	0.03%	0.004%
52	7.915	2136	2138	2140	rVV	841	404	0.02%	0.002%
53	7.947	2140	2148	2155	rVV8	2667	4458	0.19%	0.026%
54	7.976	2155	2157	2163	rVB3	1605	1064	0.05%	0.006%
55	8.095	2183	2194	2227	rBV	510323	988247	42.84%	5.708%
56	8.670	2370	2373	2374	rBV2	554	329	0.01%	0.002%
57	8.715	2384	2387	2390	rVB3	697	361	0.02%	0.002%
58	8.763	2399	2402	2404	rBV2	556	372	0.02%	0.002%
59	8.779	2404	2407	2411	rBV3	709	631	0.03%	0.004%
60	8.857	2419	2431	2462	rBV	1047169	1713454	74.28%	9.896%
61	9.233	2545	2548	2552	rVB4	876	554	0.02%	0.003%
62	9.365	2587	2589	2593	rVB3	584	280	0.01%	0.002%
63	9.439	2608	2612	2617	rVB3	588	514	0.02%	0.003%
64	9.612	2663	2666	2668	rBV3	841	454	0.02%	0.003%
65	9.725	2697	2701	2703	rBV	523	478	0.02%	0.003%
66	9.815	2727	2729	2732	rBV2	563	275	0.01%	0.002%
67	9.831	2732	2734	2736	rVV	507	298	0.01%	0.002%
68	9.873	2745	2747	2752	rBV2	670	529	0.02%	0.003%
69	9.985	2778	2782	2783	rBV2	377	299	0.01%	0.002%
70	10.011	2786	2790	2792	rBV3	599	445	0.02%	0.003%
71	10.066	2805	2807	2810	rBV2	386	296	0.01%	0.002%
72	10.085	2810	2813	2816	rBV	508	381	0.02%	0.002%
73	10.140	2824	2830	2833	rBV3	583	604	0.03%	0.003%
74	10.223	2843	2856	2879	rBV	724182	1121594	48.62%	6.478%
75	10.307	2879	2882	2888	rVB3	1407	1339	0.06%	0.008%
76	10.371	2900	2902	2904	rBV	1097	588	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020856.D
 Acq On : 01 Apr 2021 22:46
 Operator : SY/MD
 Sample : M1845-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1A4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	10.525	2948	2950	2955	rVB2	715	391	0.02%	0.002%
78	10.551	2955	2958	2959	rBV2	705	424	0.02%	0.002%
79	10.770	3023	3026	3028	rVB2	620	337	0.01%	0.002%
80	10.786	3028	3031	3036	rBV4	871	1073	0.05%	0.006%
81	10.853	3047	3052	3053	rBV2	1165	706	0.03%	0.004%
82	10.892	3060	3064	3065	rBV	664	462	0.02%	0.003%
83	10.976	3088	3090	3095	rVB	675	443	0.02%	0.003%
84	11.004	3095	3099	3102	rBV3	825	575	0.02%	0.003%
85	11.197	3157	3159	3162	rVB2	632	348	0.02%	0.002%
86	11.255	3165	3177	3198	rBV	1013943	1564746	67.84%	9.038%
87	11.631	3281	3294	3316	rBV	1075683	1690347	73.28%	9.763%
88	11.985	3402	3404	3406	rBV	976	478	0.02%	0.003%
89	12.024	3414	3416	3420	rVB	575	366	0.02%	0.002%
90	12.072	3428	3431	3433	rBV2	809	427	0.02%	0.002%
91	12.188	3465	3467	3473	rBV4	835	755	0.03%	0.004%
92	12.287	3496	3498	3499	rBV4	609	266	0.01%	0.002%
93	12.387	3526	3529	3532	rBV2	634	543	0.02%	0.003%
94	12.435	3540	3544	3547	rBV3	1183	634	0.03%	0.004%
95	12.648	3607	3610	3611	rBV2	784	451	0.02%	0.003%
96	12.766	3643	3647	3649	rBV	721	615	0.03%	0.004%
97	12.808	3655	3660	3662	rBV3	631	581	0.03%	0.003%
98	12.918	3692	3694	3699	rVB3	1009	595	0.03%	0.003%
99	13.127	3756	3759	3762	rBV3	1193	992	0.04%	0.006%
100	13.274	3803	3805	3807	rBV3	1027	697	0.03%	0.004%




Sum of corrected areas: 17313747

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020856.D
Acq On : 01 Apr 2021 22:46
Operator : SY/MD
Sample : M1845-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1A4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

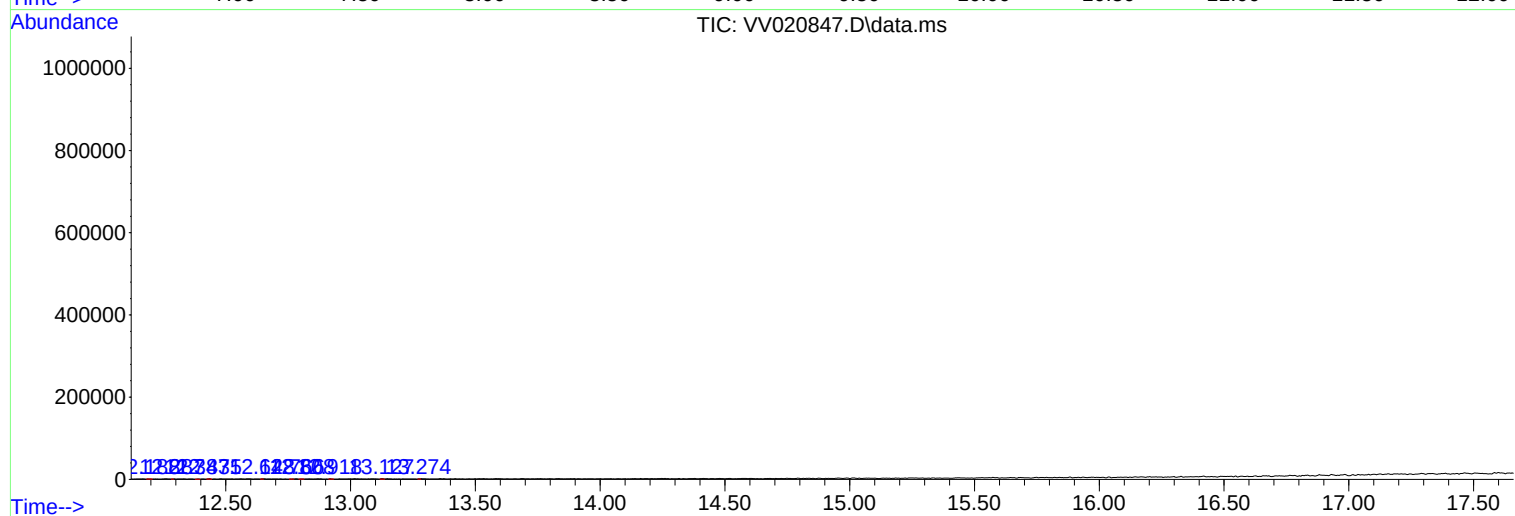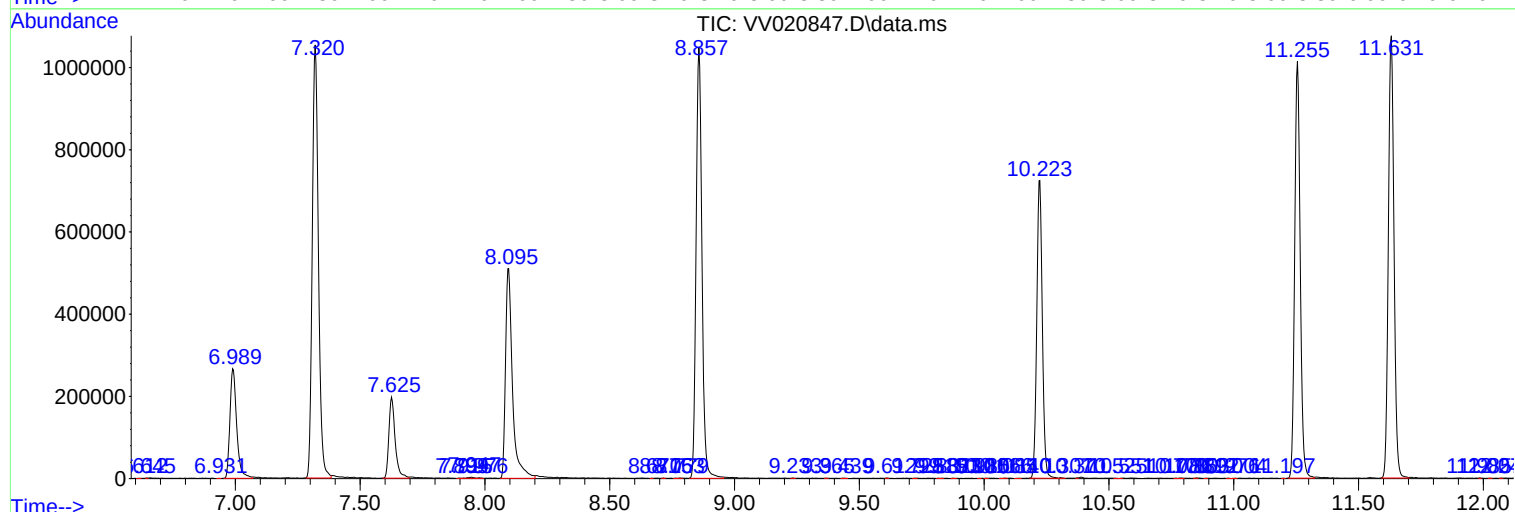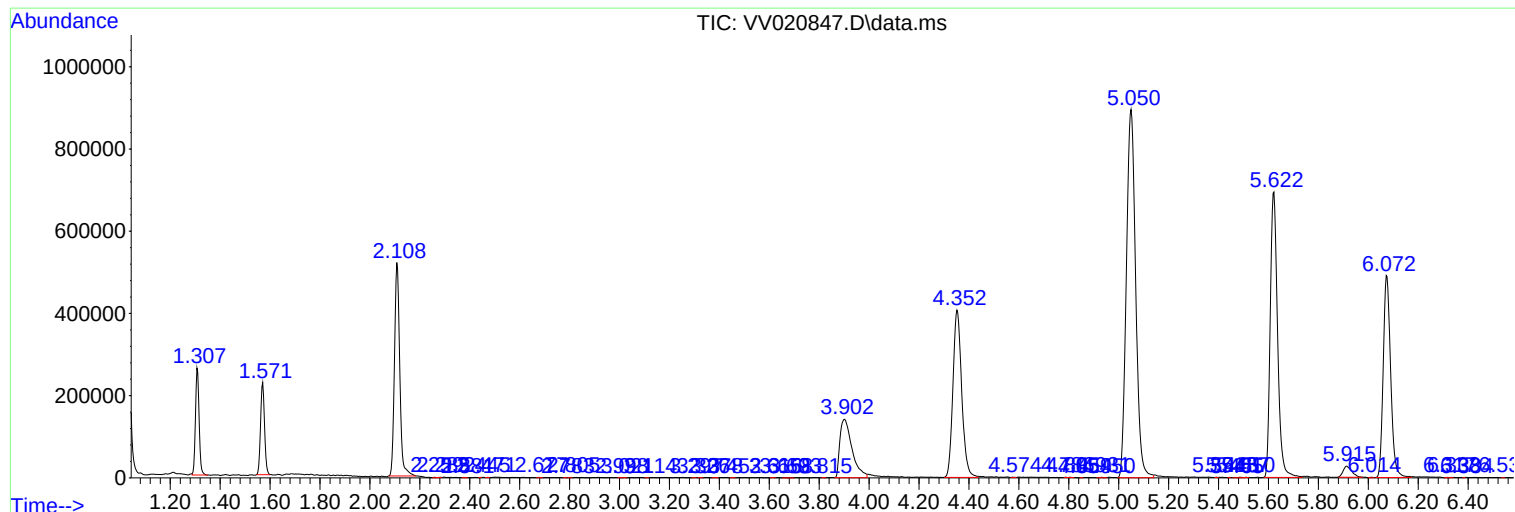

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020856.D
Acq On : 01 Apr 2021 22:46
Operator : SY/MD
Sample : M1845-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1A4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020856.D
Acq On : 01 Apr 2021 22:46
Operator : SY/MD
Sample : M1845-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1A4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
