

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020860.D
 Acq On : 02 Apr 2021 00:21
 Operator : SY/MD
 Sample : M1845-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020851.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	99	rBV2	930322	962074	41.22%	4.851%
2	1.571	158	165	180	rVB	218769	252939	10.84%	1.275%
3	2.108	322	332	355	rBV	505897	771372	33.05%	3.890%
4	2.281	382	386	388	rBV2	911	768	0.03%	0.004%
5	2.426	428	431	432	rBV2	724	437	0.02%	0.002%
6	2.500	449	454	457	rBV4	1147	1136	0.05%	0.006%
7	2.680	503	510	514	rBV4	983	1152	0.05%	0.006%
8	2.732	524	526	528	rBV2	448	268	0.01%	0.001%
9	2.764	530	536	538	rBV4	5650	5545	0.24%	0.028%
10	2.828	552	556	557	rBV	720	452	0.02%	0.002%
11	2.860	564	566	568	rBV	403	169	0.01%	0.001%
12	2.937	587	590	591	rBV	420	269	0.01%	0.001%
13	2.963	596	598	599	rBV	318	84	0.00%	0.000%
14	2.982	602	604	605	rBV	710	290	0.01%	0.001%
15	3.037	619	621	625	rVB2	415	292	0.01%	0.001%
16	3.063	625	629	630	rBV	364	241	0.01%	0.001%
17	3.140	651	653	655	rVB2	403	167	0.01%	0.001%
18	3.198	655	671	682	rBV3	8507	18182	0.78%	0.092%
19	3.265	690	692	693	rBV	513	246	0.01%	0.001%
20	3.297	699	702	707	rVB4	650	508	0.02%	0.003%
21	3.333	711	713	718	rVB3	418	289	0.01%	0.001%
22	3.359	718	721	722	rBV	350	177	0.01%	0.001%
23	3.368	722	724	725	rBV	312	110	0.00%	0.001%
24	3.384	728	729	732	rBV2	419	265	0.01%	0.001%
25	3.484	757	760	761	rBV2	219	121	0.01%	0.001%
26	3.568	783	786	791	rVB4	423	409	0.02%	0.002%
27	3.645	806	810	812	rVB2	594	352	0.02%	0.002%
28	3.677	818	820	821	rBV2	316	148	0.01%	0.001%
29	3.712	827	831	836	rBV3	799	698	0.03%	0.004%
30	3.732	836	837	839	rVB2	136	51	0.00%	0.000%
31	3.741	839	840	841	rBV	233	65	0.00%	0.000%
32	3.780	849	852	855	rBV	615	488	0.02%	0.002%
33	3.822	861	865	866	rBV	401	255	0.01%	0.001%
34	3.915	877	894	927	rBV2	875012	2333715	100.00%	11.768%
35	4.352	1016	1030	1056	rVB	397619	965403	41.37%	4.868%
36	4.786	1163	1165	1170	rVB3	654	521	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020860.D
 Acq On : 02 Apr 2021 00:21
 Operator : SY/MD
 Sample : M1845-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	4.812	1170	1173	1176	rVB3	479	215	0.01%	0.001%
38	4.902	1199	1201	1204	rVB3	407	191	0.01%	0.001%
39	4.918	1204	1206	1209	rBV2	314	191	0.01%	0.001%
40	5.050	1229	1247	1291	rBV2	887429	2286377	97.97%	11.529%

41	5.420	1359	1362	1366	rVB3	1087	746	0.03%	0.004%
42	5.510	1388	1390	1392	rBV3	424	158	0.01%	0.001%
43	5.545	1398	1401	1404	rVB2	879	489	0.02%	0.002%
44	5.558	1404	1405	1406	rBV	263	83	0.00%	0.000%
45	5.571	1407	1409	1411	rBV3	559	243	0.01%	0.001%

46	5.622	1411	1425	1453	rBV	698319	1423579	61.00%	7.179%
47	6.072	1553	1565	1591	rVB	486413	984697	42.19%	4.966%
48	6.516	1700	1703	1705	rBV2	1066	648	0.03%	0.003%
49	6.989	1838	1850	1877	rBV	272819	502078	21.51%	2.532%
50	7.320	1942	1953	1980	rBV	1039949	1793818	76.87%	9.046%

51	7.567	2028	2030	2034	rBV4	1126	1112	0.05%	0.006%
52	7.625	2037	2048	2075	rBV	198786	353225	15.14%	1.781%
53	7.821	2107	2109	2112	rVB2	1202	600	0.03%	0.003%
54	7.841	2112	2115	2116	rBV2	663	328	0.01%	0.002%
55	8.053	2175	2181	2183	rBV6	1082	1036	0.04%	0.005%

56	8.091	2183	2193	2224	rBV	535490	970683	41.59%	4.895%
57	8.751	2395	2398	2401	rBV4	983	729	0.03%	0.004%
58	8.857	2419	2431	2454	rBV	1059971	1706477	73.12%	8.605%
59	9.153	2520	2523	2526	rVB4	1586	1176	0.05%	0.006%
60	9.294	2565	2567	2569	rBV2	748	312	0.01%	0.002%

61	9.368	2588	2590	2594	rVB4	1149	671	0.03%	0.003%
62	9.413	2602	2604	2609	rVB4	1075	679	0.03%	0.003%
63	9.638	2670	2674	2677	rBV4	817	701	0.03%	0.004%
64	9.689	2688	2690	2692	rBV3	1234	717	0.03%	0.004%
65	9.947	2767	2770	2773	rBV2	729	420	0.02%	0.002%

66	10.005	2786	2788	2789	rBV	554	242	0.01%	0.001%
67	10.066	2803	2807	2809	rVB2	875	632	0.03%	0.003%
68	10.079	2809	2811	2814	rBV2	753	477	0.02%	0.002%
69	10.107	2816	2820	2822	rVV3	680	427	0.02%	0.002%
70	10.223	2844	2856	2879	rBV	719113	1134600	48.62%	5.721%

71	10.342	2889	2893	2895	rBV4	1037	752	0.03%	0.004%
72	10.580	2964	2967	2970	rBV3	795	597	0.03%	0.003%
73	10.677	2994	2997	2998	rBV3	739	402	0.02%	0.002%
74	10.982	3090	3092	3095	rVB3	755	354	0.02%	0.002%
75	11.021	3099	3104	3107	rBV3	943	710	0.03%	0.004%

76	11.037	3107	3109	3111	rBV	651	349	0.01%	0.002%
----	--------	------	------	------	-----	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020860.D
 Acq On : 02 Apr 2021 00:21
 Operator : SY/MD
 Sample : M1845-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	11.255	3165	3177	3201	rBV	1057081	1616769	69.28%	8.153%
78	11.474	3243	3245	3249	rBV3	624	328	0.01%	0.002%
79	11.632	3281	3294	3314	rBV	1087613	1713591	73.43%	8.641%
80	11.860	3363	3365	3369	rBV4	831	602	0.03%	0.003%
81	12.117	3442	3445	3446	rBV	733	447	0.02%	0.002%
82	12.268	3487	3492	3495	rBV4	770	673	0.03%	0.003%
83	12.320	3505	3508	3513	rBV4	1119	1010	0.04%	0.005%
84	12.429	3539	3542	3543	rBV	467	234	0.01%	0.001%
85	12.615	3597	3600	3601	rBV2	723	326	0.01%	0.002%
86	13.056	3735	3737	3739	rBV2	768	405	0.02%	0.002%
87	13.149	3764	3766	3767	rBV	617	240	0.01%	0.001%
88	13.365	3830	3833	3834	rBV2	780	391	0.02%	0.002%
89	13.522	3880	3882	3884	rBV2	822	450	0.02%	0.002%
90	13.577	3895	3899	3903	rBV5	949	982	0.04%	0.005%
91	13.789	3964	3965	3969	rBV3	840	492	0.02%	0.002%
92	13.808	3969	3971	3977	rVB3	1100	880	0.04%	0.004%
93	13.995	4026	4029	4031	rBV3	1218	957	0.04%	0.005%
94	14.049	4044	4046	4048	rVB2	1018	334	0.01%	0.002%




Sum of corrected areas: 19830690

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020860.D
Acq On : 02 Apr 2021 00:21
Operator : SY/MD
Sample : M1845-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

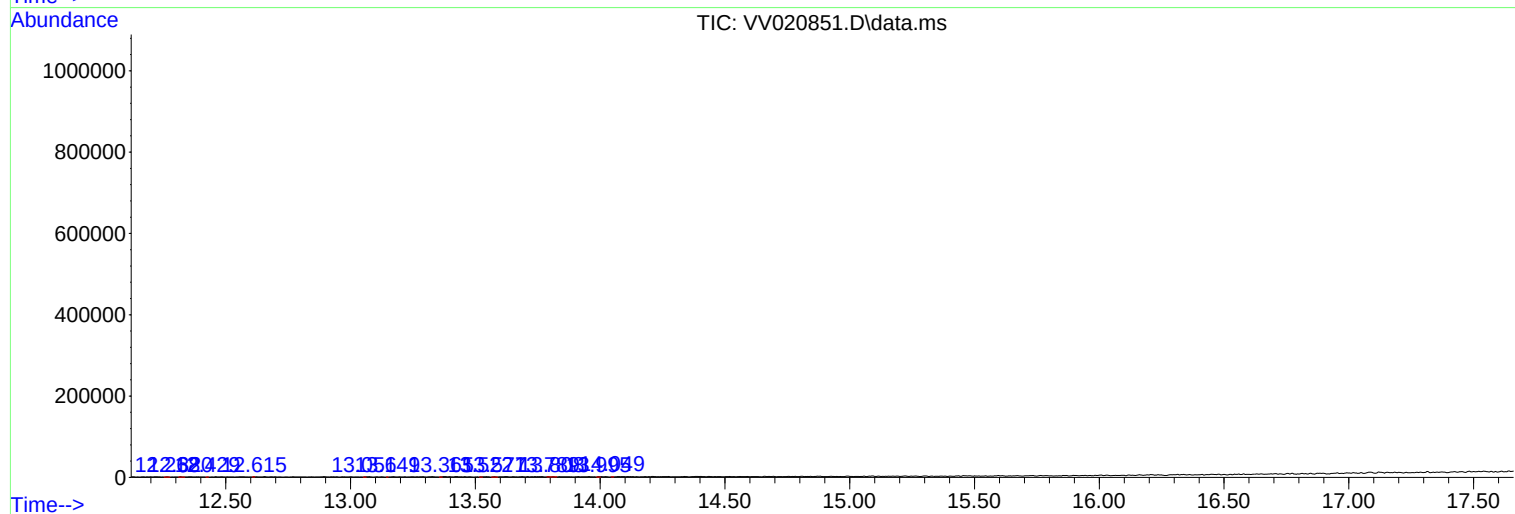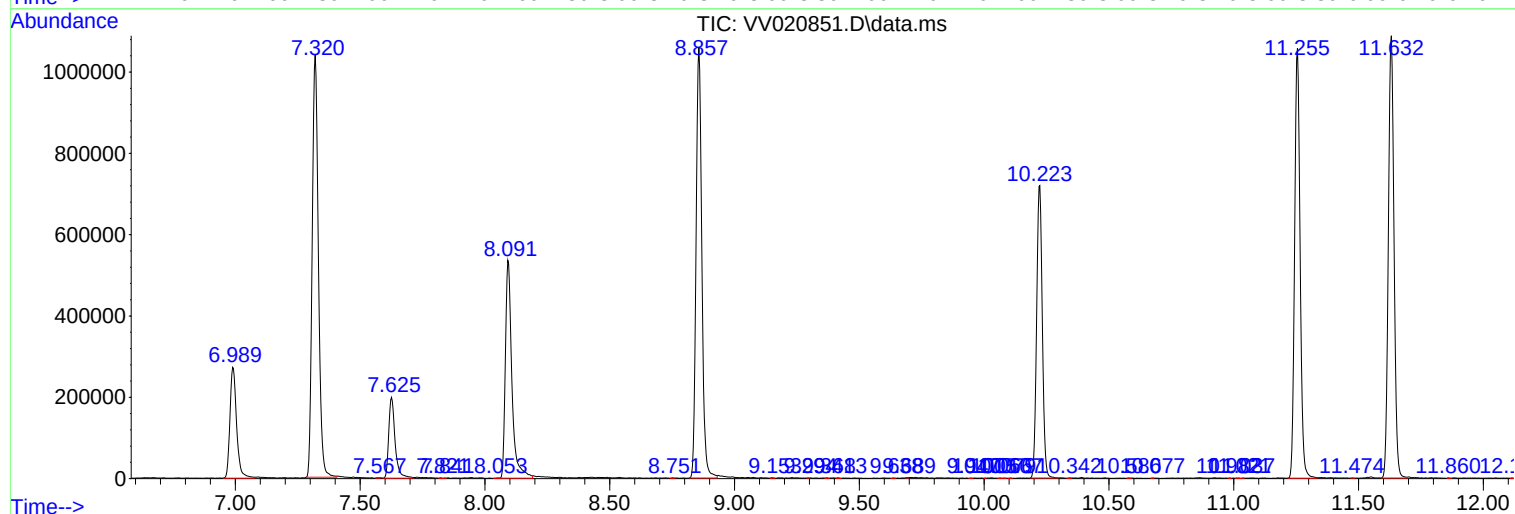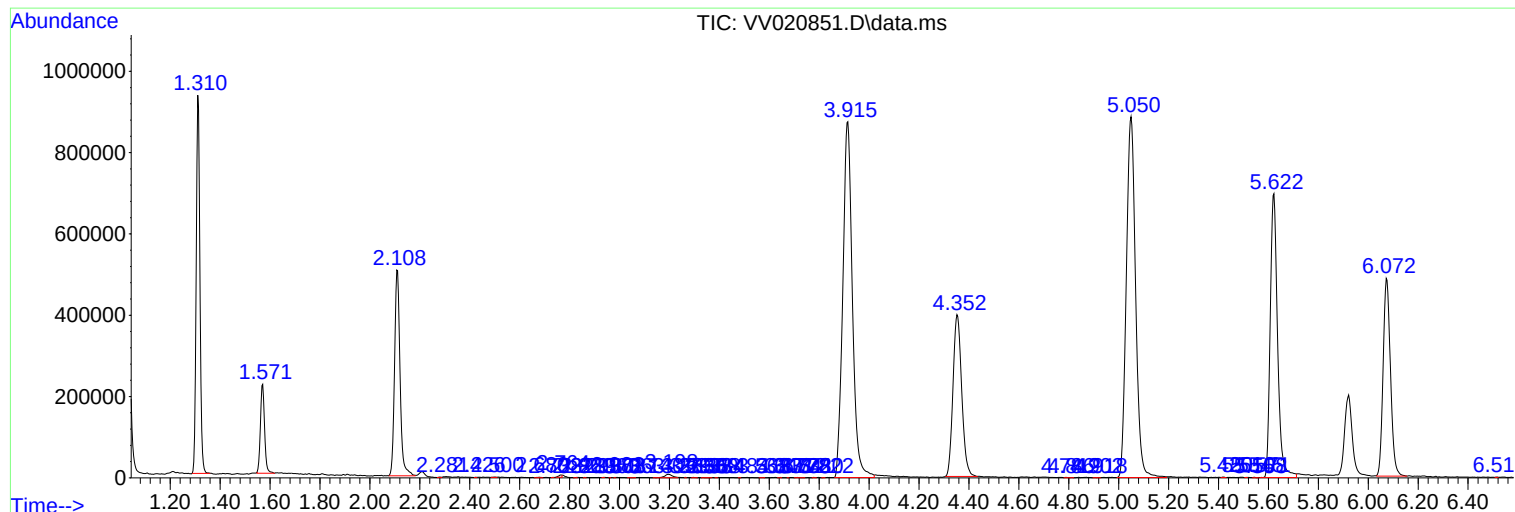

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020860.D
Acq On : 02 Apr 2021 00:21
Operator : SY/MD
Sample : M1845-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020860.D
Acq On : 02 Apr 2021 00:21
Operator : SY/MD
Sample : M1845-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
