

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020864.D
 Acq On : 02 Apr 2021 01:57
 Operator : SY/MD
 Sample : M1845-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1C5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020855.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	110	rVB	12510978	13052966	30.34%	17.941%
2	1.571	158	165	176	rBV	214800	238696	0.55%	0.328%
3	2.111	323	333	355	rVB	511734	782864	1.82%	1.076%
4	2.381	414	417	419	rBV2	722	529	0.00%	0.001%
5	2.551	468	470	473	rVB2	770	460	0.00%	0.001%
6	2.590	480	482	483	rBV2	496	226	0.00%	0.000%
7	2.641	496	498	502	rVB3	756	388	0.00%	0.001%
8	2.667	503	506	507	rBV3	897	411	0.00%	0.001%
9	2.703	511	517	519	rBV3	1013	1122	0.00%	0.002%
10	2.767	526	537	552	rBV2	49355	88022	0.20%	0.121%
11	2.957	590	596	597	rBV3	515	427	0.00%	0.001%
12	3.027	617	618	620	rBV	502	160	0.00%	0.000%
13	3.075	631	633	634	rBV	277	85	0.00%	0.000%
14	3.156	653	658	659	rBV3	621	523	0.00%	0.001%
15	3.194	659	670	690	rVB3	22338	49566	0.12%	0.068%
16	3.262	690	691	693	rBV	424	189	0.00%	0.000%
17	3.304	702	704	708	rVB	458	244	0.00%	0.000%
18	3.368	720	724	725	rBV2	438	282	0.00%	0.000%
19	3.403	733	735	737	rBV	333	114	0.00%	0.000%
20	3.416	737	739	742	rVB	527	253	0.00%	0.000%
21	3.442	742	747	748	rBV2	759	466	0.00%	0.001%
22	3.506	765	767	770	rBV	206	101	0.00%	0.000%
23	3.522	770	772	774	rBV2	572	262	0.00%	0.000%
24	3.564	782	785	786	rBV2	271	141	0.00%	0.000%
25	3.603	796	797	800	rVB	483	141	0.00%	0.000%
26	3.619	800	802	805	rBV	483	281	0.00%	0.000%
27	3.667	812	817	818	rBV	458	314	0.00%	0.000%
28	3.696	823	826	828	rBV2	372	270	0.00%	0.000%
29	3.751	841	843	846	rBV	466	314	0.00%	0.000%
30	3.838	867	870	874	rBV2	594	552	0.00%	0.001%
31	3.915	874	894	933	rBV	17827933	43025173	100.00%	59.138%
32	4.352	1017	1030	1061	rVB2	399162	983698	2.29%	1.352%
33	4.931	1208	1210	1214	rVB3	826	500	0.00%	0.001%
34	5.050	1230	1247	1277	rBV3	892953	2281155	5.30%	3.135%
35	5.474	1377	1379	1380	rBV2	772	265	0.00%	0.000%
36	5.619	1412	1424	1450	rBV	702231	1409249	3.28%	1.937%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW040121\
 Data File : VW020864.D
 Acq On : 02 Apr 2021 01:57
 Operator : SY/MD
 Sample : M1845-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1C5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	6.072	1553	1565	1584	rBV	487286	972960	2.26%	1.337%
38	6.548	1710	1713	1715	rBV2	930	609	0.00%	0.001%
39	6.635	1738	1740	1742	rBV3	868	490	0.00%	0.001%
40	6.780	1783	1785	1789	rBV3	775	540	0.00%	0.001%
41	6.802	1789	1792	1793	rBV	883	449	0.00%	0.001%
42	6.934	1830	1833	1835	rBV3	582	329	0.00%	0.000%
43	6.989	1839	1850	1879	rBV	273966	501695	1.17%	0.690%
44	7.320	1941	1953	1974	rBV	1059691	1807004	4.20%	2.484%
45	7.625	2037	2048	2065	rBV2	204267	359963	0.84%	0.495%
46	7.937	2141	2145	2146	rBV	1311	978	0.00%	0.001%
47	7.995	2160	2163	2170	rVB4	1342	1129	0.00%	0.002%
48	8.046	2176	2179	2183	rBV6	1024	961	0.00%	0.001%
49	8.091	2183	2193	2219	rBV	535905	980838	2.28%	1.348%
50	8.657	2367	2369	2372	rBV3	1035	633	0.00%	0.001%
51	8.718	2386	2388	2391	rBV3	1112	807	0.00%	0.001%
52	8.857	2419	2431	2454	rBV	1051961	1717649	3.99%	2.361%
53	9.226	2544	2546	2549	rBV2	1565	836	0.00%	0.001%
54	9.397	2597	2599	2603	rVB2	632	222	0.00%	0.000%
55	9.419	2603	2606	2608	rBV2	783	506	0.00%	0.001%
56	9.519	2635	2637	2641	rBV2	603	431	0.00%	0.001%
57	9.699	2691	2693	2695	rBV	351	145	0.00%	0.000%
58	9.831	2732	2734	2735	rBV2	515	200	0.00%	0.000%
59	9.953	2768	2772	2774	rBV	785	438	0.00%	0.001%
60	9.995	2781	2785	2786	rBV	690	464	0.00%	0.001%
61	10.130	2825	2827	2832	rBV4	737	492	0.00%	0.001%
62	10.220	2844	2855	2873	rBV	715028	1136807	2.64%	1.563%
63	10.368	2899	2901	2903	rBV2	910	508	0.00%	0.001%
64	10.496	2939	2941	2943	rBV2	665	310	0.00%	0.000%
65	10.757	3020	3022	3025	rBV2	590	386	0.00%	0.001%
66	10.850	3048	3051	3052	rBV3	714	429	0.00%	0.001%
67	10.905	3065	3068	3070	rBV2	727	532	0.00%	0.001%
68	11.255	3166	3177	3200	rBV	1069842	1628454	3.78%	2.238%
69	11.631	3282	3294	3312	rBV	1110182	1711998	3.98%	2.353%
70	11.998	3404	3408	3410	rBV3	861	715	0.00%	0.001%
71	12.934	3697	3699	3701	rBV	734	339	0.00%	0.000%
72	13.419	3849	3850	3856	rVB4	750	442	0.00%	0.001%
73	14.927	4316	4319	4321	rBV3	1575	1212	0.00%	0.002%




Sum of corrected areas: 72753309

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020864.D
Acq On : 02 Apr 2021 01:57
Operator : SY/MD
Sample : M1845-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

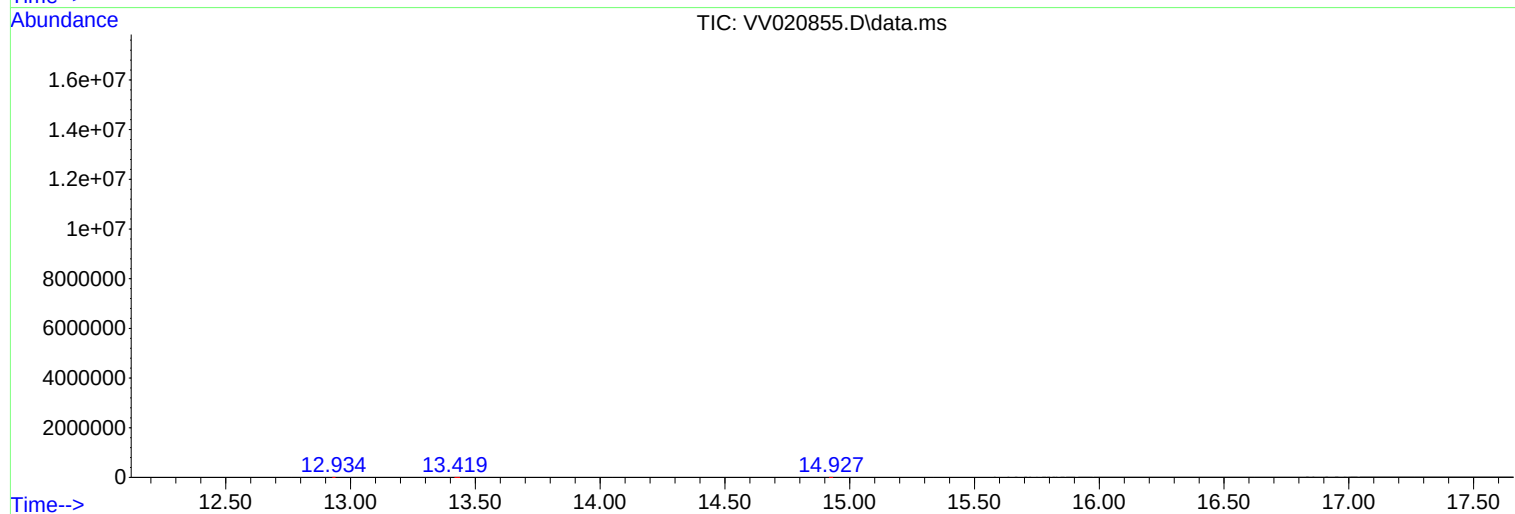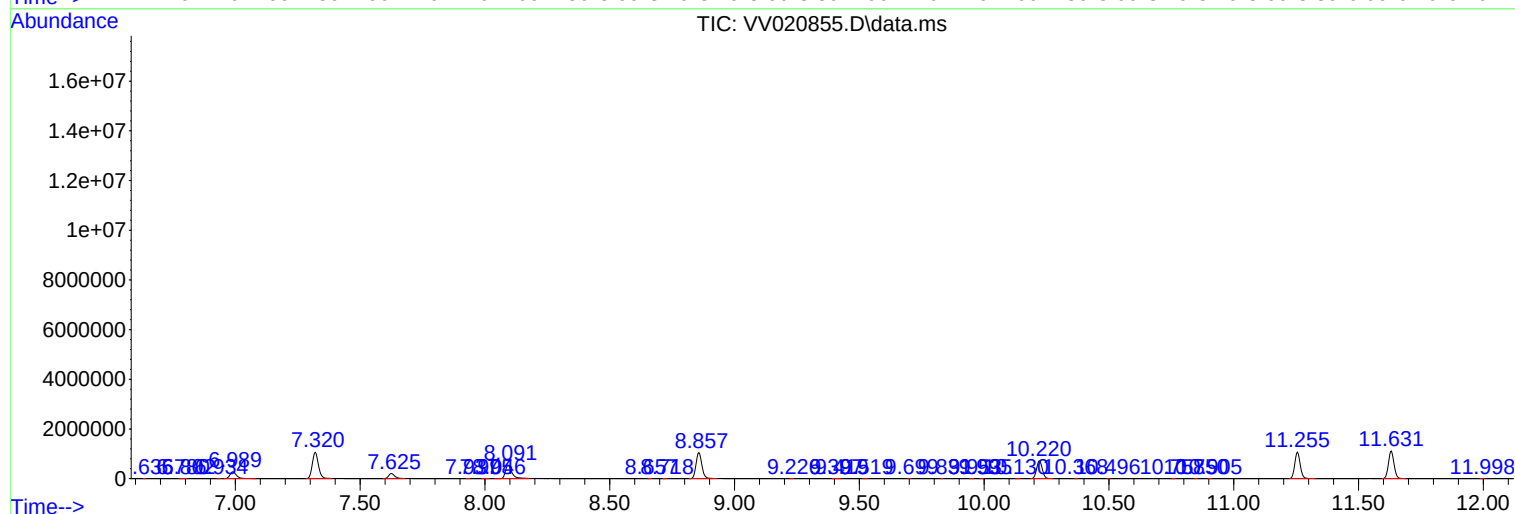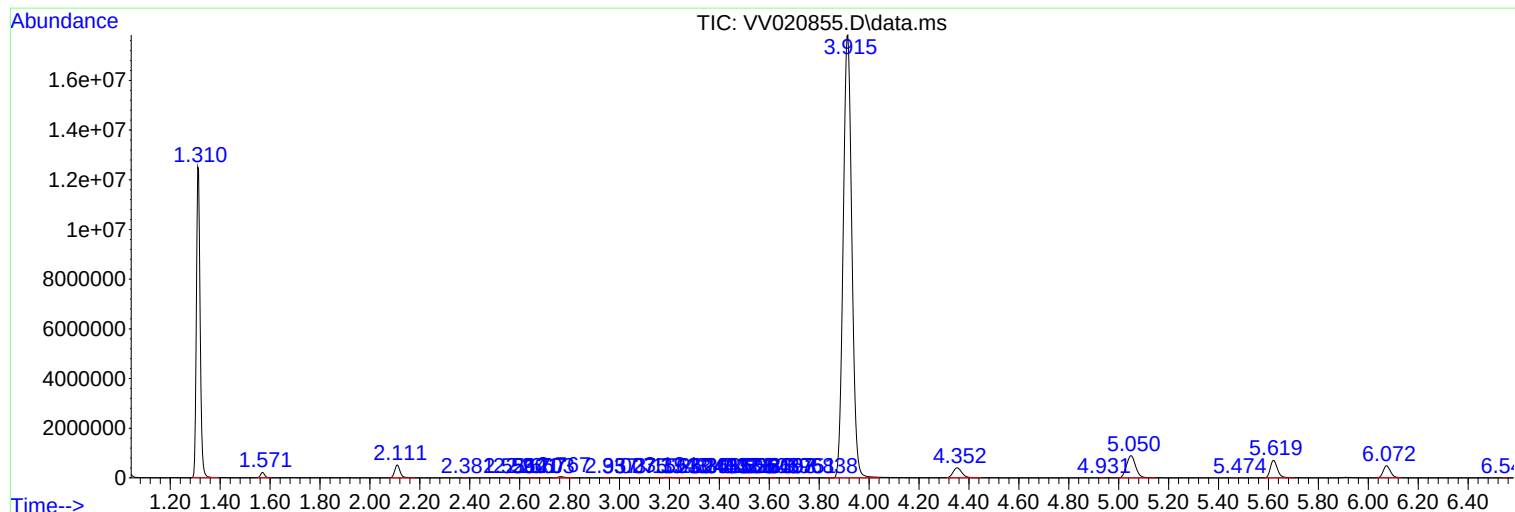

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020864.D
Acq On : 02 Apr 2021 01:57
Operator : SY/MD
Sample : M1845-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
Data File : VV020864.D
Acq On : 02 Apr 2021 01:57
Operator : SY/MD
Sample : M1845-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
