
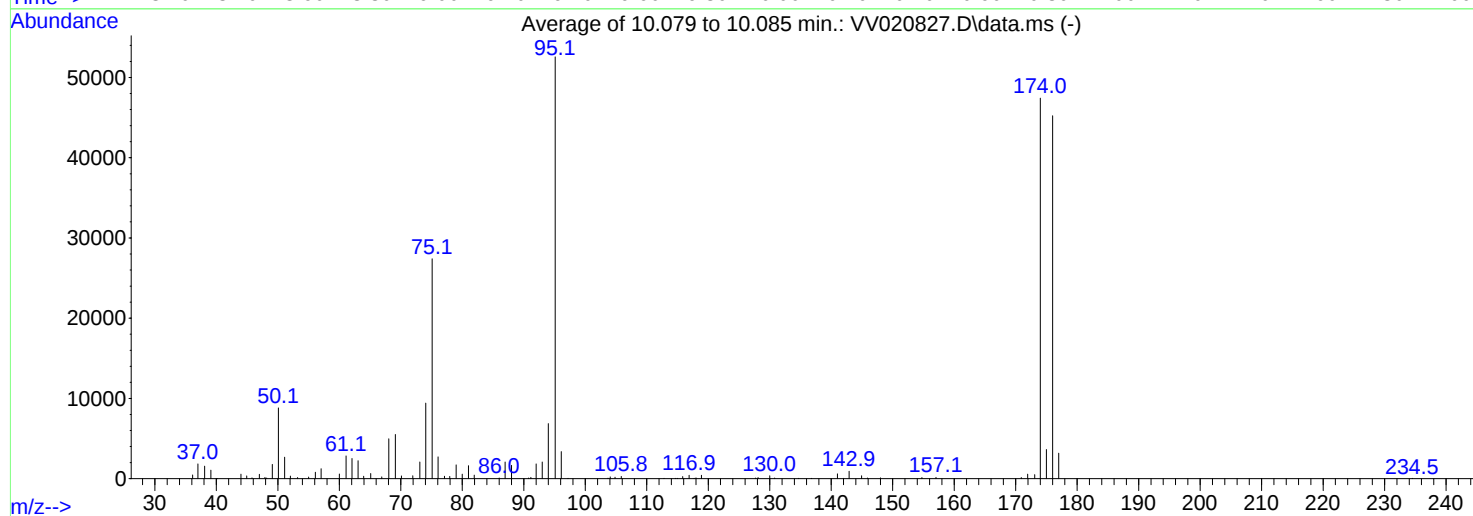


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040121\
 Data File : VV020827.D
 Acq On : 01 Apr 2021 09:16
 Operator : SY/MD
 Sample : BFB70
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB70

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis
 Last Update : Tue Apr 06 06:22:01 2021

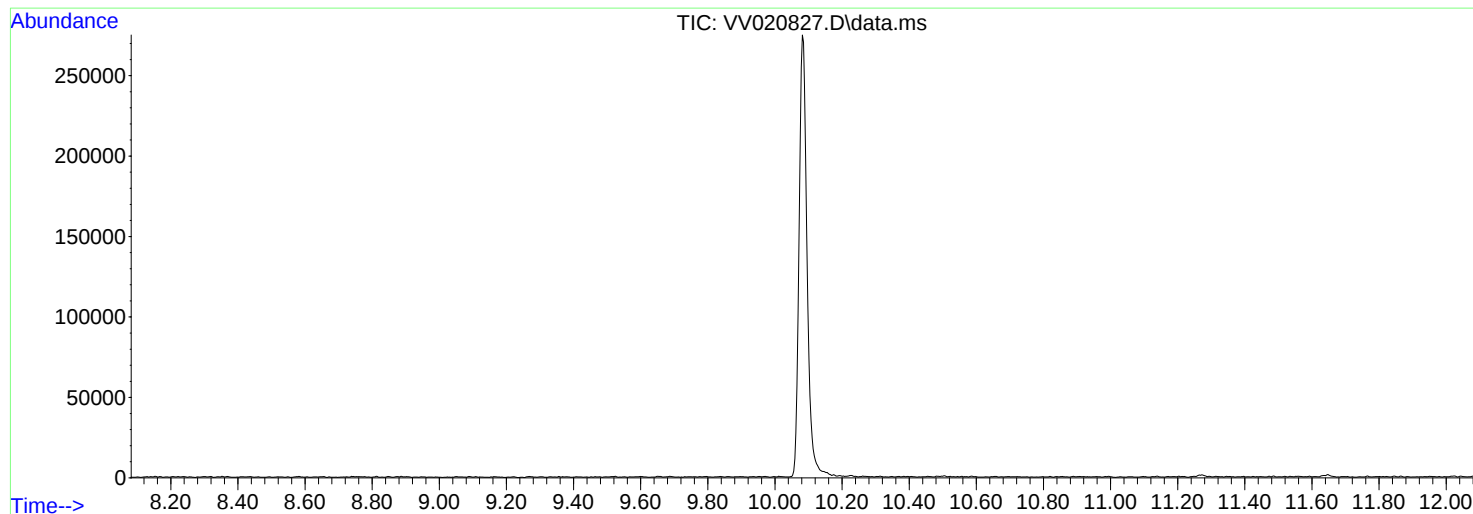

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	8818	PASS
75	95	30	80	52.1	27400	PASS
95	95	100	100	100.0	52573	PASS
96	95	5	9	6.4	3376	PASS
173	174	0.00	2	1.0	491	PASS
174	95	50	120	90.2	47424	PASS
175	174	5	9	7.7	3633	PASS
176	174	95	101	95.4	45232	PASS
177	176	5	9	7.0	3175	PASS

m/z	Abundance
36.20	507.0
37.00	1907.0
38.10	1572.0
39.10	1132.0
39.90	280.0
44.00	961.0
45.00	348.0
45.80	131.0
47.00	583.0
47.90	212.0
49.10	1845.0
50.10	9122.0
51.10	2785.0
52.00	359.0
53.20	125.0
55.00	202.0
56.10	821.0
57.00	1280.0
60.00	618.0
61.10	2905.0
62.00	2567.0
63.10	2385.0
63.90	300.0
65.10	672.0
66.90	229.0
68.10	5141.0
69.10	5759.0
70.10	348.0
72.00	376.0
73.10	2085.0
74.00	9772.0
75.10	28472.0
76.10	2764.0
77.10	311.0
78.00	301.0
79.00	1783.0
80.00	567.0
81.00	1632.0
81.90	421.0
86.00	136.0
87.00	2088.0
88.00	1695.0
91.10	234.0
92.00	1913.0
93.00	2098.0
94.00	7101.0
95.10	54280.0
96.10	3447.0
104.10	221.0
104.90	208.0
105.90	297.0
115.80	250.0
116.90	439.0
118.00	136.0
118.90	460.0
127.70	124.0
128.10	172.0
130.00	360.0
130.80	107.0
141.00	615.0
142.90	925.0
144.90	374.0
145.90	112.0
148.00	127.0
154.70	132.0
157.10	192.0
170.90	143.0
171.90	541.0
173.10	726.0
174.00	48568.0
175.00	3825.0
176.00	46288.0
177.00	3221.0
234.50	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.10	446.0
37.00	1844.0
38.10	1538.0
39.10	1112.0
39.90	282.0
44.00	888.0
44.90	343.0
45.80	148.0
47.00	428.0
48.20	248.0
49.10	1691.0
50.10	8473.0
51.10	2629.0
52.00	313.0
53.20	183.0
55.00	217.0
56.10	847.0
57.10	1286.0
60.00	665.0
61.10	2915.0
62.10	2641.0
63.10	2323.0
63.90	295.0
65.10	773.0
67.00	144.0
68.10	4806.0
69.10	5663.0
70.10	295.0
72.00	382.0
73.10	1937.0
74.10	9557.0
75.10	26880.0
76.00	2701.0
77.10	247.0
78.00	317.0
79.00	1701.0
80.00	634.0
81.00	1696.0
82.00	500.0
86.00	127.0
87.00	2220.0
88.00	1919.0
90.80	217.0
92.00	1952.0
93.00	1844.0
94.00	6892.0
95.10	52104.0
96.10	3536.0
104.00	279.0
104.90	236.0
105.90	344.0
114.70	106.0
115.90	252.0
116.90	418.0
118.00	154.0
118.90	388.0
128.10	267.0
130.00	377.0
130.80	116.0
134.70	115.0
141.00	619.0
142.00	151.0
142.90	926.0
144.90	329.0
148.00	190.0
154.80	138.0
157.10	141.0
170.90	106.0
171.90	588.0
174.00	49680.0
175.00	3719.0
176.00	47152.0
177.00	3195.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
40.10	258.0
41.50	102.0
43.90	374.0
48.50	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.20	403.0
37.00	1761.0
38.10	1590.0
39.10	952.0
40.00	219.0
44.10	922.0
45.00	314.0
47.00	599.0
47.90	260.0
49.10	1784.0
50.10	8859.0
51.10	2594.0
52.10	283.0
53.20	103.0
55.00	180.0
56.10	756.0
57.00	1144.0
60.00	470.0
61.10	2710.0
62.00	2318.0
63.00	1999.0
64.00	284.0
65.10	484.0
66.90	276.0
68.00	4926.0
69.10	5110.0
70.10	367.0
71.90	337.0
73.10	2231.0
74.10	8934.0
75.10	26848.0
76.10	2690.0
77.10	363.0
77.90	248.0
79.00	1683.0
80.00	462.0
81.00	1514.0
81.90	382.0
86.90	1948.0
88.00	1337.0
91.20	245.0
92.00	1630.0
93.00	2313.0
94.00	6599.0
95.10	51336.0
96.10	3146.0
97.20	116.0
103.70	176.0
104.10	169.0
104.80	126.0
105.80	216.0
112.80	114.0
115.00	115.0
115.80	260.0
116.90	414.0
117.70	135.0
118.90	395.0
127.70	102.0
130.00	355.0
136.80	116.0
141.00	537.0
142.90	901.0
145.00	347.0
145.90	122.0
154.80	129.0
157.00	176.0
170.90	185.0
172.00	521.0
173.10	746.0
174.00	44024.0
175.00	3354.0
176.00	42256.0
177.00	3109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70