

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
 Data File : VV034914.D
 Acq On : 01 Apr 2024 09:40
 Operator : SY/MD
 Sample : VV0401WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK258

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034914.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	229550	245195	15.84%	2.157%
2	1.532	146	153	170	rVB	242263	280357	18.11%	2.466%
3	2.059	307	317	335	rBV	393163	570300	36.85%	5.017%
4	2.696	513	515	517	rBV	375	162	0.01%	0.001%
5	2.847	557	562	567	rVB3	639	662	0.04%	0.006%
6	2.879	567	572	573	rBV	427	327	0.02%	0.003%
7	2.950	591	594	599	rVB3	627	499	0.03%	0.004%
8	2.979	600	603	604	rVV3	261	139	0.01%	0.001%
9	2.992	605	607	611	rVB3	810	412	0.03%	0.004%
10	3.047	622	624	627	rBV2	283	133	0.01%	0.001%
11	3.156	656	658	659	rBV2	320	125	0.01%	0.001%
12	3.169	659	662	665	rVB	605	444	0.03%	0.004%
13	3.188	665	668	671	rBV3	423	350	0.02%	0.003%
14	3.233	679	682	684	rVB	387	224	0.01%	0.002%
15	3.252	684	688	691	rBV2	610	557	0.04%	0.005%
16	3.320	706	709	711	rBV2	370	236	0.02%	0.002%
17	3.532	771	775	778	rBV2	520	381	0.02%	0.003%
18	3.596	792	795	797	rBV	549	374	0.02%	0.003%
19	3.664	814	816	817	rBV	207	67	0.00%	0.001%
20	3.744	839	841	842	rBV	380	171	0.01%	0.002%
21	3.793	846	856	899	rBV	106220	331894	21.44%	2.920%
22	4.246	983	997	1026	rBV	238975	612388	39.57%	5.387%
23	4.715	1141	1143	1146	rBV2	452	215	0.01%	0.002%
24	4.754	1152	1155	1156	rBV	478	205	0.01%	0.002%
25	4.786	1163	1165	1167	rBV	283	124	0.01%	0.001%
26	4.857	1181	1187	1191	rBV3	599	642	0.04%	0.006%
27	4.953	1202	1217	1254	rBV2	585722	1547776	100.00%	13.617%
28	5.429	1361	1365	1369	rBV4	696	586	0.04%	0.005%
29	5.532	1386	1397	1432	rBV	415970	868419	56.11%	7.640%
30	5.747	1462	1464	1467	rVB3	951	496	0.03%	0.004%
31	5.831	1482	1490	1503	rBV4	12505	25957	1.68%	0.228%
32	5.985	1525	1538	1562	rBV	342722	711648	45.98%	6.261%
33	6.239	1615	1617	1619	rBV	841	433	0.03%	0.004%
34	6.461	1678	1686	1691	rBV3	598	727	0.05%	0.006%
35	6.497	1695	1697	1699	rBV	299	153	0.01%	0.001%
36	6.558	1714	1716	1722	rBV3	376	342	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
 Data File : VV034914.D
 Acq On : 01 Apr 2024 09:40
 Operator : SY/MD
 Sample : VV0401WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK258

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.635	1738	1740	1742	rBV2	258	101	0.01%	0.001%
38	6.667	1748	1750	1751	rBV	329	142	0.01%	0.001%
39	6.706	1759	1762	1765	rBV3	615	289	0.02%	0.003%
40	6.747	1773	1775	1777	rBV2	219	80	0.01%	0.001%
41	6.760	1777	1779	1781	rBV	381	182	0.01%	0.002%
42	6.834	1800	1802	1804	rBV	347	204	0.01%	0.002%
43	6.911	1815	1826	1857	rBV	170966	333906	21.57%	2.938%
44	7.159	1900	1903	1906	rBV4	878	765	0.05%	0.007%
45	7.243	1918	1929	1962	rBV	662780	1175219	75.93%	10.339%
46	7.554	2015	2026	2052	rBV	114613	218905	14.14%	1.926%
47	7.976	2154	2157	2160	rBV2	513	252	0.02%	0.002%
48	8.027	2163	2173	2218	rBV2	312001	699707	45.21%	6.156%
49	8.403	2287	2290	2292	rBV3	729	598	0.04%	0.005%
50	8.615	2353	2356	2360	rBV3	415	359	0.02%	0.003%
51	8.783	2397	2408	2441	rBV	630746	1056668	68.27%	9.296%
52	9.053	2489	2492	2495	rVB3	757	418	0.03%	0.004%
53	9.072	2495	2498	2500	rBV2	639	417	0.03%	0.004%
54	9.181	2530	2532	2533	rBV	449	218	0.01%	0.002%
55	9.345	2581	2583	2586	rBV	399	206	0.01%	0.002%
56	9.439	2610	2612	2613	rBV	319	111	0.01%	0.001%
57	9.654	2677	2679	2681	rBV2	272	165	0.01%	0.001%
58	9.841	2735	2737	2739	rBV	353	199	0.01%	0.002%
59	9.853	2739	2741	2743	rVV	276	145	0.01%	0.001%
60	9.924	2762	2763	2764	rBV	342	101	0.01%	0.001%
61	9.956	2770	2773	2776	rBV2	668	455	0.03%	0.004%
62	10.004	2784	2788	2792	rBV2	445	455	0.03%	0.004%
63	10.152	2819	2834	2856	rBV	450273	728910	47.09%	6.413%
64	10.451	2925	2927	2931	rBV3	363	229	0.01%	0.002%
65	10.474	2932	2934	2937	rVB2	395	201	0.01%	0.002%
66	10.525	2947	2950	2952	rBV2	528	256	0.02%	0.002%
67	10.561	2958	2961	2963	rVB2	521	249	0.02%	0.002%
68	10.815	3038	3040	3042	rBV	311	184	0.01%	0.002%
69	10.860	3051	3054	3055	rBV2	463	293	0.02%	0.003%
70	10.921	3070	3073	3076	rBV2	652	329	0.02%	0.003%
71	10.953	3081	3083	3091	rVB2	682	527	0.03%	0.005%
72	10.992	3091	3095	3096	rBV2	380	222	0.01%	0.002%
73	11.024	3103	3105	3107	rBV	325	115	0.01%	0.001%
74	11.184	3144	3155	3178	rBV	578046	911672	58.90%	8.020%
75	11.484	3244	3248	3249	rBV2	430	273	0.02%	0.002%
76	11.557	3260	3271	3294	rBV	620534	992889	64.15%	8.735%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
Data File : VV034914.D
Acq On : 01 Apr 2024 09:40
Operator : SY/MD
Sample : VV0401WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK258

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

77	12.085	3433	3435	3436	rVB	347	95	0.01%	0.001%
78	12.834	3661	3668	3670	rBV3	610	588	0.04%	0.005%
79	12.847	3670	3672	3674	rBV	405	247	0.02%	0.002%
80	13.210	3776	3785	3795	rBV8	4109	6594	0.43%	0.058%
81	13.393	3840	3842	3843	rBV	558	188	0.01%	0.002%
82	13.445	3850	3858	3873	rBV	13631	23652	1.53%	0.208%
83	13.686	3927	3933	3940	rBV8	4033	5746	0.37%	0.051%




Sum of corrected areas: 11366846

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
Data File : VV034914.D
Acq On : 01 Apr 2024 09:40
Operator : SY/MD
Sample : VV0401WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK258

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

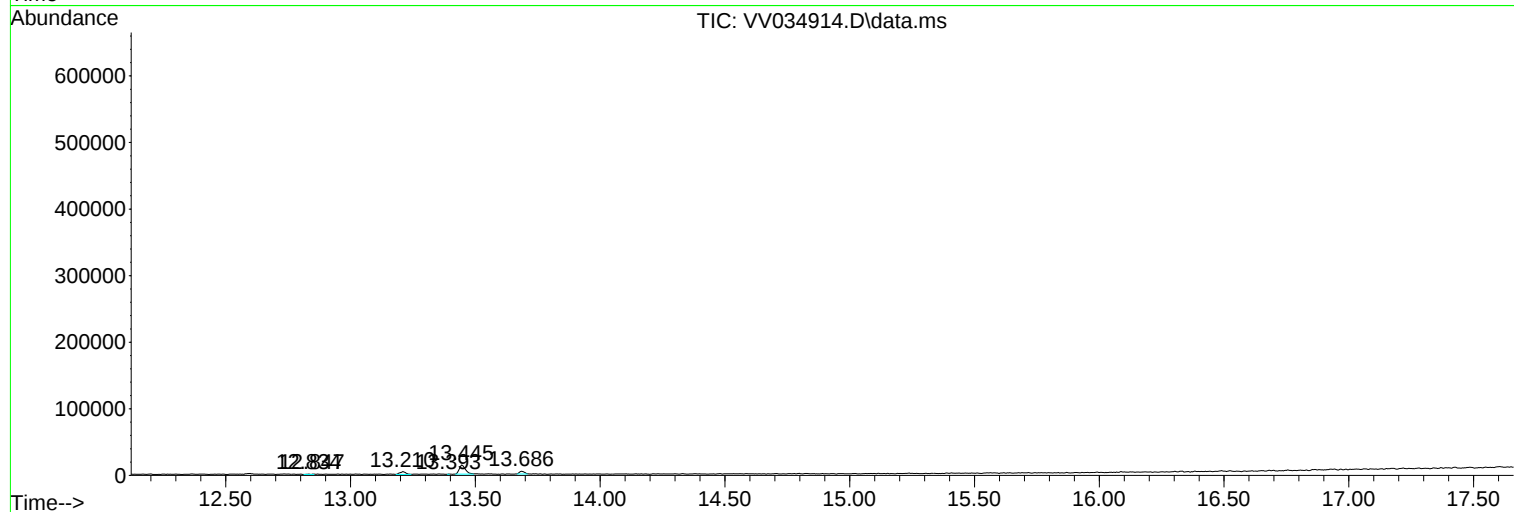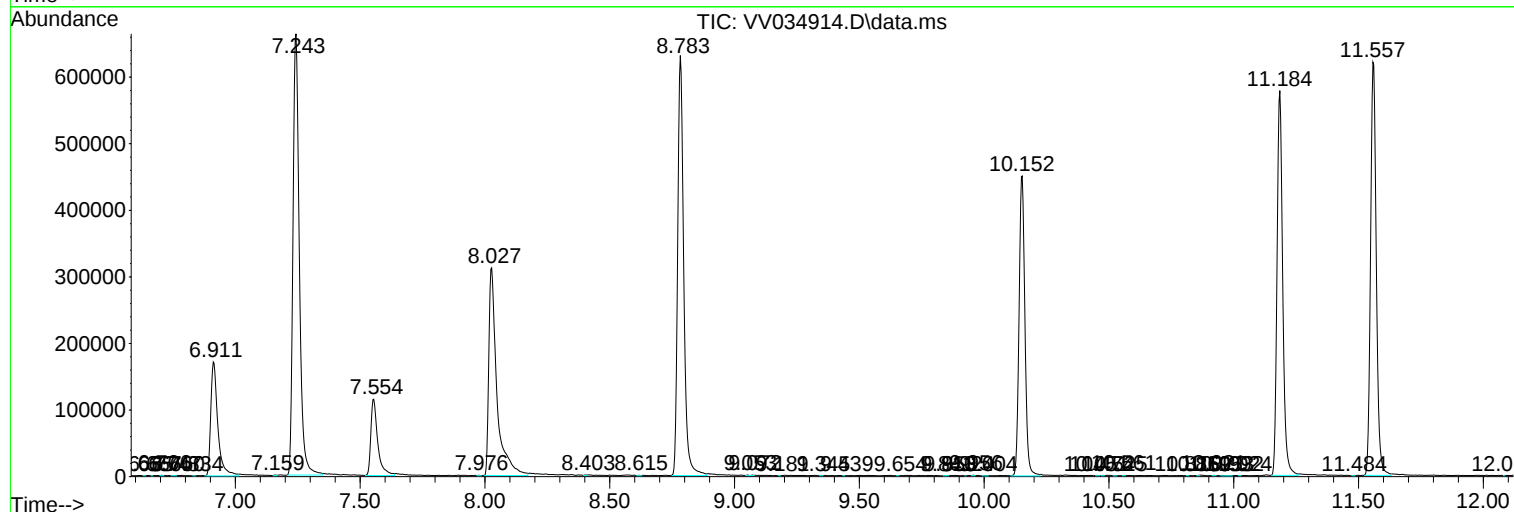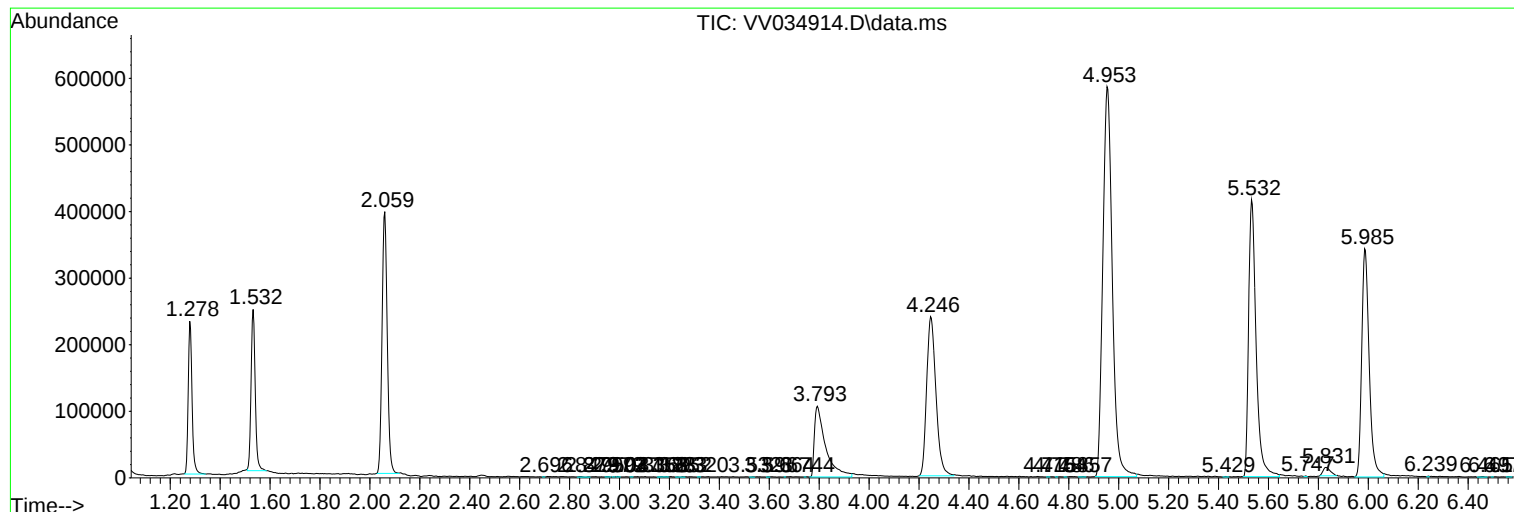

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
Data File : VV034914.D
Acq On : 01 Apr 2024 09:40
Operator : SY/MD
Sample : VV0401WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK258

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
Data File : VV034914.D
Acq On : 01 Apr 2024 09:40
Operator : SY/MD
Sample : VV0401WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK258

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------