

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
 Data File : VV034915.D
 Acq On : 01 Apr 2024 10:48
 Operator : SY/MD
 Sample : P1934-02DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R36DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV034915.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	230928	243861	11.57%	1.824%
2	1.529	146	152	176	rVB	260797	313683	14.88%	2.346%
3	2.057	306	316	331	rBV	403009	585237	27.76%	4.377%
4	2.446	430	437	452	rVB5	3693	6949	0.33%	0.052%
5	2.520	458	460	462	rBV2	435	262	0.01%	0.002%
6	2.828	554	556	558	rBV	302	95	0.00%	0.001%
7	2.880	570	572	574	rVB	245	114	0.01%	0.001%
8	2.896	574	577	579	rBV2	444	244	0.01%	0.002%
9	2.909	579	581	582	rBV2	227	110	0.01%	0.001%
10	3.015	611	614	616	rBV	308	198	0.01%	0.001%
11	3.092	636	638	642	rVB	499	323	0.02%	0.002%
12	3.140	642	653	655	rBV2	442	717	0.03%	0.005%
13	3.182	663	666	670	rVB3	408	303	0.01%	0.002%
14	3.214	672	676	677	rBV	365	252	0.01%	0.002%
15	3.272	689	694	696	rBV2	534	443	0.02%	0.003%
16	3.314	704	707	712	rBV3	290	283	0.01%	0.002%
17	3.391	728	731	733	rBV	157	84	0.00%	0.001%
18	3.442	744	747	749	rBV2	324	192	0.01%	0.001%
19	3.484	758	760	761	rBV2	184	83	0.00%	0.001%
20	3.516	768	770	772	rBV	443	237	0.01%	0.002%
21	3.642	806	809	812	rBV3	218	200	0.01%	0.001%
22	3.661	812	815	816	rVV	281	162	0.01%	0.001%
23	3.671	816	818	825	rVB2	501	493	0.02%	0.004%
24	3.706	825	829	833	rBV2	445	442	0.02%	0.003%
25	3.751	840	843	846	rBV3	444	408	0.02%	0.003%
26	3.790	846	855	888	rBV	99325	307911	14.61%	2.303%
27	4.243	981	996	1032	rBV	231359	605233	28.71%	4.527%
28	4.574	1097	1099	1101	rVB2	445	190	0.01%	0.001%
29	4.629	1114	1116	1118	rBV	431	172	0.01%	0.001%
30	4.745	1150	1152	1155	rVB2	482	189	0.01%	0.001%
31	4.767	1155	1159	1162	rBV2	868	521	0.02%	0.004%
32	4.883	1192	1195	1199	rBV2	420	389	0.02%	0.003%
33	4.950	1201	1216	1264	rVV2	573482	1535049	72.82%	11.481%
34	5.355	1339	1342	1344	rVB	377	190	0.01%	0.001%
35	5.529	1385	1396	1433	rBV	411752	864190	41.00%	6.464%
36	5.828	1481	1489	1508	rVB3	11886	26683	1.27%	0.200%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
 Data File : VV034915.D
 Acq On : 01 Apr 2024 10:48
 Operator : SY/MD
 Sample : P1934-02DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R36DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.986	1524	1538	1567	rBV	332746	695851	33.01%	5.204%
38	6.317	1638	1641	1643	rBV4	603	316	0.01%	0.002%
39	6.423	1669	1674	1676	rBV2	277	209	0.01%	0.002%
40	6.442	1676	1680	1683	rVV3	500	336	0.02%	0.003%
41	6.458	1683	1685	1687	rVV	258	109	0.01%	0.001%
42	6.474	1687	1690	1695	rVB3	447	446	0.02%	0.003%
43	6.500	1695	1698	1701	rBV3	598	314	0.01%	0.002%
44	6.516	1701	1703	1706	rBV	471	258	0.01%	0.002%
45	6.568	1716	1719	1724	rVB2	432	368	0.02%	0.003%
46	6.590	1724	1726	1729	rVB2	379	170	0.01%	0.001%
47	6.625	1731	1737	1738	rBV3	577	536	0.03%	0.004%
48	6.654	1743	1746	1748	rBV2	546	382	0.02%	0.003%
49	6.722	1765	1767	1769	rVB	397	128	0.01%	0.001%
50	6.738	1769	1772	1774	rBV	368	187	0.01%	0.001%
51	6.793	1786	1789	1790	rBV	474	282	0.01%	0.002%
52	6.847	1800	1806	1809	rVV3	406	472	0.02%	0.004%
53	6.912	1815	1826	1862	rBV	170747	334077	15.85%	2.499%
54	7.150	1897	1900	1902	rBV3	908	578	0.03%	0.004%
55	7.240	1917	1928	1957	rBV	666754	1166639	55.34%	8.726%
56	7.551	2016	2025	2050	rBV	114190	213173	10.11%	1.594%
57	7.863	2118	2122	2126	rBV3	824	873	0.04%	0.007%
58	7.912	2135	2137	2139	rBV	297	149	0.01%	0.001%
59	7.950	2145	2149	2151	rBV3	524	314	0.01%	0.002%
60	8.024	2163	2172	2217	rBV2	284013	646902	30.69%	4.838%
61	8.503	2319	2321	2323	rBV	399	191	0.01%	0.001%
62	8.645	2362	2365	2366	rBV2	516	315	0.01%	0.002%
63	8.680	2374	2376	2377	rBV2	459	196	0.01%	0.001%
64	8.728	2390	2391	2392	rBV2	285	92	0.00%	0.001%
65	8.783	2397	2408	2442	rBV2	653688	1320646	62.65%	9.878%
66	8.995	2472	2474	2476	rBV2	533	226	0.01%	0.002%
67	9.166	2525	2527	2530	rVB2	884	391	0.02%	0.003%
68	9.188	2530	2534	2537	rBV2	451	454	0.02%	0.003%
69	9.227	2544	2546	2548	rBV	381	208	0.01%	0.002%
70	9.326	2574	2577	2578	rBV	201	109	0.01%	0.001%
71	9.355	2584	2586	2589	rBV2	467	267	0.01%	0.002%
72	9.391	2595	2597	2600	rBV2	208	104	0.00%	0.001%
73	9.407	2600	2602	2604	rBV2	335	146	0.01%	0.001%
74	9.513	2633	2635	2639	rBV3	255	155	0.01%	0.001%
75	9.532	2639	2641	2643	rVB3	214	80	0.00%	0.001%
76	9.548	2643	2646	2653	rVB4	846	620	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
 Data File : VV034915.D
 Acq On : 01 Apr 2024 10:48
 Operator : SY/MD
 Sample : P1934-02DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R36DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.590	2657	2659	2660	rBV	261	128	0.01%	0.001%
78	9.731	2701	2703	2705	rBV	241	102	0.00%	0.001%
79	9.886	2749	2751	2758	rVB3	709	499	0.02%	0.004%
80	9.921	2758	2762	2765	rBV3	638	521	0.02%	0.004%
81	9.940	2765	2768	2771	rVB2	379	247	0.01%	0.002%
82	10.043	2797	2800	2803	rBV3	358	238	0.01%	0.002%
83	10.149	2821	2833	2856	rBV	434088	698613	33.14%	5.225%
84	10.397	2906	2910	2912	rBV3	565	434	0.02%	0.003%
85	10.487	2936	2938	2941	rVB	500	212	0.01%	0.002%
86	10.619	2974	2979	2984	rBV3	665	705	0.03%	0.005%
87	10.686	2999	3000	3001	rBV	425	102	0.00%	0.001%
88	10.709	3005	3007	3009	rBV2	263	97	0.00%	0.001%
89	10.728	3012	3013	3014	rBV2	293	79	0.00%	0.001%
90	10.992	3092	3095	3096	rBV2	344	190	0.01%	0.001%
91	11.120	3126	3135	3144	rBV2	27714	43372	2.06%	0.324%
92	11.185	3145	3155	3180	rVB2	639108	1244469	59.04%	9.308%
93	11.571	3259	3275	3299	rBV2	880795	2108000	100.00%	15.766%
94	12.538	3575	3576	3579	rBV3	500	276	0.01%	0.002%
95	12.590	3585	3592	3607	rBV4	5493	11388	0.54%	0.085%
96	13.043	3730	3733	3734	rBV2	658	306	0.01%	0.002%
97	13.198	3771	3781	3802	rBV	159130	254817	12.09%	1.906%
98	13.452	3854	3860	3868	rBV2	3914	5407	0.26%	0.040%
99	13.680	3921	3931	3947	rBV2	72582	116158	5.51%	0.869%
100	14.339	4134	4136	4140	rVB2	850	518	0.02%	0.004%




Sum of corrected areas: 13370239

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
Data File : VV034915.D
Acq On : 01 Apr 2024 10:48
Operator : SY/MD
Sample : P1934-02DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R36DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

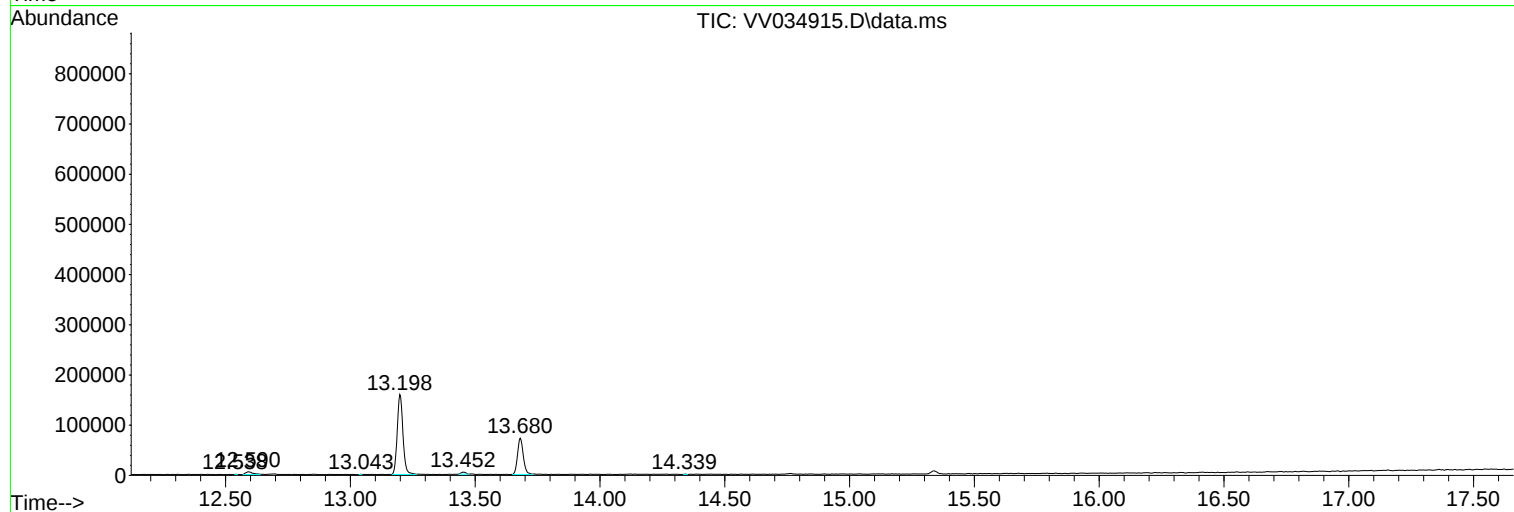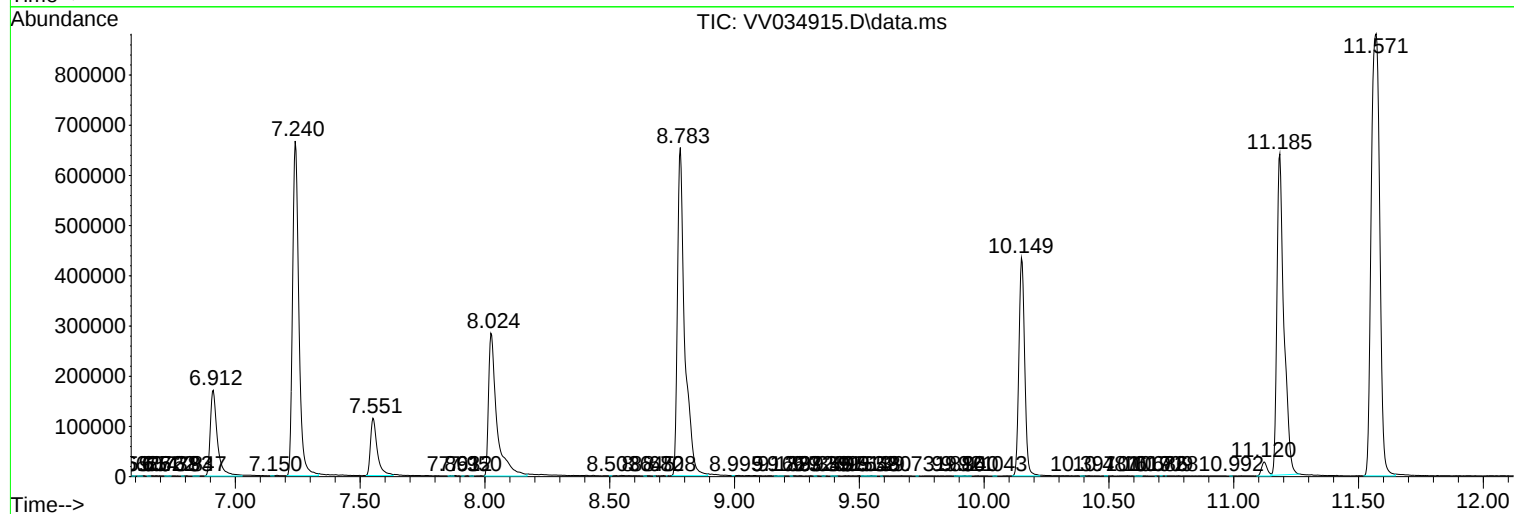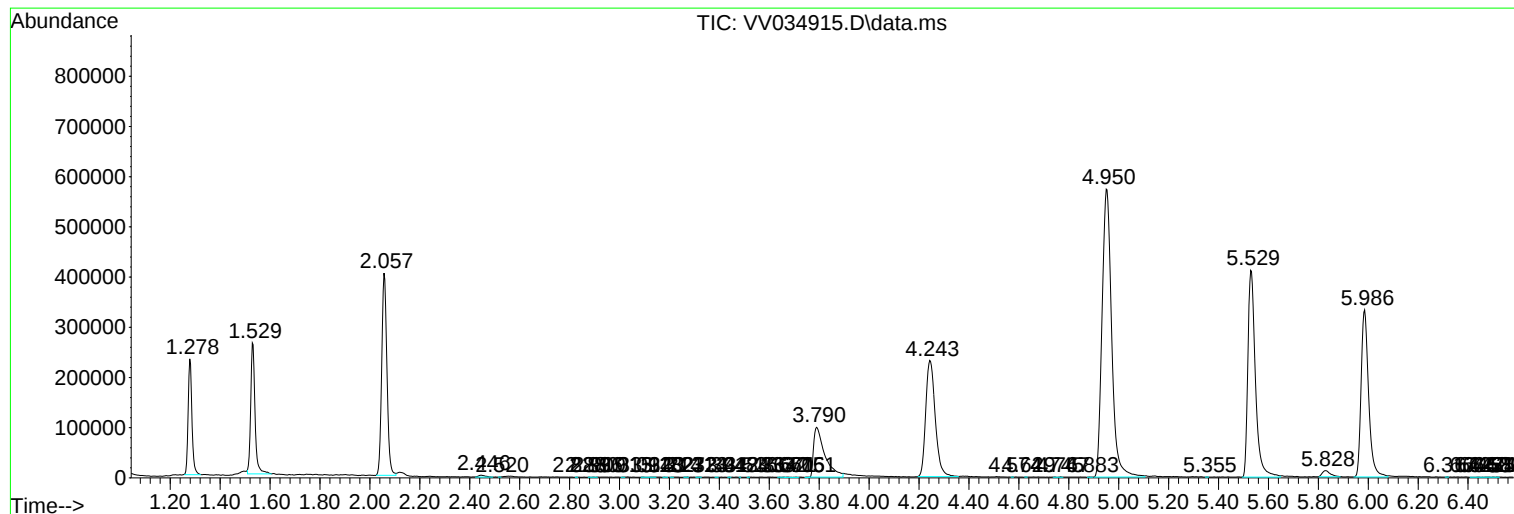

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
Data File : VV034915.D
Acq On : 01 Apr 2024 10:48
Operator : SY/MD
Sample : P1934-02DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R36DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
Data File : VV034915.D
Acq On : 01 Apr 2024 10:48
Operator : SY/MD
Sample : P1934-02DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R36DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc