

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
 Data File : VV034916.D
 Acq On : 01 Apr 2024 11:12
 Operator : SY/MD
 Sample : P1934-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034916.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	92	rBV	236791	248706	15.92%	2.174%
2	1.532	146	153	166	rBV	241129	273245	17.49%	2.389%
3	2.056	307	316	335	rBV	402731	589172	37.71%	5.151%
4	2.500	451	454	456	rBV2	588	422	0.03%	0.004%
5	2.539	462	466	468	rBV2	666	261	0.02%	0.002%
6	2.552	468	470	471	rBV2	522	202	0.01%	0.002%
7	2.786	540	543	545	rBV2	330	209	0.01%	0.002%
8	2.864	564	567	568	rBV	355	152	0.01%	0.001%
9	2.905	577	580	584	rBV2	399	211	0.01%	0.002%
10	2.970	597	600	603	rVV	304	241	0.02%	0.002%
11	3.005	609	611	614	rBV2	303	181	0.01%	0.002%
12	3.053	620	626	635	rVB3	546	879	0.06%	0.008%
13	3.092	635	638	641	rBV2	364	236	0.02%	0.002%
14	3.118	642	646	648	rBV	326	216	0.01%	0.002%
15	3.243	681	685	686	rBV2	489	218	0.01%	0.002%
16	3.265	690	692	694	rBV	418	199	0.01%	0.002%
17	3.285	695	698	701	rVB2	450	294	0.02%	0.003%
18	3.343	713	716	718	rBV	467	260	0.02%	0.002%
19	3.436	740	745	748	rBV3	425	408	0.03%	0.004%
20	3.455	748	751	754	rVB3	503	366	0.02%	0.003%
21	3.471	754	756	758	rVB2	273	136	0.01%	0.001%
22	3.552	777	781	785	rVB3	490	500	0.03%	0.004%
23	3.590	785	793	797	rBV3	648	912	0.06%	0.008%
24	3.616	797	801	804	rVB4	615	455	0.03%	0.004%
25	3.635	804	807	811	rVB2	340	246	0.02%	0.002%
26	3.658	811	814	816	rBV	273	172	0.01%	0.002%
27	3.680	818	821	824	rBV2	391	270	0.02%	0.002%
28	3.732	833	837	839	rBV2	292	207	0.01%	0.002%
29	3.764	845	847	848	rBV	297	138	0.01%	0.001%
30	3.793	848	856	886	rBV	99394	297519	19.04%	2.601%
31	4.246	983	997	1027	rBV	238818	614169	39.31%	5.369%
32	4.780	1158	1163	1166	rBV2	527	386	0.02%	0.003%
33	4.799	1167	1169	1172	rBV3	364	213	0.01%	0.002%
34	4.953	1200	1217	1251	rBV2	588356	1562330	100.00%	13.659%
35	5.388	1350	1352	1355	rBV	418	311	0.02%	0.003%
36	5.433	1363	1366	1369	rBV2	569	416	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
 Data File : VV034916.D
 Acq On : 01 Apr 2024 11:12
 Operator : SY/MD
 Sample : P1934-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.461	1373	1375	1377	rVB2	432	191	0.01%	0.002%
38	5.532	1386	1397	1431	rBV	423338	884703	56.63%	7.735%
39	5.831	1481	1490	1504	rVB3	16176	33492	2.14%	0.293%
40	5.986	1526	1538	1572	rBV	340256	718227	45.97%	6.279%
41	6.407	1665	1669	1672	rBV3	617	524	0.03%	0.005%
42	6.439	1676	1679	1682	rBV3	373	304	0.02%	0.003%
43	6.490	1693	1695	1700	rVV4	362	266	0.02%	0.002%
44	6.529	1704	1707	1710	rBV2	429	282	0.02%	0.002%
45	6.619	1731	1735	1737	rBV4	566	359	0.02%	0.003%
46	6.696	1756	1759	1766	rVB3	930	666	0.04%	0.006%
47	6.777	1777	1784	1787	rBV3	857	864	0.06%	0.008%
48	6.793	1787	1789	1791	rVB	486	230	0.01%	0.002%
49	6.825	1797	1799	1802	rVB	344	181	0.01%	0.002%
50	6.857	1807	1809	1812	rBV2	312	152	0.01%	0.001%
51	6.912	1816	1826	1859	rBV	174052	337989	21.63%	2.955%
52	7.150	1896	1900	1902	rBV3	525	387	0.02%	0.003%
53	7.243	1918	1929	1963	rBV	672114	1197977	76.68%	10.473%
54	7.551	2017	2025	2049	rBV	114881	213609	13.67%	1.867%
55	7.725	2077	2079	2083	rBV3	734	534	0.03%	0.005%
56	7.834	2110	2113	2118	rVB3	763	639	0.04%	0.006%
57	7.863	2118	2122	2123	rBV3	686	335	0.02%	0.003%
58	7.924	2138	2141	2142	rBV2	353	166	0.01%	0.001%
59	8.027	2163	2173	2214	rBV2	304938	686828	43.96%	6.005%
60	8.461	2306	2308	2313	rBV4	761	565	0.04%	0.005%
61	8.706	2381	2384	2388	rBV4	547	491	0.03%	0.004%
62	8.741	2392	2395	2396	rBV	327	183	0.01%	0.002%
63	8.783	2396	2408	2437	rBV	630533	1067714	68.34%	9.335%
64	9.249	2550	2553	2555	rBV3	406	313	0.02%	0.003%
65	9.313	2572	2573	2575	rBV3	312	161	0.01%	0.001%
66	9.339	2579	2581	2583	rVB	355	147	0.01%	0.001%
67	9.387	2592	2596	2600	rBV2	632	545	0.03%	0.005%
68	9.413	2602	2604	2609	rBV2	467	359	0.02%	0.003%
69	9.439	2609	2612	2614	rBV3	476	313	0.02%	0.003%
70	9.519	2634	2637	2640	rBV3	620	352	0.02%	0.003%
71	9.555	2645	2648	2652	rBV	415	302	0.02%	0.003%
72	9.654	2672	2679	2681	rBV2	575	681	0.04%	0.006%
73	9.789	2718	2721	2722	rBV2	450	257	0.02%	0.002%
74	9.860	2740	2743	2744	rBV	285	153	0.01%	0.001%
75	9.950	2769	2771	2777	rBV3	256	226	0.01%	0.002%
76	9.989	2780	2783	2785	rBV2	332	230	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
 Data File : VV034916.D
 Acq On : 01 Apr 2024 11:12
 Operator : SY/MD
 Sample : P1934-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R42

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.024	2791	2794	2801	rBV	350	318	0.02%	0.003%
78	10.053	2801	2803	2806	rBV2	260	203	0.01%	0.002%
79	10.108	2818	2820	2822	rBV	285	164	0.01%	0.001%
80	10.149	2822	2833	2859	rVV	448125	716178	45.84%	6.261%
81	10.513	2944	2946	2948	rVB2	462	188	0.01%	0.002%
82	10.757	3020	3022	3024	rBV	252	139	0.01%	0.001%
83	10.895	3063	3065	3068	rVB3	414	184	0.01%	0.002%
84	11.130	3134	3138	3140	rBV2	695	585	0.04%	0.005%
85	11.185	3144	3155	3179	rBV	595124	932793	59.71%	8.155%
86	11.455	3237	3239	3242	rBV3	771	496	0.03%	0.004%
87	11.516	3255	3258	3259	rBV2	543	312	0.02%	0.003%
88	11.558	3260	3271	3296	rVV	627096	1012230	64.79%	8.849%
89	11.857	3362	3364	3369	rBV3	603	468	0.03%	0.004%
90	11.902	3376	3378	3380	rBV	363	210	0.01%	0.002%
91	11.921	3382	3384	3387	rVB2	469	190	0.01%	0.002%
92	11.976	3399	3401	3405	rBV	646	393	0.03%	0.003%
93	12.262	3487	3490	3492	rBV2	442	241	0.02%	0.002%
94	12.374	3523	3525	3526	rBV2	532	249	0.02%	0.002%
95	12.731	3632	3636	3639	rBV2	619	467	0.03%	0.004%
96	13.079	3742	3744	3746	rBV	529	249	0.02%	0.002%
97	13.207	3775	3784	3799	rBV3	8490	15233	0.98%	0.133%
98	13.612	3907	3910	3914	rBV2	785	712	0.05%	0.006%
99	13.683	3924	3932	3948	rBV8	5130	9382	0.60%	0.082%
100	13.747	3949	3952	3956	rBV	570	401	0.03%	0.004%




Sum of corrected areas: 11438340

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
Data File : VV034916.D
Acq On : 01 Apr 2024 11:12
Operator : SY/MD
Sample : P1934-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

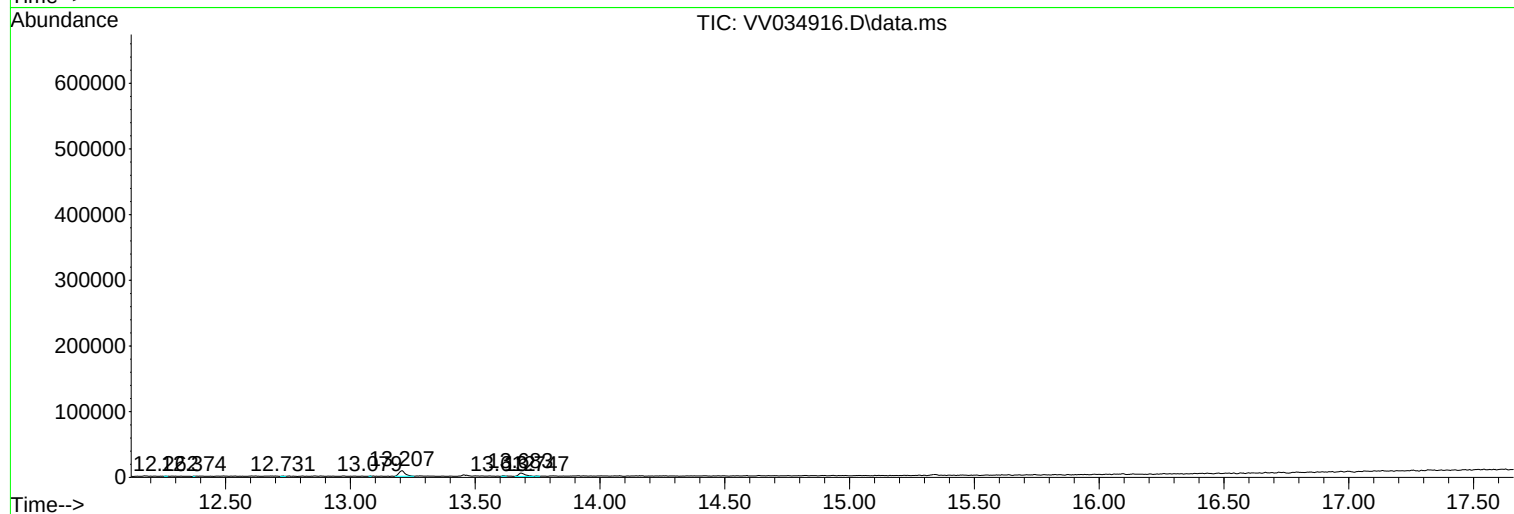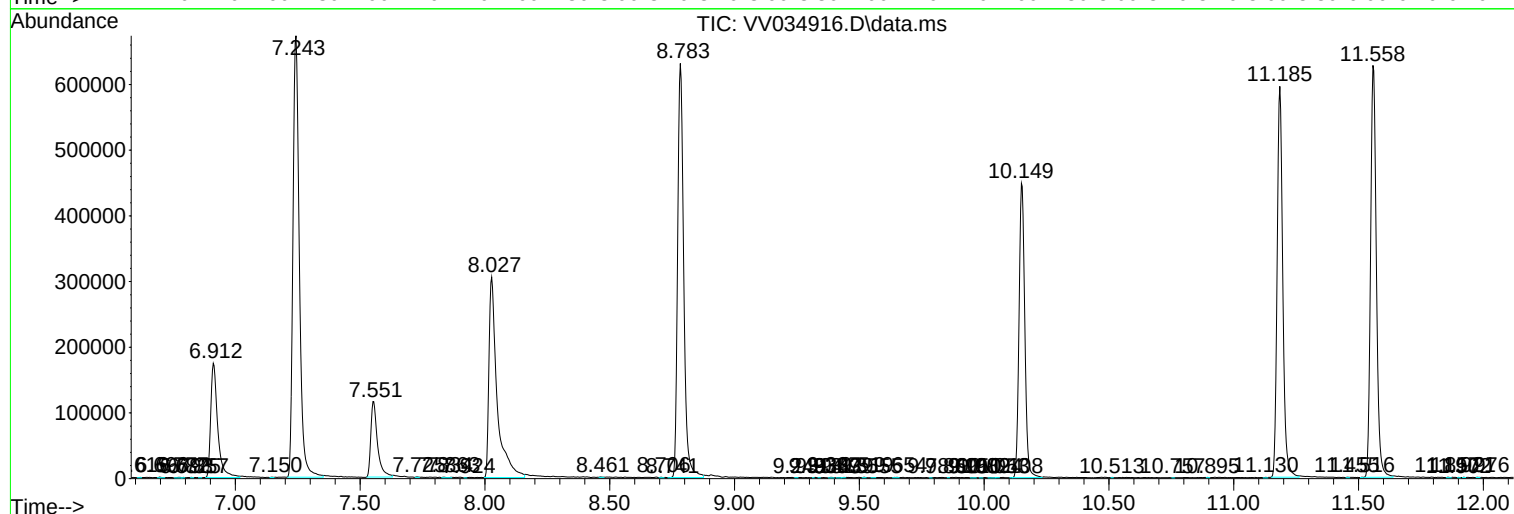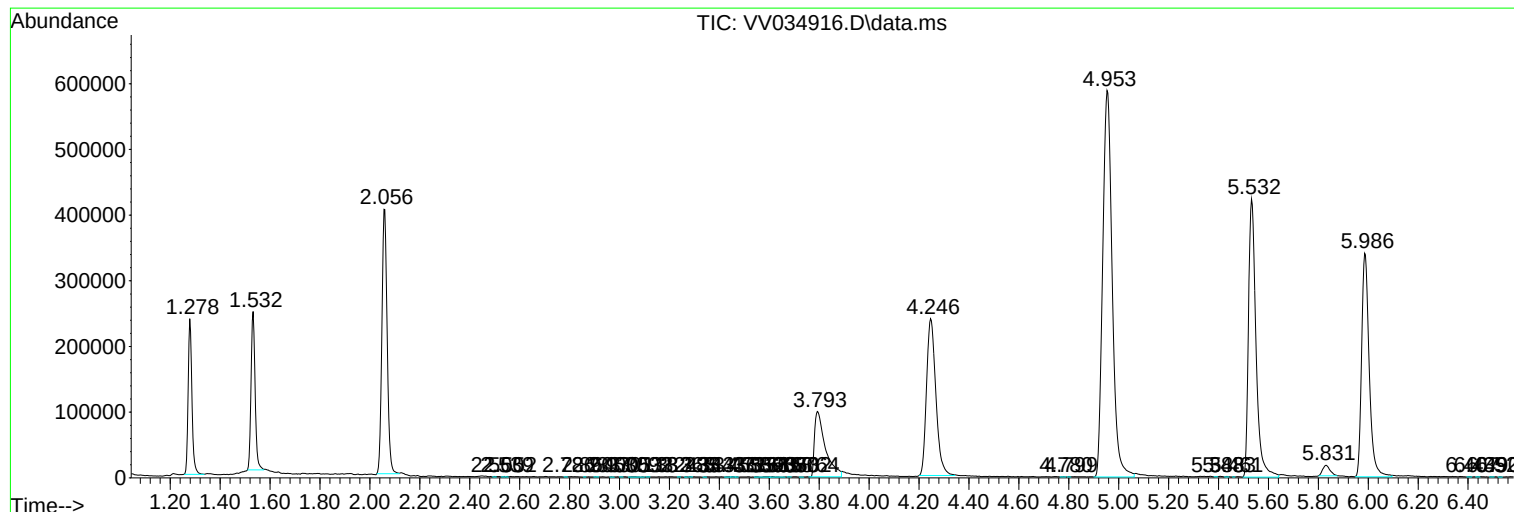

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
Data File : VV034916.D
Acq On : 01 Apr 2024 11:12
Operator : SY/MD
Sample : P1934-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
Data File : VV034916.D
Acq On : 01 Apr 2024 11:12
Operator : SY/MD
Sample : P1934-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
