

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
 Data File : VV034917.D
 Acq On : 01 Apr 2024 11:36
 Operator : SY/MD
 Sample : P1934-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034917.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	205669	220043	14.93%	2.042%
2	1.532	146	153	174	rVB	218118	252915	17.16%	2.347%
3	2.060	307	317	335	rBV	350631	513192	34.82%	4.763%
4	2.519	457	460	462	rBV2	661	467	0.03%	0.004%
5	2.683	508	511	513	rBV2	193	137	0.01%	0.001%
6	2.699	513	516	518	rVB2	437	272	0.02%	0.003%
7	2.715	518	521	522	rBV2	472	263	0.02%	0.002%
8	2.764	533	536	543	rVB	354	384	0.03%	0.004%
9	2.802	543	548	549	rBV2	440	357	0.02%	0.003%
10	2.847	560	562	565	rVB	569	306	0.02%	0.003%
11	2.870	565	569	570	rBV2	248	128	0.01%	0.001%
12	2.908	578	581	583	rVB2	476	225	0.02%	0.002%
13	2.924	583	586	587	rBV2	281	119	0.01%	0.001%
14	2.986	601	605	607	rBV2	310	247	0.02%	0.002%
15	3.031	615	619	620	rBV2	310	201	0.01%	0.002%
16	3.130	648	650	652	rBV2	315	177	0.01%	0.002%
17	3.223	675	679	684	rBV3	555	437	0.03%	0.004%
18	3.317	705	708	709	rBV	451	252	0.02%	0.002%
19	3.362	719	722	725	rVB2	535	371	0.03%	0.003%
20	3.458	749	752	753	rBV	243	127	0.01%	0.001%
21	3.522	765	772	779	rBV3	514	752	0.05%	0.007%
22	3.555	779	782	785	rBV	482	276	0.02%	0.003%
23	3.590	788	793	797	rVB3	521	437	0.03%	0.004%
24	3.616	799	801	803	rBV2	348	166	0.01%	0.002%
25	3.661	810	815	817	rBV3	257	221	0.01%	0.002%
26	3.686	817	823	827	rBV3	404	383	0.03%	0.004%
27	3.796	844	857	897	rBV	104059	335916	22.79%	3.118%
28	4.246	983	997	1029	rBV	229357	585792	39.75%	5.437%
29	4.754	1153	1155	1159	rBV2	638	380	0.03%	0.004%
30	4.863	1184	1189	1191	rBV2	389	352	0.02%	0.003%
31	4.953	1202	1217	1255	rBV2	553611	1473803	100.00%	13.678%
32	5.400	1352	1356	1358	rBV2	693	497	0.03%	0.005%
33	5.493	1381	1385	1386	rBV2	823	532	0.04%	0.005%
34	5.532	1386	1397	1436	rVV	382719	810157	54.97%	7.519%
35	5.831	1480	1490	1511	rBV2	14014	33467	2.27%	0.311%
36	5.985	1524	1538	1563	rBV	326506	684140	46.42%	6.349%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
 Data File : VV034917.D
 Acq On : 01 Apr 2024 11:36
 Operator : SY/MD
 Sample : P1934-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.333	1642	1646	1651	rBV3	291	244	0.02%	0.002%
38	6.445	1679	1681	1686	rVB	286	161	0.01%	0.001%
39	6.471	1686	1689	1690	rBV2	300	127	0.01%	0.001%
40	6.484	1690	1693	1697	rVB3	583	320	0.02%	0.003%
41	6.500	1697	1698	1701	rBV2	210	131	0.01%	0.001%
42	6.526	1704	1706	1711	rVB3	430	244	0.02%	0.002%
43	6.567	1715	1719	1721	rBV3	492	321	0.02%	0.003%
44	6.632	1735	1739	1740	rBV	367	204	0.01%	0.002%
45	6.645	1740	1743	1746	rBV	416	290	0.02%	0.003%
46	6.667	1746	1750	1753	rVV3	402	346	0.02%	0.003%
47	6.770	1779	1782	1784	rBV3	568	301	0.02%	0.003%
48	6.844	1803	1805	1806	rBV	336	139	0.01%	0.001%
49	6.911	1816	1826	1853	rBV	160363	315560	21.41%	2.929%
50	7.243	1918	1929	1958	rBV	617089	1086552	73.72%	10.084%
51	7.554	2016	2026	2052	rBV	109424	209061	14.19%	1.940%
52	7.857	2118	2120	2121	rBV	368	118	0.01%	0.001%
53	7.902	2130	2134	2135	rBV	399	235	0.02%	0.002%
54	7.972	2153	2156	2158	rBV2	708	430	0.03%	0.004%
55	8.027	2164	2173	2220	rBV2	303468	696225	47.24%	6.461%
56	8.667	2367	2372	2373	rBV2	557	395	0.03%	0.004%
57	8.725	2388	2390	2391	rBV	323	171	0.01%	0.002%
58	8.783	2397	2408	2444	rBV	595019	998896	67.78%	9.270%
59	9.220	2542	2544	2547	rVB	417	182	0.01%	0.002%
60	9.265	2556	2558	2559	rBV	295	115	0.01%	0.001%
61	9.307	2569	2571	2575	rBV3	432	254	0.02%	0.002%
62	9.368	2587	2590	2592	rBV	448	310	0.02%	0.003%
63	9.400	2597	2600	2602	rBV2	513	287	0.02%	0.003%
64	9.625	2667	2670	2675	rBV2	695	693	0.05%	0.006%
65	9.709	2693	2696	2698	rBV2	321	214	0.01%	0.002%
66	9.779	2713	2718	2720	rBV2	403	323	0.02%	0.003%
67	9.828	2730	2733	2734	rBV2	308	163	0.01%	0.002%
68	9.937	2765	2767	2769	rVB	349	149	0.01%	0.001%
69	9.956	2771	2773	2775	rBV	278	123	0.01%	0.001%
70	9.992	2780	2784	2785	rBV	361	206	0.01%	0.002%
71	10.072	2804	2809	2810	rBV2	478	397	0.03%	0.004%
72	10.149	2821	2833	2862	rBV	445180	716256	48.60%	6.647%
73	10.349	2893	2895	2897	rBV2	438	210	0.01%	0.002%
74	10.593	2969	2971	2973	rBV	238	168	0.01%	0.002%
75	10.628	2979	2982	2983	rBV2	443	261	0.02%	0.002%
76	10.728	3011	3013	3016	rBV	246	117	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
 Data File : VV034917.D
 Acq On : 01 Apr 2024 11:36
 Operator : SY/MD
 Sample : P1934-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.783	3026	3030	3032	rBV	189	146	0.01%	0.001%
78	10.796	3032	3034	3035	rBV	324	132	0.01%	0.001%
79	10.908	3066	3069	3071	rBV	426	271	0.02%	0.003%
80	11.014	3100	3102	3104	rBV	288	126	0.01%	0.001%
81	11.062	3114	3117	3119	rVB3	506	255	0.02%	0.002%
82	11.104	3127	3130	3134	rVB	312	166	0.01%	0.002%
83	11.130	3134	3138	3142	rBV2	528	403	0.03%	0.004%
84	11.185	3144	3155	3182	rBV	547678	865572	58.73%	8.033%
85	11.467	3240	3243	3244	rBV3	624	342	0.02%	0.003%
86	11.558	3260	3271	3297	rBV	589252	951002	64.53%	8.826%
87	11.969	3397	3399	3401	rBV2	641	383	0.03%	0.004%
88	12.027	3415	3417	3421	rBV2	460	205	0.01%	0.002%
89	12.168	3456	3461	3462	rBV2	447	278	0.02%	0.003%
90	12.606	3595	3597	3599	rVB	458	155	0.01%	0.001%
91	12.654	3607	3612	3614	rBV2	596	588	0.04%	0.005%
92	12.754	3634	3643	3646	rBV2	812	1072	0.07%	0.010%
93	12.805	3656	3659	3661	rBV2	276	169	0.01%	0.002%
94	12.860	3674	3676	3679	rBV2	426	290	0.02%	0.003%
95	13.146	3763	3765	3770	rBV3	698	420	0.03%	0.004%
96	13.184	3775	3777	3778	rBV	350	123	0.01%	0.001%
97	13.210	3778	3785	3795	rBV6	2103	3322	0.23%	0.031%
98	13.747	3950	3952	3955	rBV2	522	287	0.02%	0.003%
99	13.956	4015	4017	4021	rBV2	483	292	0.02%	0.003%
100	14.098	4058	4061	4062	rBV2	419	256	0.02%	0.002%




Sum of corrected areas: 10775045

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
Data File : VV034917.D
Acq On : 01 Apr 2024 11:36
Operator : SY/MD
Sample : P1934-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

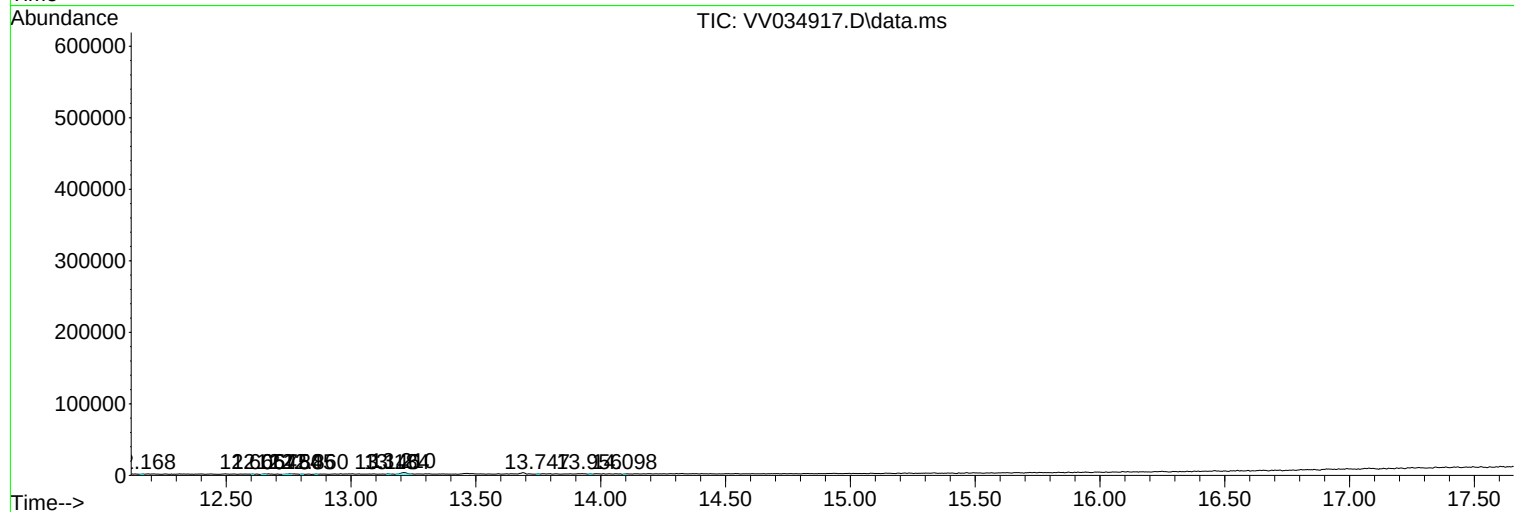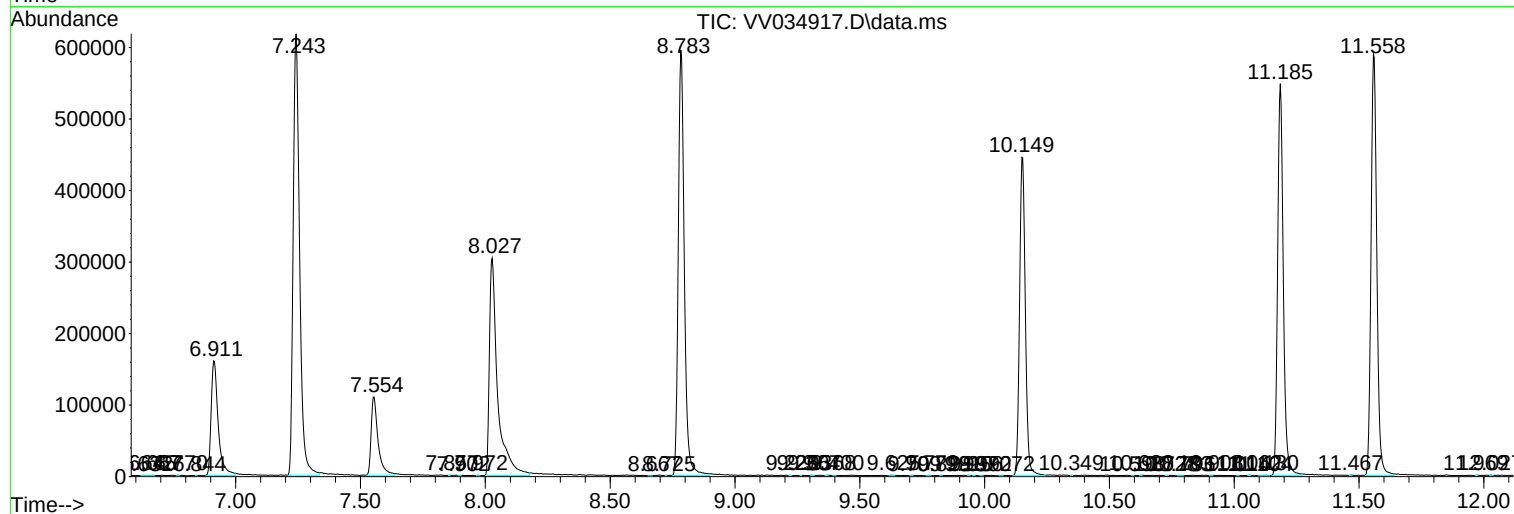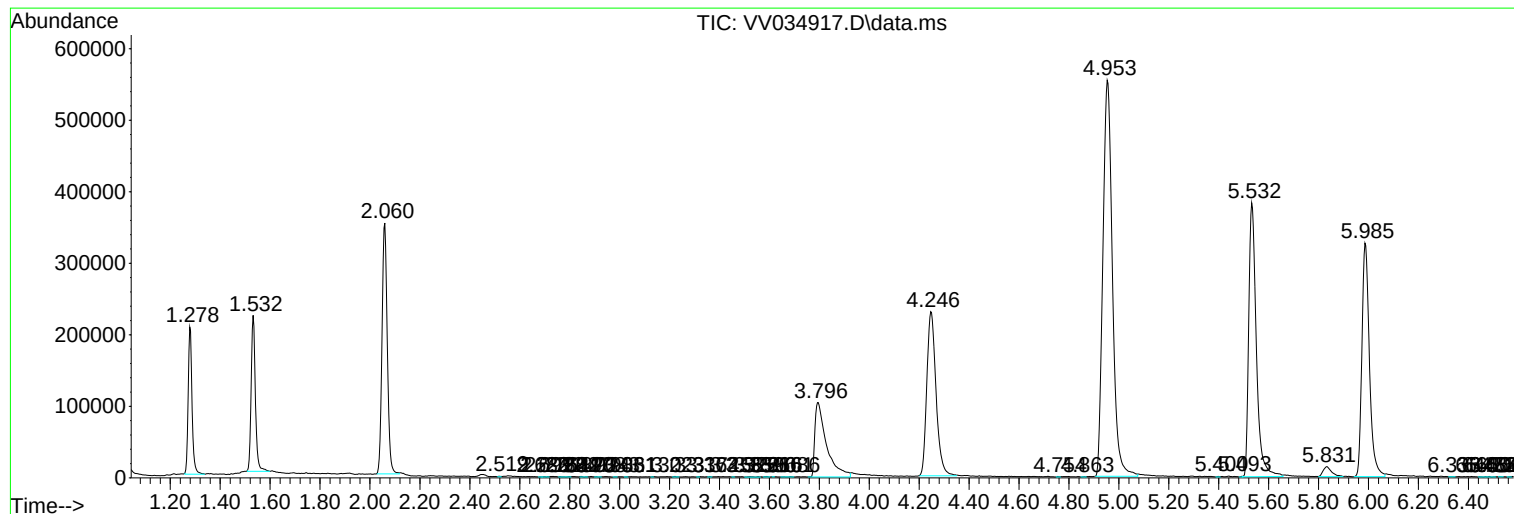

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
Data File : VV034917.D
Acq On : 01 Apr 2024 11:36
Operator : SY/MD
Sample : P1934-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
Data File : VV034917.D
Acq On : 01 Apr 2024 11:36
Operator : SY/MD
Sample : P1934-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------