
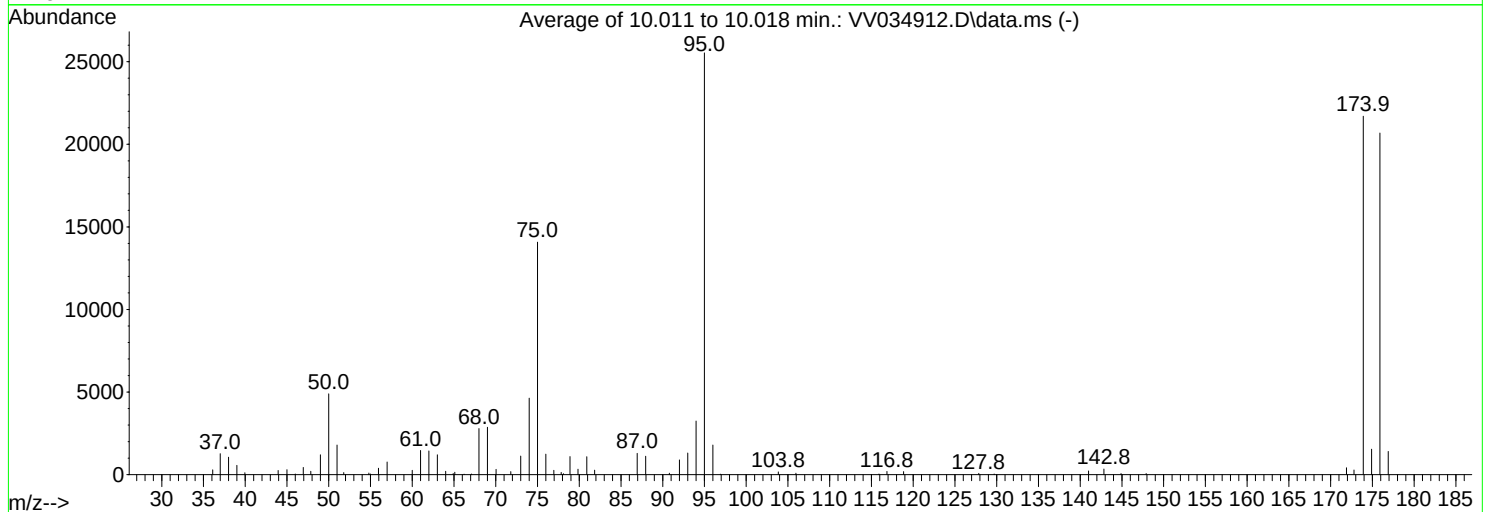


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040124\
Data File : VV034912.D
Acq On : 01 Apr 2024 08:22
Operator : SY/MD
Sample : BFB279
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB279

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis
Last Update : Tue Apr 02 02:07:06 2024

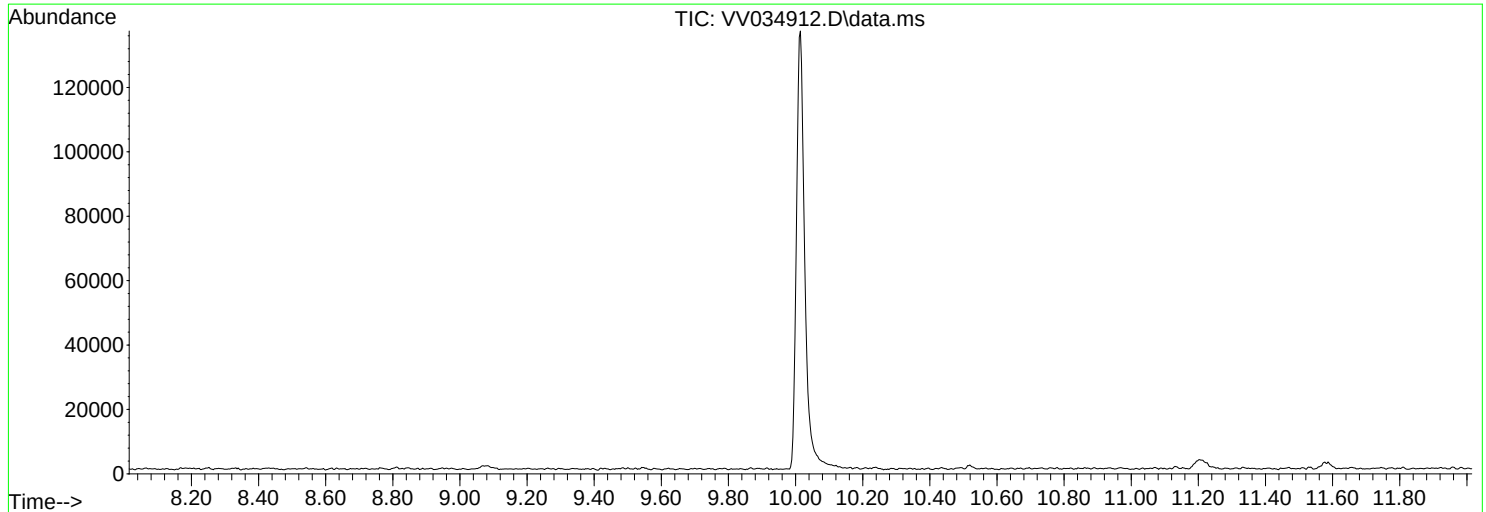

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2780

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	4893	PASS
75	95	30	80	55.1	14071	PASS
95	95	100	100	100.0	25536	PASS
96	95	5	9	7.0	1794	PASS
173	174	0.00	2	1.3	280	PASS
174	95	50	120	85.0	21696	PASS
175	174	5	9	7.1	1539	PASS
176	174	95	105	95.3	20680	PASS
177	176	5	10	6.8	1404	PASS

m/z	Abundance
39.00	137.0
39.90	1116.0
44.00	277.0

Instrument :
MSVOA_V
ClientSampleId :
BFB279

m/z	Abundance
36.10	291.0
37.00	1358.0
38.00	1121.0
39.00	704.0
40.00	1124.0
44.00	536.0
45.00	305.0
47.00	427.0
47.80	214.0
49.00	1159.0
50.00	4975.0
51.00	1801.0
51.80	118.0
54.80	175.0
56.00	463.0
57.00	805.0
60.00	265.0
61.00	1457.0
62.00	1541.0
63.00	1274.0
64.00	199.0
64.90	191.0
67.10	111.0
68.00	2899.0
69.00	2884.0
70.00	331.0
71.90	238.0
73.00	1139.0
74.00	4785.0
75.00	14522.0
76.00	1268.0
77.00	247.0
78.10	165.0
78.90	1151.0
79.80	318.0
80.90	1117.0
81.90	268.0
87.00	1259.0
88.00	1170.0
92.00	945.0
93.00	1361.0
94.00	3255.0
95.00	26216.0
96.00	1855.0
96.90	100.0
103.80	161.0
106.00	155.0
115.90	114.0
116.80	211.0
118.90	170.0
129.70	109.0
140.90	229.0
142.80	343.0
145.00	105.0
147.90	110.0
171.90	405.0
172.80	252.0
173.90	21752.0
174.90	1531.0
175.90	20352.0
176.90	1478.0

Instrument :
MSVOA_V
ClientSampleId :
BFB279

m/z	Abundance
36.10	293.0
37.00	1298.0
38.00	1074.0
39.00	732.0
40.00	1262.0
43.90	526.0
45.00	308.0
47.00	461.0
47.80	192.0
49.00	1217.0
50.00	5011.0
51.00	1861.0
51.80	128.0
54.80	132.0
56.00	389.0
57.00	777.0
60.00	278.0
61.00	1546.0
62.00	1486.0
63.00	1246.0
64.00	217.0
65.10	205.0
66.20	100.0
68.00	2864.0
69.00	2993.0
70.10	330.0
71.80	175.0
73.00	1123.0
74.00	4706.0
75.00	14548.0
76.00	1287.0
76.90	263.0
77.80	184.0
78.90	1116.0
79.90	328.0
80.90	1134.0
81.80	269.0
86.90	1357.0
87.90	1128.0
90.80	113.0
92.00	921.0
93.00	1344.0
94.00	3419.0
95.00	26344.0
96.00	1813.0
103.80	172.0
105.90	111.0
116.90	199.0
118.90	194.0
127.80	105.0
141.00	226.0
142.80	343.0
147.90	103.0
171.90	450.0
172.80	304.0
173.90	22408.0
174.90	1596.0
175.90	21336.0
176.90	1458.0

Instrument :
MSVOA_V
ClientSampleId :
BFB279

m/z	Abundance
36.10	288.0
37.00	1151.0
38.00	976.0
39.00	662.0
40.00	1315.0
43.90	529.0
45.00	281.0
46.00	104.0
46.90	419.0
47.90	193.0
49.00	1218.0
50.00	4694.0
51.00	1725.0
51.80	129.0
55.00	116.0
55.90	311.0
57.00	719.0
60.00	246.0
61.00	1395.0
62.00	1285.0
63.00	1083.0
64.00	203.0
65.10	226.0
68.00	2612.0
69.00	2732.0
70.10	295.0
71.70	142.0
73.00	1097.0
74.00	4413.0
75.00	13144.0
76.00	1171.0
76.90	263.0
77.90	215.0
78.90	1011.0
79.90	331.0
80.90	1013.0
81.80	288.0
86.90	1257.0
87.90	1047.0
90.80	151.0
92.00	821.0
93.00	1228.0
94.00	3056.0
95.00	24048.0
96.00	1714.0
103.90	168.0
116.90	168.0
118.80	196.0
127.90	123.0
141.10	223.0
142.90	325.0
144.80	103.0
171.90	408.0
172.80	283.0
173.90	20928.0
174.90	1491.0
175.90	20352.0
176.90	1277.0

Instrument :
MSVOA_V
ClientSampleId :
BFB279