


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV040219\
 Data File : VV010055.D
 Acq On : 02 Apr 2019 10:50
 Operator : SY/MD
 Sample : BFB82
 Misc : 5.00G/10mL/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB82

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040219S.M
 Title : VOC Analysis
 Last Update : Fri Apr 05 01:26:41 2019

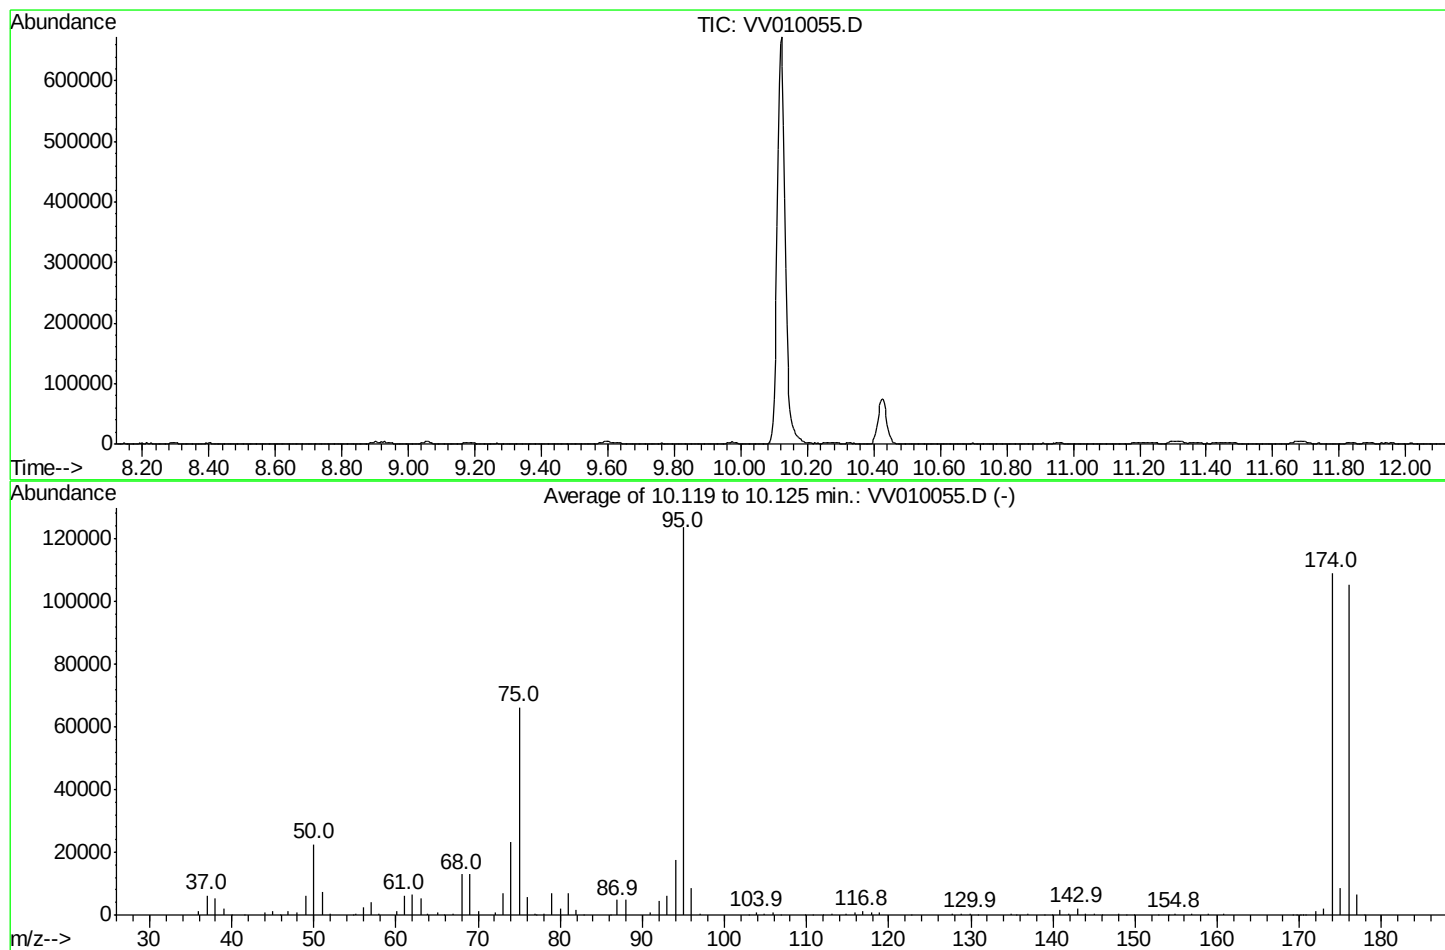

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	22520	PASS
75	95	30	80	53.6	66232	PASS
95	95	100	100	100.0	123640	PASS
96	95	5	9	7.0	8619	PASS
173	174	0.00	2	1.9	2045	PASS
174	95	50	120	88.2	109037	PASS
175	174	5	9	7.8	8526	PASS
176	174	95	101	96.6	105288	PASS
177	176	5	9	6.2	6529	PASS

Scan 2794 (10.074 min): VV010055.D
BFB82

m/z	Abundance
40.10	128.0
44.20	364.0
97.60	116.0
207.00	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
36.00	1218.0
37.00	6288.0
38.00	5802.0
39.00	2431.0
40.00	226.0
41.60	108.0
44.00	1398.0
45.00	1356.0
45.90	165.0
46.90	1273.0
48.00	868.0
49.00	6234.0
50.00	23696.0
51.00	7326.0
51.90	467.0
54.80	339.0
55.10	336.0
56.00	2675.0
57.00	4209.0
57.90	236.0
60.10	1416.0
61.00	6594.0
62.00	6364.0
63.10	5556.0
63.80	513.0
65.10	561.0
67.00	218.0
68.00	13455.0
69.00	13779.0
70.00	1186.0
72.00	954.0
73.00	6582.0
74.00	24496.0
75.00	67216.0
76.00	6034.0
76.90	575.0
78.00	665.0
78.90	7142.0
80.00	1889.0
80.90	6776.0
81.90	1694.0
82.90	188.0
86.90	4875.0
88.00	5241.0
91.00	772.0
92.00	4507.0
93.00	6353.0
94.00	17968.0
95.00	125360.0
96.00	9229.0
97.00	287.0
103.90	918.0
104.80	291.0
105.90	900.0
106.80	110.0
109.80	188.0
110.80	171.0
111.90	156.0
113.00	250.0
114.80	198.0
116.00	619.0
116.80	1384.0
117.90	693.0
118.90	1023.0
127.80	448.0
128.80	267.0
130.00	620.0
130.90	266.0
134.80	242.0
136.90	353.0
139.90	175.0
140.90	1512.0
141.90	256.0
142.90	2198.0
143.90	246.0
145.00	453.0
145.90	219.0
148.00	278.0
149.00	128.0
149.80	170.0
152.90	109.0
154.10	139.0
154.90	506.0
156.80	318.0
158.80	267.0
160.80	290.0
169.10	158.0
169.70	181.0
170.50	184.0
172.00	995.0
173.00	2049.0
174.00	109320.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

175.00	8455.0
176.00	103808.0
177.00	6584.0
177.80	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
36.00	1125.0
37.00	6440.0
38.00	5522.0
39.10	2298.0
40.00	177.0
41.60	103.0
44.00	1283.0
45.00	1389.0
45.90	188.0
46.90	1268.0
48.00	930.0
49.00	6195.0
50.00	23048.0
51.00	7590.0
51.90	501.0
55.10	322.0
56.00	2551.0
57.00	4222.0
58.00	295.0
60.00	1194.0
61.00	6454.0
62.00	6719.0
63.10	5515.0
63.80	408.0
65.00	684.0
65.90	109.0
67.00	261.0
68.00	13231.0
69.00	13490.0
70.00	1252.0
72.10	1023.0
73.00	7071.0
74.00	23784.0
75.00	68648.0
76.10	5844.0
76.90	535.0
78.00	645.0
78.90	7223.0
80.00	1930.0
80.90	7156.0
81.90	1800.0
82.90	169.0
86.10	228.0
86.90	5004.0
88.00	4856.0
91.00	802.0
92.00	4463.0
93.00	6133.0
94.00	17984.0
95.00	127096.0
96.00	8841.0
97.00	242.0
103.90	849.0
104.80	293.0
105.90	780.0
106.80	160.0
109.80	125.0
110.80	179.0
112.00	191.0
113.00	268.0
114.90	248.0
116.00	693.0
116.80	1504.0
117.90	722.0
118.80	916.0
122.80	101.0
127.80	499.0
128.80	287.0
129.90	608.0
130.90	183.0
134.80	241.0
135.50	108.0
137.00	362.0
139.80	116.0
140.90	1445.0
142.00	230.0
142.90	2196.0
143.90	296.0
145.00	297.0
145.90	239.0
148.00	363.0
149.80	207.0
152.90	107.0
154.00	110.0
154.90	577.0
156.90	295.0
158.90	260.0
160.70	275.0
169.20	112.0
169.70	166.0
172.00	1066.0
173.00	2144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

174.00	112320.0
175.00	8795.0
176.00	108792.0
177.00	6717.0
177.90	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
35.90	964.0
37.00	5863.0
38.00	4747.0
39.10	1979.0
39.90	131.0
44.00	1227.0
45.00	1326.0
45.90	153.0
46.90	1043.0
48.00	850.0
49.00	5629.0
50.00	20816.0
51.00	6839.0
51.90	467.0
55.10	241.0
56.00	2200.0
57.00	3686.0
58.00	278.0
60.00	1046.0
61.00	5705.0
62.00	6410.0
63.00	5279.0
63.80	348.0
65.00	747.0
67.00	274.0
68.00	12204.0
69.00	12142.0
70.00	1223.0
72.10	863.0
73.00	6727.0
74.00	21280.0
75.00	62832.0
76.10	5051.0
77.10	525.0
77.90	568.0
78.90	6790.0
80.00	1803.0
80.90	7227.0
81.90	1737.0
82.90	153.0
86.90	4582.0
88.00	4048.0
90.90	758.0
92.00	4004.0
93.00	5463.0
94.00	16624.0
95.00	118464.0
96.00	7788.0
96.90	196.0
102.90	125.0
103.90	757.0
104.80	328.0
106.00	659.0
106.80	187.0
110.80	119.0
112.00	209.0
113.00	243.0
114.90	224.0
115.90	745.0
116.80	1312.0
117.90	681.0
118.80	858.0
127.80	505.0
128.80	263.0
129.90	611.0
134.90	268.0
137.00	349.0
138.90	113.0
140.90	1437.0
142.00	186.0
143.00	1977.0
143.90	256.0
145.00	193.0
146.00	183.0
148.00	396.0
149.90	245.0
154.80	664.0
157.00	252.0
158.80	272.0
160.70	240.0
169.30	138.0
169.60	115.0
170.20	104.0
170.80	223.0
172.00	1172.0
173.00	1944.0
174.00	105472.0
175.00	8328.0
176.00	103264.0
177.00	6288.0
178.00	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82