
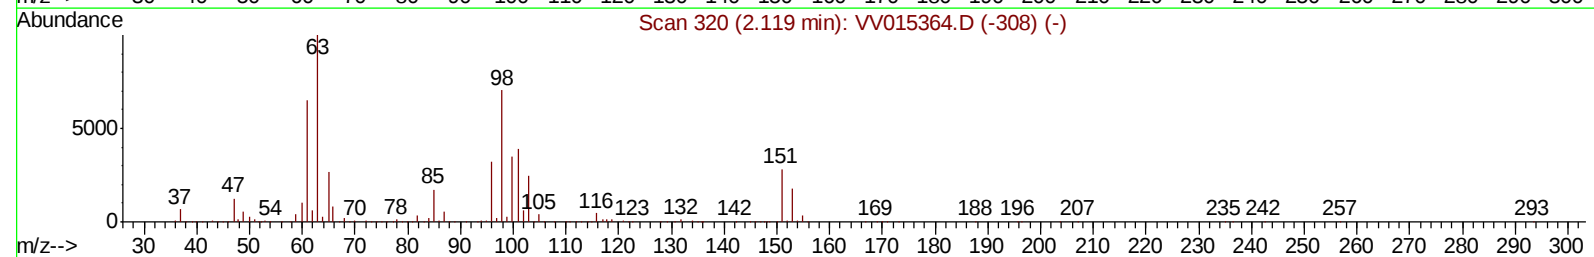
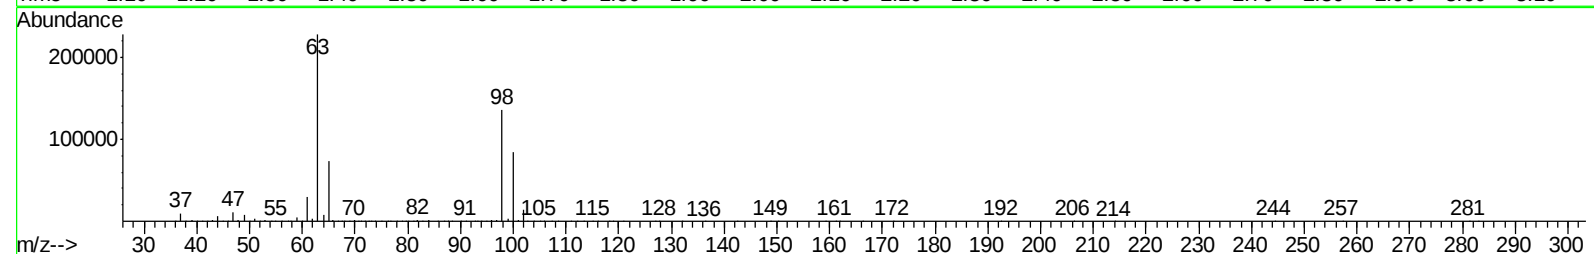


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
Data File : VV015376.D
Acq On : 02 Apr 2020 16:01
Operator : SY/MD
Sample : VIBLK64
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 01:34:06 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 03 01:25:45 2020
Response via : Initial Calibration

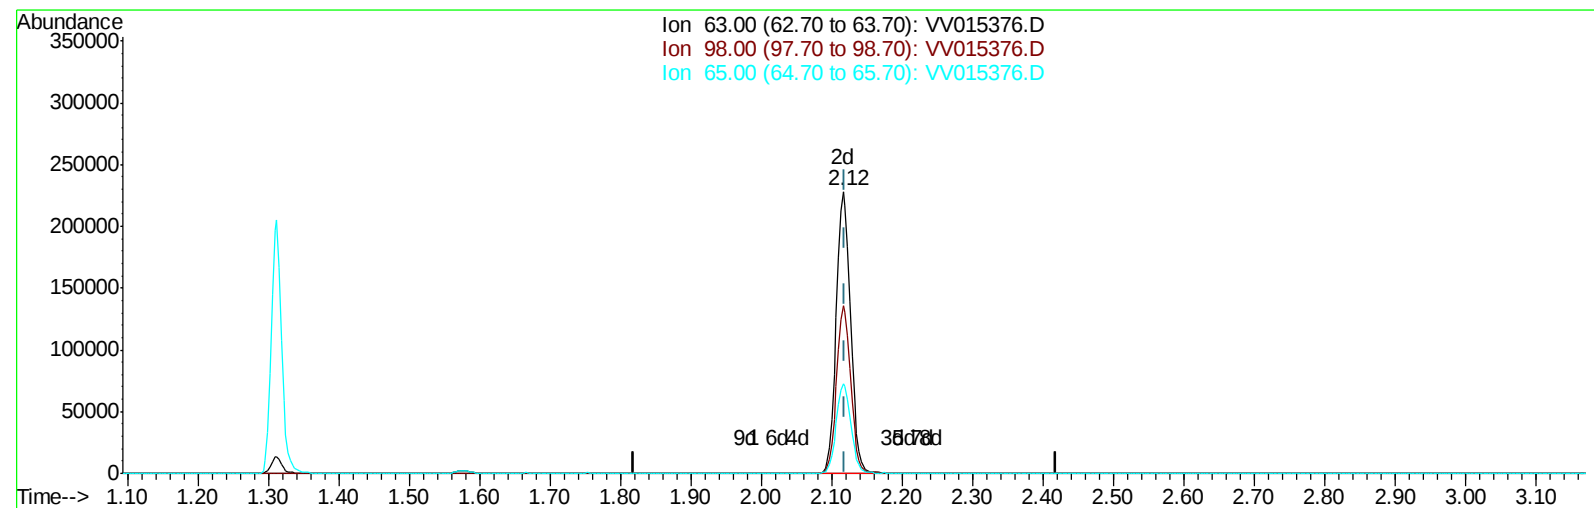

TIC: VV015376.D

(11) 1,1-Dichloroethene-d2 (S)

2.116min (-0.003) 31.07ug/L m

response 321424

Ion	Exp%	Act%
63.00	100	100
98.00	73.70	0.06#
65.00	24.00	0.02#
0.00	0.00	0.00