

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015379.D
 Acq On : 02 Apr 2020 17:14
 Operator : SY/MD
 Sample : L2003-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL6

Manual Integrations
 APPROVED

sam
 4/3/2020 5:50:04 PM

Quant Time: Apr 03 01:34:37 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 03 01:25:45 2020
 Response via : Initial Calibration

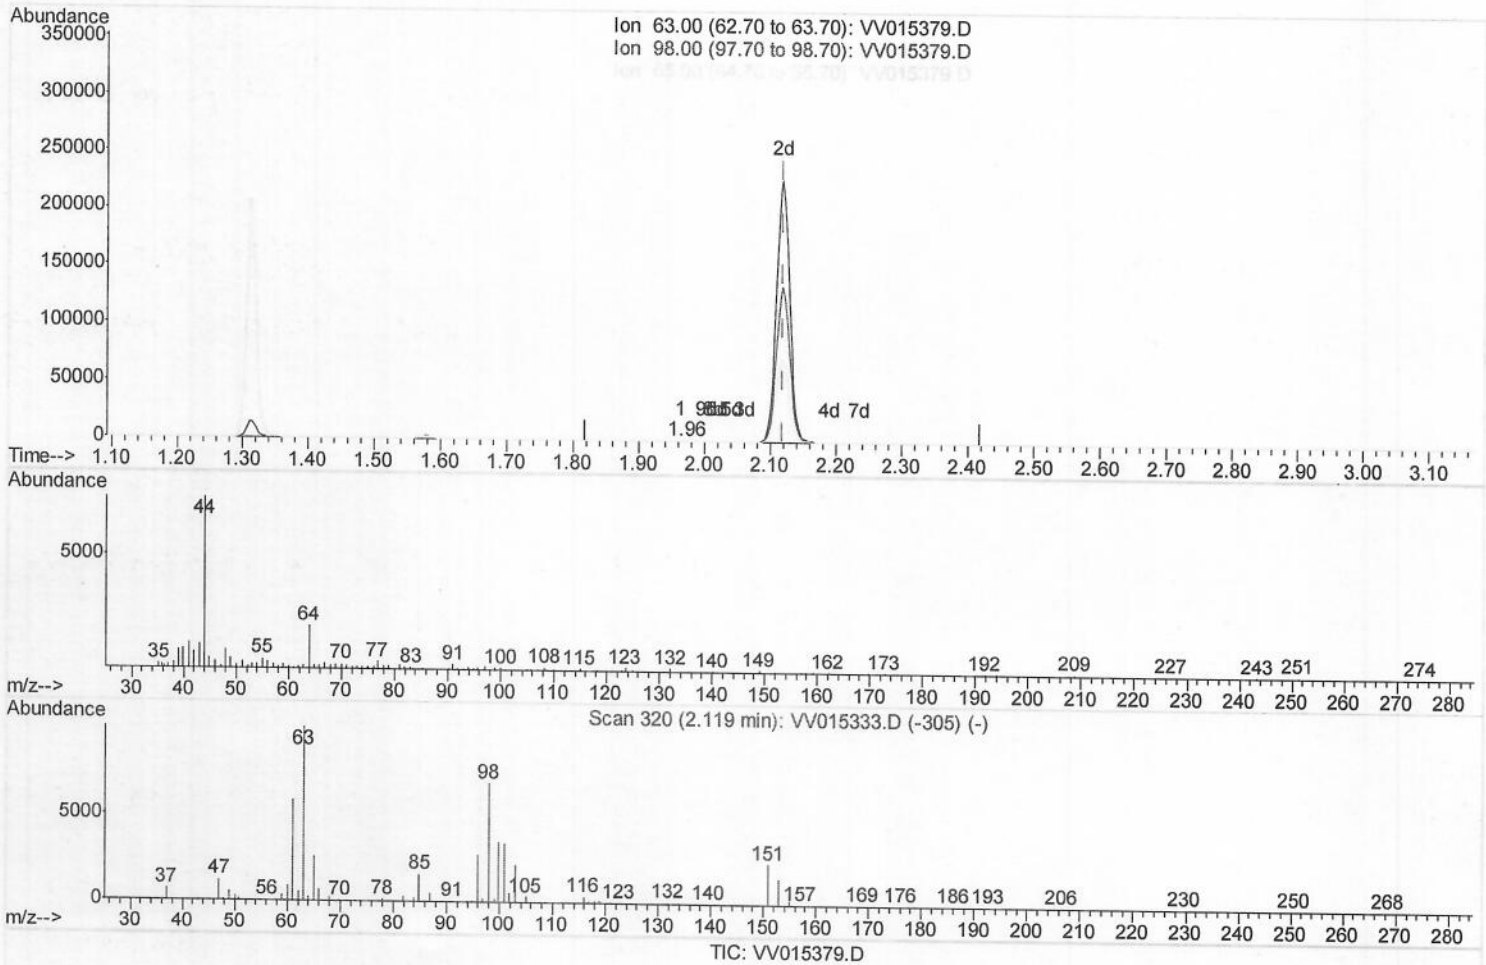

(11) 1,1-Dichloroethene-d2 (S)

1.965min (-0.154) 0.02ug/L

response 266

Ion	Exp%	Act%
63.00	100	100
98.00	73.70	54.14
65.00	24.00	17.67
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015379.D
 Acq On : 02 Apr 2020 17:14
 Operator : SY/MD
 Sample : L2003-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL6

Manual Integrations
 APPROVED

sam
 4/3/2020 5:50:04 PM

Quant Time: Apr 03 01:34:37 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 03 01:25:45 2020
 Response via : Initial Calibration

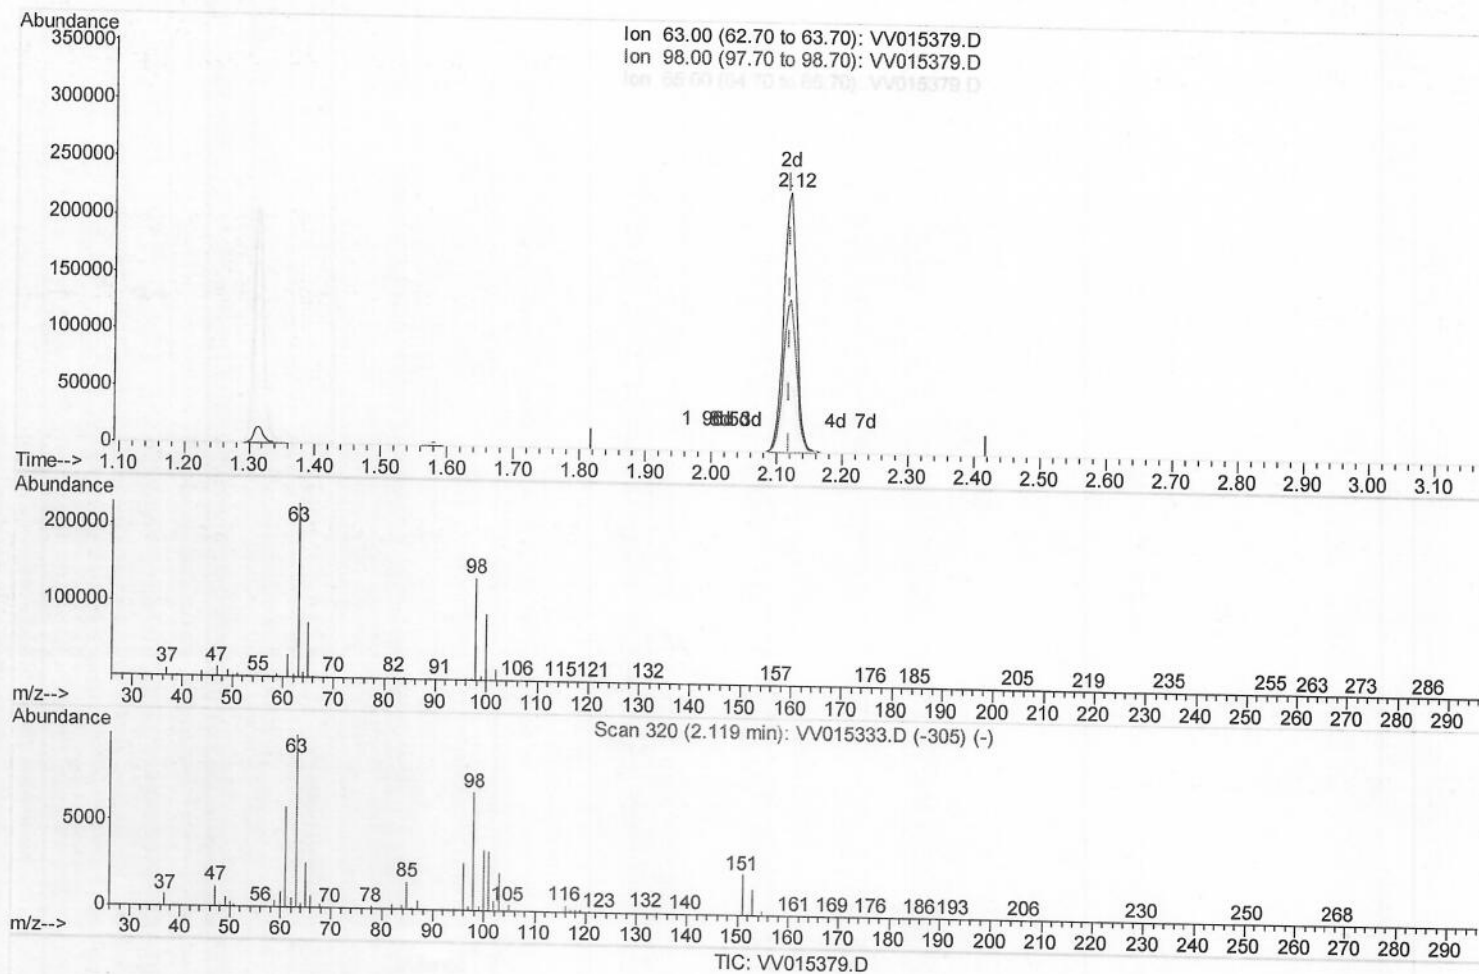

(11) 1,1-Dichloroethene-d2 (S)

2.119min (-0.000) 26.43ug/L m

response 317442

Ion	Exp%	Act%
63.00	100	100
98.00	73.70	0.05#
65.00	24.00	0.01#
0.00	0.00	0.00

MD
 04/3/2020

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015379.D
 Acq On : 02 Apr 2020 17:14
 Operator : SY/MD
 Sample : L2003-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL6

Manual Integrations
 APPROVED

sam
 4/3/2020 5:50:04 PM

Quant Time: Apr 03 01:34:37 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 03 01:25:45 2020
 Response via : Initial Calibration

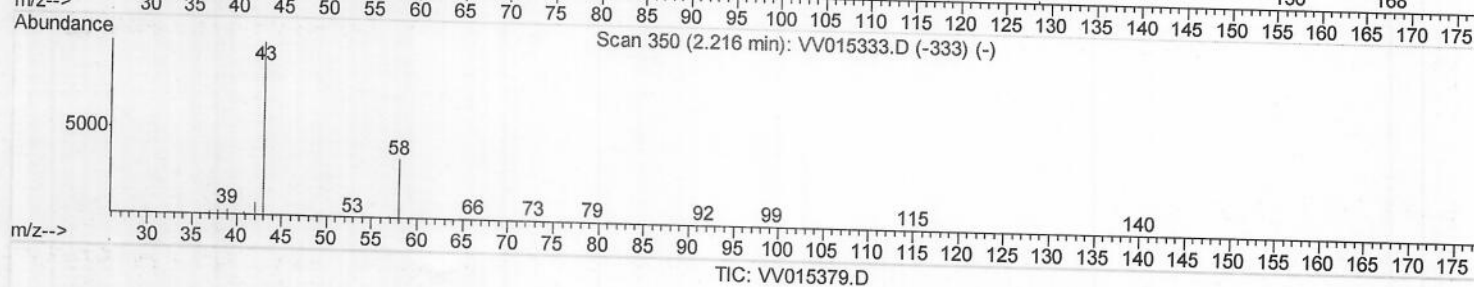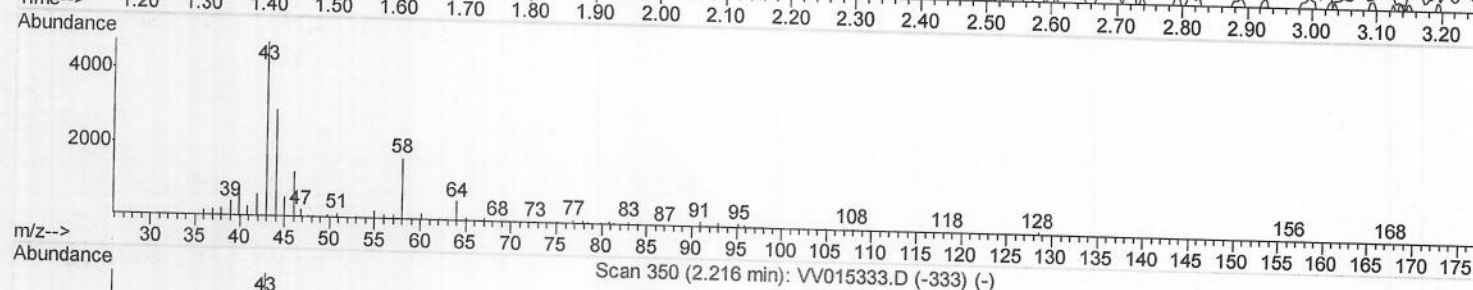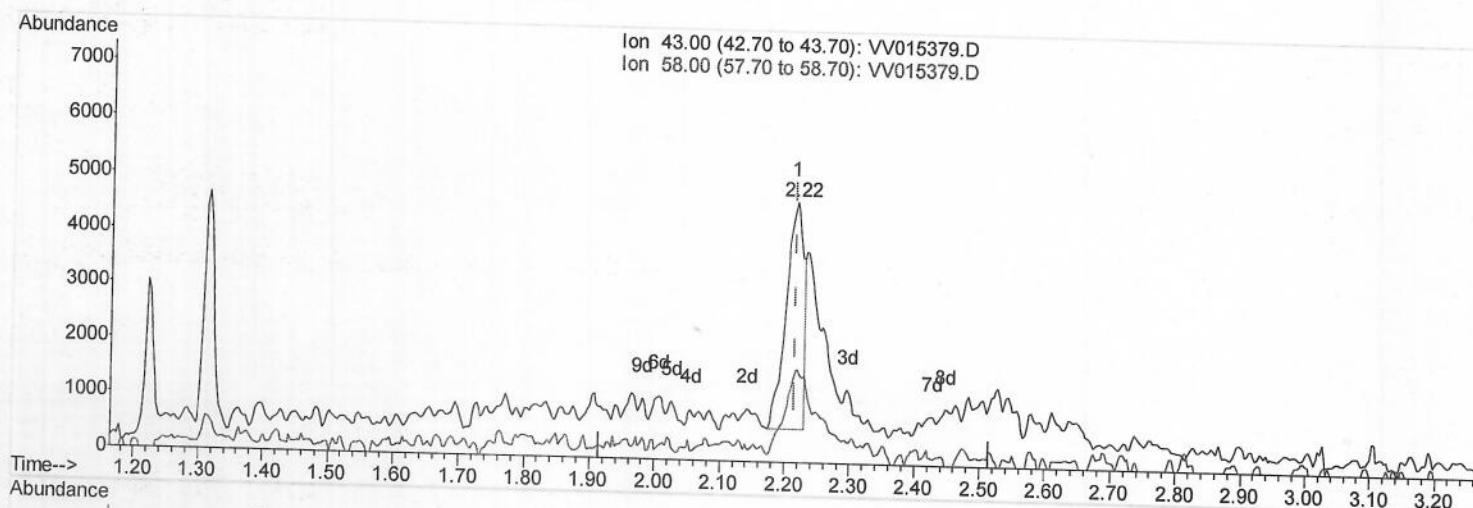

(13) Acetone (T)

2.216min (-0.000) 3.22ug/L

response 7548

Ion	Exp%	Act%
43.00	100	100
58.00	34.10	35.20
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
Data File : VV015379.D
Acq On : 02 Apr 2020 17:14
Operator : SY/MD
Sample : L2003-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL6

Manual Integrations
APPROVED

sam
4/3/2020 5:50:04 PM




Quant Time: Apr 03 01:34:37 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M

Quant Title : VOC Analysis

QLast Update : Fri Apr 03 01:25:45 2020

Response via : Initial Calibration

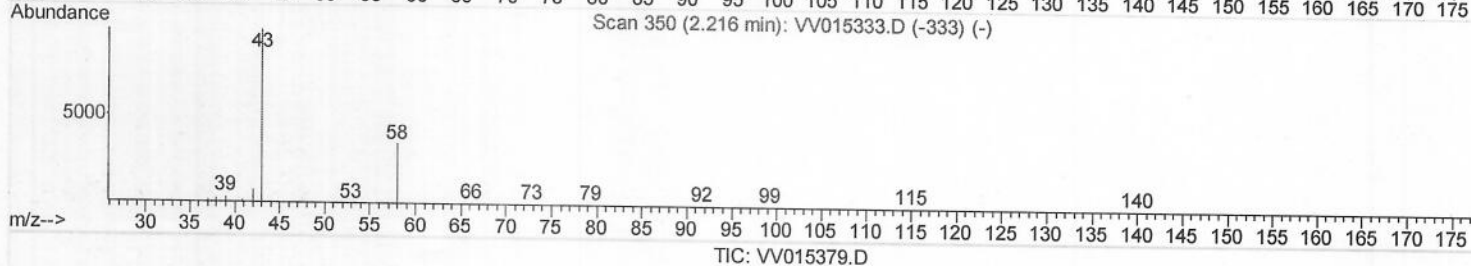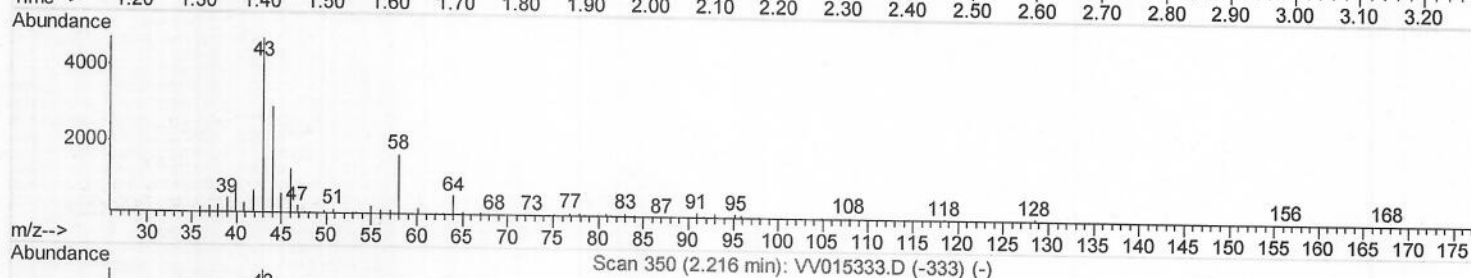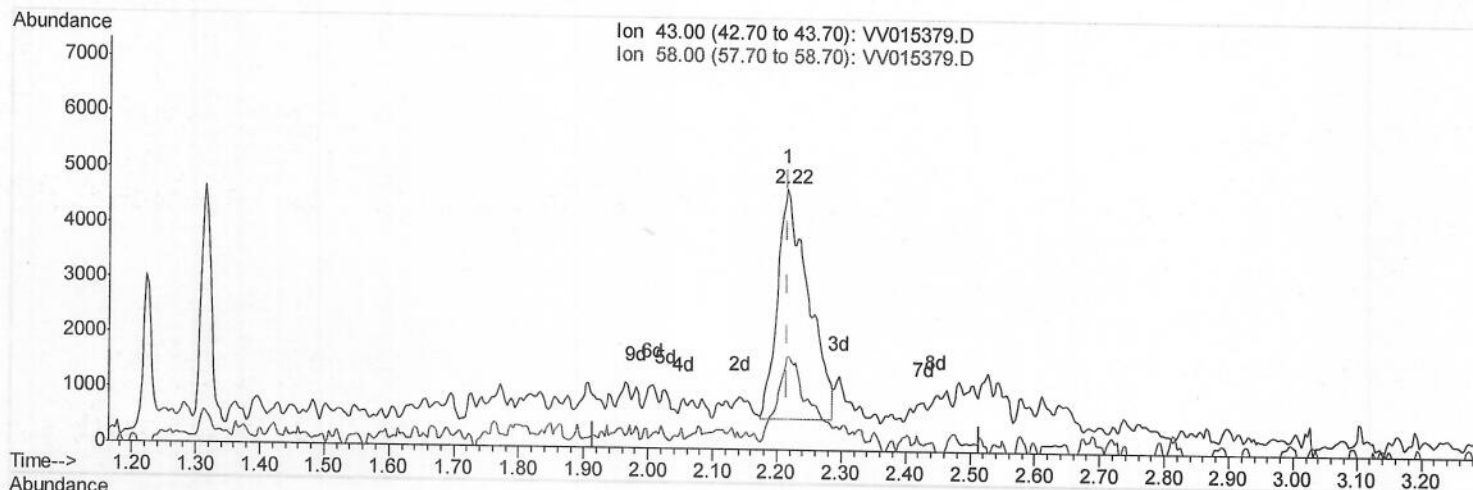

(13) Acetone (T)

2.216min (-0.000) 5.90ug/L m >

response 13841

Ion	Exp%	Act%
43.00	100	100
58.00	34.10	19.20
0.00	0.00	0.00
0.00	0.00	0.00

MD
04/3/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015379.D
 Acq On : 02 Apr 2020 17:14
 Operator : SY/MD
 Sample : L2003-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL6

Manual Integrations
 APPROVED

sam
 4/3/2020 5:50:04 PM

Quant Time: Apr 03 03:50:41 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 03 01:25:45 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	749383	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	713351	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	321543	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.31	65	211085	31.41	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	62.82%		
7) Chloroethane-d5	1.58	69	189712	33.05	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	66.10%#		
11) 1,1-Dichloroethene-d2	2.12	63	317442m	26.43	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	52.86%#		
21) 2-Butanone-d5	3.94	46	294521	82.47	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	82.47%		
24) Chloroform-d	4.38	84	398453	35.92	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	71.84%		
26) 1,2-Dichloroethane-d4	5.06	65	261186	37.80	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	75.60%		
32) Benzene-d6	5.07	84	828237	37.70	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	75.40%		
36) 1,2-Dichloropropane-d6	6.09	67	249713	38.55	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	77.10%		
41) Toluene-d8	7.34	98	805172	38.33	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	76.66%#		
43) trans-1,3-Dichloropropene-	7.64	79	124496	34.79	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.58%		
47) 2-Hexanone-d5	8.12	63	231381	78.22	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	78.22%		
57) 1,1,2,2-Tetrachloroethane-	10.24	84	362813	39.37	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	78.74%		
64) 1,2-Dichlorobenzene-d4	11.65	152	294608	40.28	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	80.56%		

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.22	43	13841m7	5.904	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

MD
 04/3/2020

MD
 04/3/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015379.D
 Acq On : 02 Apr 2020 17:14
 Operator : SY/MD
 Sample : L2003-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL6

Manual Integrations
 APPROVED

sam
 4/3/2020 5:50:04 PM

Quant Time: Apr 03 03:50:41 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 03 01:25:45 2020
 Response via : Initial Calibration

