

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015369.D
 Acq On : 02 Apr 2020 13:11
 Operator : SY/MD
 Sample : L2005-01 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	83	rVB	378500	384282	4.06%	0.988%
2	1.579	145	152	165	rVB	321574	387191	4.09%	0.995%
3	2.119	312	320	347	rVB	712462	1083525	11.44%	2.785%
4	3.090	620	622	623	rBV2	1434	554	0.01%	0.001%
5	3.103	624	626	630	rVV5	2109	1488	0.02%	0.004%
6	3.168	643	646	648	rBV2	766	527	0.01%	0.001%
7	3.193	648	654	658	rVV8	2619	3037	0.03%	0.008%
8	3.409	720	721	725	rVB4	1602	793	0.01%	0.002%
9	3.444	727	732	733	rBV5	1935	1766	0.02%	0.005%
10	3.544	761	763	766	rBV4	1731	1420	0.01%	0.004%
11	3.579	770	774	776	rBV5	935	617	0.01%	0.002%
12	3.602	776	781	787	rBV9	2332	2754	0.03%	0.007%
13	3.692	805	809	811	rBV4	2278	1773	0.02%	0.005%
14	3.856	857	860	862	rBV4	1579	793	0.01%	0.002%
15	3.936	874	885	930	rBV	128403	577964	6.10%	1.486%
16	4.377	1002	1022	1049	rBV	419858	1058994	11.18%	2.722%
17	4.647	1102	1106	1108	rBV4	1874	1196	0.01%	0.003%
18	4.965	1202	1205	1206	rBV3	886	495	0.01%	0.001%
19	5.071	1221	1238	1248	rBV2	1051052	2610308	27.56%	6.710%
20	5.640	1403	1415	1438	rBV	824489	1622043	17.13%	4.169%
21	5.814	1467	1469	1474	rVB5	2529	1315	0.01%	0.003%
22	6.093	1542	1556	1582	rBV	576789	1169214	12.35%	3.005%
23	6.576	1705	1706	1708	rBV2	938	368	0.00%	0.001%
24	6.647	1725	1728	1730	rBV4	1929	947	0.01%	0.002%
25	6.801	1772	1776	1779	rBV6	947	872	0.01%	0.002%
26	6.823	1779	1783	1788	rBV7	1873	1758	0.02%	0.005%
27	6.910	1805	1810	1814	rBV7	2109	2132	0.02%	0.005%
28	7.007	1829	1840	1858	rBV	354972	632099	6.67%	1.625%
29	7.232	1904	1910	1913	rBV8	1809	1743	0.02%	0.004%
30	7.338	1930	1943	1975	rBV	1301741	2302886	24.32%	5.920%
31	7.643	2028	2038	2057	rBV	252822	427961	4.52%	1.100%
32	7.862	2104	2106	2107	rVB	1001	365	0.00%	0.001%
33	7.888	2107	2114	2117	rBV9	2353	2528	0.03%	0.006%
34	7.907	2117	2120	2127	rVB8	1993	1839	0.02%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015369.D
 Acq On : 02 Apr 2020 13:11
 Operator : SY/MD
 Sample : L2005-01 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

35	7.942	2127	2131	2134	rBV6	2873	2406	0.03%	0.006%
36	8.116	2174	2185	2227	rBV2	661814	1374554	14.51%	3.533%
37	8.515	2308	2309	2310	rBV	1287	457	0.00%	0.001%
38	8.540	2315	2317	2319	rBV2	1018	702	0.01%	0.002%
39	8.569	2322	2326	2327	rBV4	2441	1767	0.02%	0.005%
40	8.611	2337	2339	2342	rVB3	2008	1001	0.01%	0.003%
41	8.627	2342	2344	2348	rVB5	1093	793	0.01%	0.002%
42	8.717	2369	2372	2373	rBV3	959	498	0.01%	0.001%
43	8.749	2377	2382	2385	rBV6	2313	1735	0.02%	0.004%
44	8.769	2385	2388	2389	rBV3	1104	677	0.01%	0.002%
45	8.810	2399	2401	2404	rBV4	1189	535	0.01%	0.001%
46	8.904	2404	2430	2462	rBV2	4623308	9470060	100.00%	24.343%
47	9.264	2540	2542	2543	rBV2	787	244	0.00%	0.001%
48	9.273	2543	2545	2547	rBV3	1322	684	0.01%	0.002%
49	9.450	2598	2600	2605	rVB6	1996	1063	0.01%	0.003%
50	9.511	2615	2619	2620	rBV4	1497	1283	0.01%	0.003%
51	9.566	2631	2636	2640	rBV6	2864	3336	0.04%	0.009%
52	9.656	2662	2664	2665	rBV2	1321	519	0.01%	0.001%
53	9.746	2691	2692	2694	rBV2	1395	546	0.01%	0.001%
54	9.846	2720	2723	2726	rBV5	1119	565	0.01%	0.001%
55	9.862	2726	2728	2729	rBV2	1135	490	0.01%	0.001%
56	9.907	2736	2742	2744	rBV5	2121	1946	0.02%	0.005%
57	10.074	2792	2794	2797	rBV3	1231	658	0.01%	0.002%
58	10.125	2809	2810	2815	rBV5	834	475	0.01%	0.001%
59	10.187	2824	2829	2831	rBV6	1619	1274	0.01%	0.003%
60	10.238	2831	2845	2861	rBV	839682	1321656	13.96%	3.397%
61	10.537	2936	2938	2941	rBV4	926	700	0.01%	0.002%
62	10.614	2959	2962	2966	rVB4	1869	1460	0.02%	0.004%
63	10.640	2968	2970	2971	rBV2	961	344	0.00%	0.001%
64	10.749	3002	3004	3006	rBV3	1583	806	0.01%	0.002%
65	10.762	3006	3008	3011	rVB3	1295	673	0.01%	0.002%
66	10.788	3015	3016	3018	rBV2	1304	500	0.01%	0.001%
67	10.875	3039	3043	3044	rBV4	2423	1598	0.02%	0.004%
68	11.071	3102	3104	3108	rVB4	1240	781	0.01%	0.002%
69	11.090	3108	3110	3113	rBV4	1911	1201	0.01%	0.003%
70	11.138	3121	3125	3127	rBV5	1000	573	0.01%	0.001%
71	11.203	3132	3145	3156	rVV	298386	473470	5.00%	1.217%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015369.D
 Acq On : 02 Apr 2020 13:11
 Operator : SY/MD
 Sample : L2005-01 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

72	11.293	3156	3173	3199	rVB2	2271299	5397141	56.99%	13.873%
73	11.582	3258	3263	3267	rBV6	2589	2799	0.03%	0.007%
74	11.662	3271	3288	3309	rVV2	2906870	6222242	65.70%	15.994%
75	11.900	3359	3362	3365	rBV5	1810	1218	0.01%	0.003%
76	12.019	3397	3399	3400	rBV2	1492	573	0.01%	0.001%
77	12.048	3406	3408	3410	rBV3	1211	668	0.01%	0.002%
78	12.161	3440	3443	3447	rBV5	1285	953	0.01%	0.002%
79	12.180	3447	3449	3453	rBV5	1181	882	0.01%	0.002%
80	12.235	3464	3466	3468	rBV3	1407	578	0.01%	0.001%
81	12.264	3474	3475	3478	rBV3	1335	848	0.01%	0.002%
82	12.328	3491	3495	3497	rBV4	2037	1469	0.02%	0.004%
83	12.421	3517	3524	3534	rVB5	13400	21342	0.23%	0.055%
84	12.611	3568	3583	3587	rBV5	6782	15198	0.16%	0.039%
85	12.711	3612	3614	3616	rBV3	1362	817	0.01%	0.002%
86	12.778	3627	3635	3644	rVB3	8756	16387	0.17%	0.042%
87	12.817	3644	3647	3648	rBV3	1092	579	0.01%	0.001%
88	12.971	3693	3695	3697	rBV3	1249	601	0.01%	0.002%
89	13.013	3704	3708	3712	rBV7	1906	2127	0.02%	0.005%
90	13.158	3751	3753	3757	rBV4	1328	877	0.01%	0.002%
91	13.225	3772	3774	3777	rVB4	1673	803	0.01%	0.002%
92	13.286	3779	3793	3815	rBV	1132644	1753020	18.51%	4.506%
93	13.582	3881	3885	3890	rBV7	2416	2659	0.03%	0.007%
94	13.768	3932	3943	3956	rBV	319761	494875	5.23%	1.272%
95	14.080	4037	4040	4044	rBV5	1845	1272	0.01%	0.003%
96	14.392	4135	4137	4138	rBV2	1625	607	0.01%	0.002%
97	14.428	4145	4148	4149	rBV3	1000	532	0.01%	0.001%
98	15.289	4414	4416	4419	rBV4	2984	2020	0.02%	0.005%


Sum of corrected areas: 38902664

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV040220\
Data File : VV015369.D
Acq On : 02 Apr 2020 13:11
Operator : SY/MD
Sample : L2005-01 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

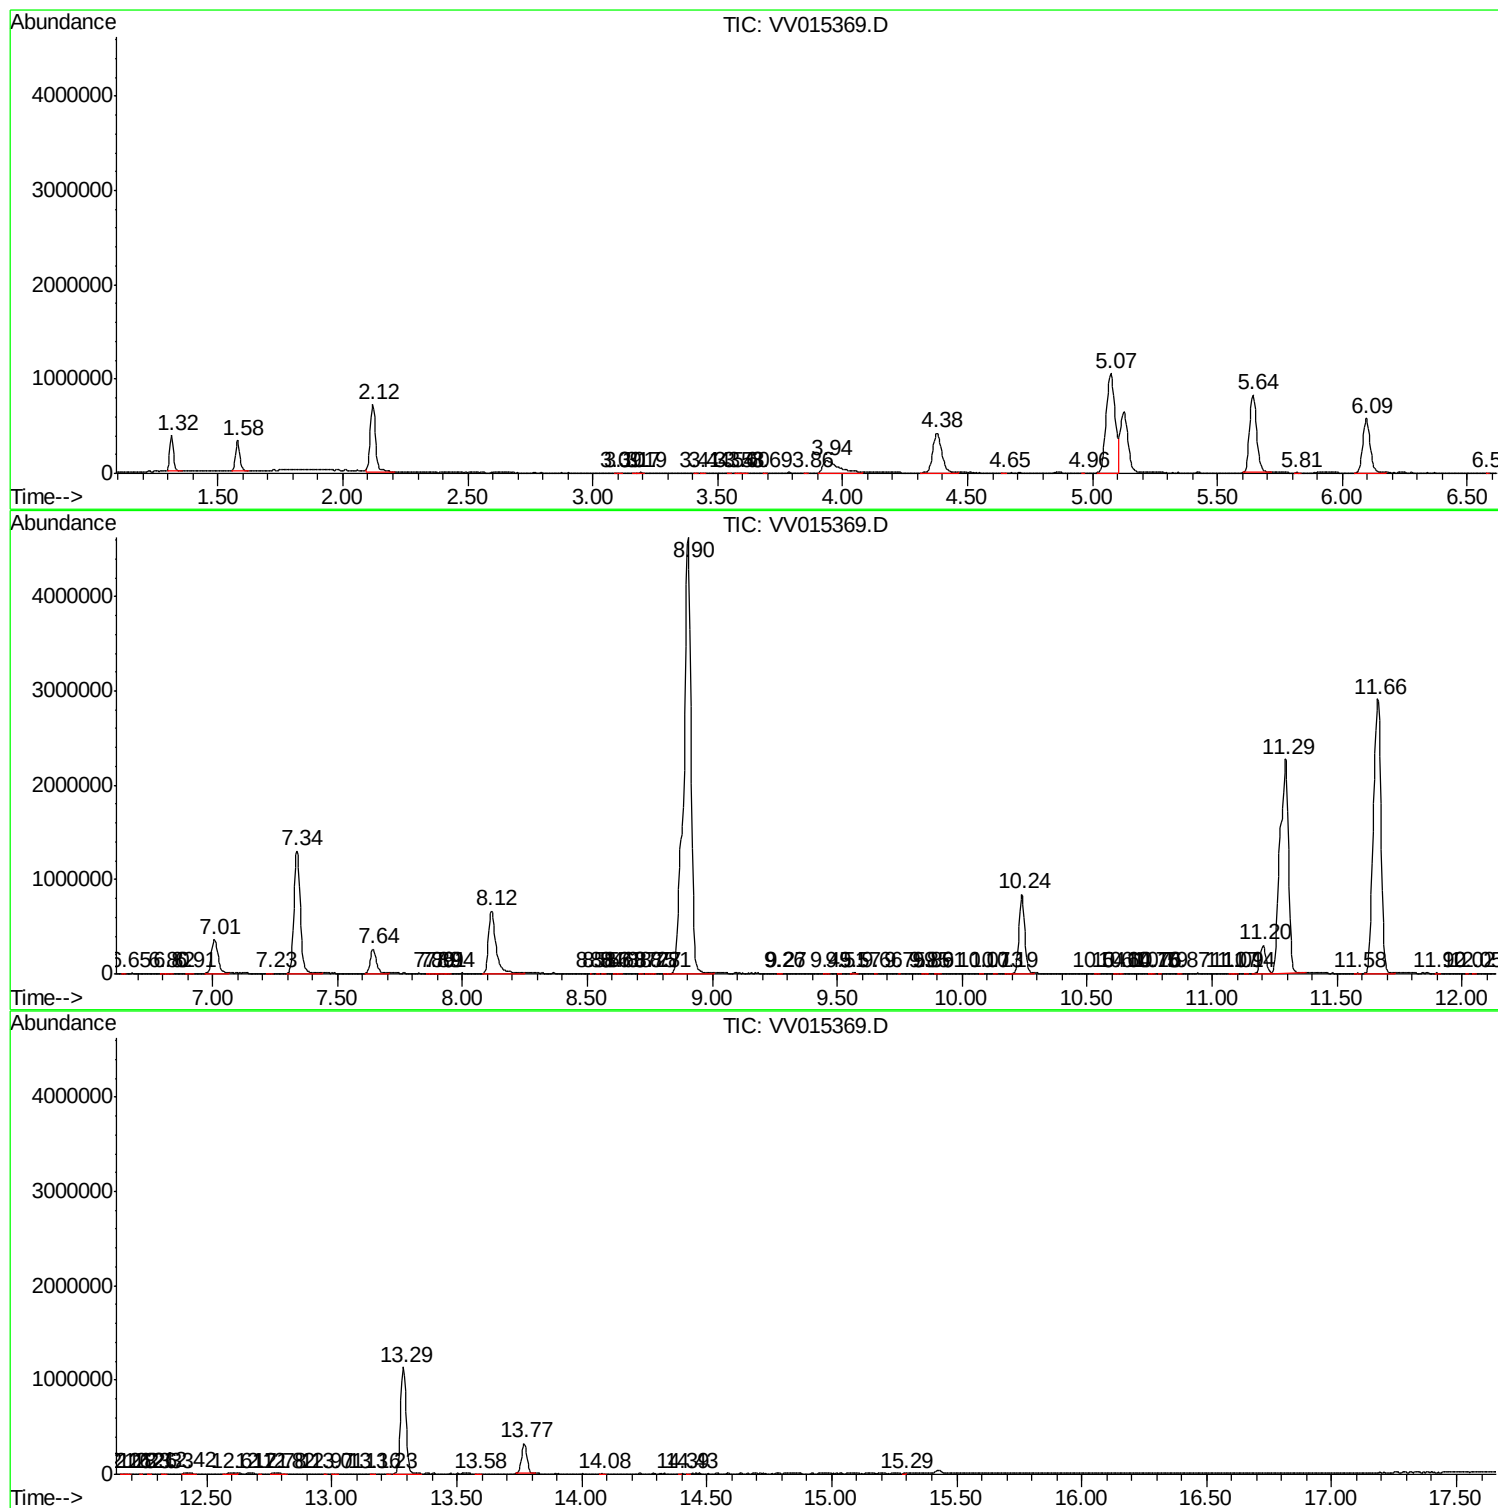

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV040220\
Data File : VV015369.D
Acq On : 02 Apr 2020 13:11
Operator : SY/MD
Sample : L2005-01 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV040220\
Data File : VV015369.D
Acq On : 02 Apr 2020 13:11
Operator : SY/MD
Sample : L2005-01 50X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DD7

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc