

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015370.D
 Acq On : 02 Apr 2020 13:35
 Operator : SY/MD
 Sample : L2005-02 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	369456	370659	4.40%	1.192%
2	1.579	145	152	166	rVB	305882	367710	4.36%	1.182%
3	2.119	312	320	333	rVB	677091	963313	11.43%	3.098%
4	3.100	623	625	628	rBV4	1727	1012	0.01%	0.003%
5	3.209	653	659	662	rBV7	2458	2528	0.03%	0.008%
6	3.283	680	682	684	rBV3	1597	669	0.01%	0.002%
7	3.319	690	693	695	rBV5	1497	1069	0.01%	0.003%
8	3.360	704	706	710	rVB3	1723	667	0.01%	0.002%
9	3.396	714	717	722	rBV6	2230	1927	0.02%	0.006%
10	3.483	742	744	746	rBV4	1126	545	0.01%	0.002%
11	3.576	771	773	776	rBV3	1933	1343	0.02%	0.004%
12	3.608	781	783	786	rVV3	1654	954	0.01%	0.003%
13	3.672	800	803	805	rBV4	1117	811	0.01%	0.003%
14	3.775	828	835	838	rBV8	2718	2857	0.03%	0.009%
15	3.794	838	841	843	rBV4	1896	1192	0.01%	0.004%
16	3.830	850	852	856	rBV4	1235	799	0.01%	0.003%
17	3.878	865	867	869	rVB3	1170	598	0.01%	0.002%
18	3.939	872	886	922	rBV2	130438	549289	6.52%	1.766%
19	4.376	1008	1022	1053	rVB	408495	1010262	11.99%	3.249%
20	4.801	1152	1154	1157	rVB3	1673	708	0.01%	0.002%
21	4.830	1157	1163	1165	rBV7	1751	1604	0.02%	0.005%
22	4.910	1184	1188	1192	rBV4	2462	2392	0.03%	0.008%
23	4.997	1213	1215	1219	rBV5	1377	1024	0.01%	0.003%
24	5.074	1222	1239	1275	rVV2	1014701	2615819	31.05%	8.412%
25	5.331	1315	1319	1321	rBV4	1777	1588	0.02%	0.005%
26	5.553	1386	1388	1390	rBV2	1320	795	0.01%	0.003%
27	5.640	1402	1415	1445	rBV	786847	1584543	18.81%	5.096%
28	6.097	1543	1557	1585	rBV	552316	1127459	13.38%	3.626%
29	6.437	1659	1663	1664	rBV4	962	588	0.01%	0.002%
30	6.524	1682	1690	1693	rBV8	2226	2726	0.03%	0.009%
31	6.630	1721	1723	1728	rBV5	1437	1173	0.01%	0.004%
32	6.833	1784	1786	1791	rVB5	1338	906	0.01%	0.003%
33	6.862	1791	1795	1797	rBV4	1587	973	0.01%	0.003%
34	6.888	1800	1803	1804	rBV3	1397	711	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015370.D
 Acq On : 02 Apr 2020 13:35
 Operator : SY/MD
 Sample : L2005-02 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DE2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

35	6.939	1818	1819	1824	rVB5	1448	1069	0.01%	0.003%
36	7.006	1824	1840	1863	rBV	348671	634769	7.53%	2.041%
37	7.338	1931	1943	1975	rBV	1286576	2225074	26.41%	7.155%
38	7.643	2028	2038	2054	rBV	243505	410271	4.87%	1.319%
39	7.881	2109	2112	2114	rBV3	2440	1236	0.01%	0.004%
40	7.942	2126	2131	2134	rBV6	1505	1537	0.02%	0.005%
41	8.116	2174	2185	2219	rBV2	657076	1353980	16.07%	4.354%
42	8.611	2337	2339	2344	rVB5	2263	1582	0.02%	0.005%
43	8.637	2344	2347	2348	rBV3	1389	870	0.01%	0.003%
44	8.875	2409	2421	2424	rBV	1305816	1855528	22.02%	5.967%
45	9.215	2523	2527	2529	rBV5	1869	1614	0.02%	0.005%
46	9.264	2539	2542	2544	rBV4	1609	1001	0.01%	0.003%
47	9.389	2578	2581	2582	rBV4	1291	688	0.01%	0.002%
48	9.527	2622	2624	2626	rBV3	1350	749	0.01%	0.002%
49	9.640	2654	2659	2660	rBV4	1854	1686	0.02%	0.005%
50	9.688	2672	2674	2677	rVB4	1363	671	0.01%	0.002%
51	9.801	2706	2709	2711	rVB4	2337	1056	0.01%	0.003%
52	9.868	2728	2730	2732	rBV3	1904	829	0.01%	0.003%
53	9.920	2740	2746	2747	rBV5	1815	1572	0.02%	0.005%
54	9.929	2747	2749	2751	rBV3	1300	700	0.01%	0.002%
55	9.987	2765	2767	2770	rVB4	1162	521	0.01%	0.002%
56	10.048	2783	2786	2788	rBV3	2048	1267	0.02%	0.004%
57	10.090	2793	2799	2802	rBV6	1924	1987	0.02%	0.006%
58	10.106	2802	2804	2808	rVB4	1456	901	0.01%	0.003%
59	10.125	2808	2810	2811	rBV2	1131	512	0.01%	0.002%
60	10.238	2833	2845	2864	rBV	831131	1296987	15.39%	4.171%
61	10.363	2881	2884	2887	rVB5	1472	928	0.01%	0.003%
62	10.399	2892	2895	2897	rBV4	1527	853	0.01%	0.003%
63	10.511	2926	2930	2934	rBV7	1184	921	0.01%	0.003%
64	10.534	2934	2937	2940	rBV4	1719	1294	0.02%	0.004%
65	10.656	2972	2975	2978	rBV4	1530	1018	0.01%	0.003%
66	10.736	2992	3000	3001	rBV7	1976	1949	0.02%	0.006%
67	10.842	3031	3033	3035	rVB3	1173	528	0.01%	0.002%
68	10.942	3062	3064	3068	rVB5	1611	746	0.01%	0.002%
69	11.116	3116	3118	3123	rVB4	2135	1361	0.02%	0.004%
70	11.154	3126	3130	3132	rBV4	1706	1088	0.01%	0.003%
71	11.206	3134	3146	3156	rBV2	168491	271788	3.23%	0.874%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015370.D
 Acq On : 02 Apr 2020 13:35
 Operator : SY/MD
 Sample : L2005-02 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

72	11.273	3156	3167	3189	rVB2	1347176	3158108	37.48%	10.156%
73	11.514	3239	3242	3246	rBV4	2220	1543	0.02%	0.005%
74	11.534	3246	3248	3251	rBV4	1630	1019	0.01%	0.003%
75	11.604	3268	3270	3271	rBV2	1501	607	0.01%	0.002%
76	11.665	3271	3289	3311	rVV2	4384681	8425617	100.00%	27.095%
77	11.977	3384	3386	3390	rBV4	1229	753	0.01%	0.002%
78	12.061	3409	3412	3415	rVB5	1942	1073	0.01%	0.003%
79	12.077	3415	3417	3422	rBV5	1364	937	0.01%	0.003%
80	12.527	3553	3557	3560	rBV5	1938	1553	0.02%	0.005%
81	12.556	3563	3566	3570	rVB5	1662	1054	0.01%	0.003%
82	12.598	3573	3579	3582	rBV7	5680	6644	0.08%	0.021%
83	12.672	3598	3602	3609	rVB9	4734	5848	0.07%	0.019%
84	12.778	3623	3635	3642	rBV9	6534	12891	0.15%	0.041%
85	12.833	3650	3652	3658	rVB6	1923	1776	0.02%	0.006%
86	12.862	3658	3661	3663	rBV3	1354	744	0.01%	0.002%
87	12.981	3696	3698	3701	rVB4	2727	1440	0.02%	0.005%
88	13.000	3701	3704	3706	rBV3	2983	1675	0.02%	0.005%
89	13.061	3721	3723	3725	rBV3	1632	788	0.01%	0.003%
90	13.125	3741	3743	3745	rVV3	1050	559	0.01%	0.002%
91	13.286	3781	3793	3815	rBV	1422634	2195986	26.06%	7.062%
92	13.492	3854	3857	3858	rBV3	1859	1037	0.01%	0.003%
93	13.524	3862	3867	3868	rBV4	3703	3391	0.04%	0.011%
94	13.681	3914	3916	3918	rBV3	2105	1043	0.01%	0.003%
95	13.698	3918	3921	3923	rBV4	1258	854	0.01%	0.003%
96	13.768	3930	3943	3959	rBV	296731	475809	5.65%	1.530%
97	14.109	4045	4049	4052	rBV5	1730	1404	0.02%	0.005%
98	14.218	4081	4083	4087	rBV4	1704	1108	0.01%	0.004%
99	14.498	4167	4170	4172	rBV3	1881	1089	0.01%	0.004%
100	15.424	4450	4458	4471	rVB4	53738	87743	1.04%	0.282%


Sum of corrected areas: 31096437

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV040220\
Data File : VV015370.D
Acq On : 02 Apr 2020 13:35
Operator : SY/MD
Sample : L2005-02 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CODE2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

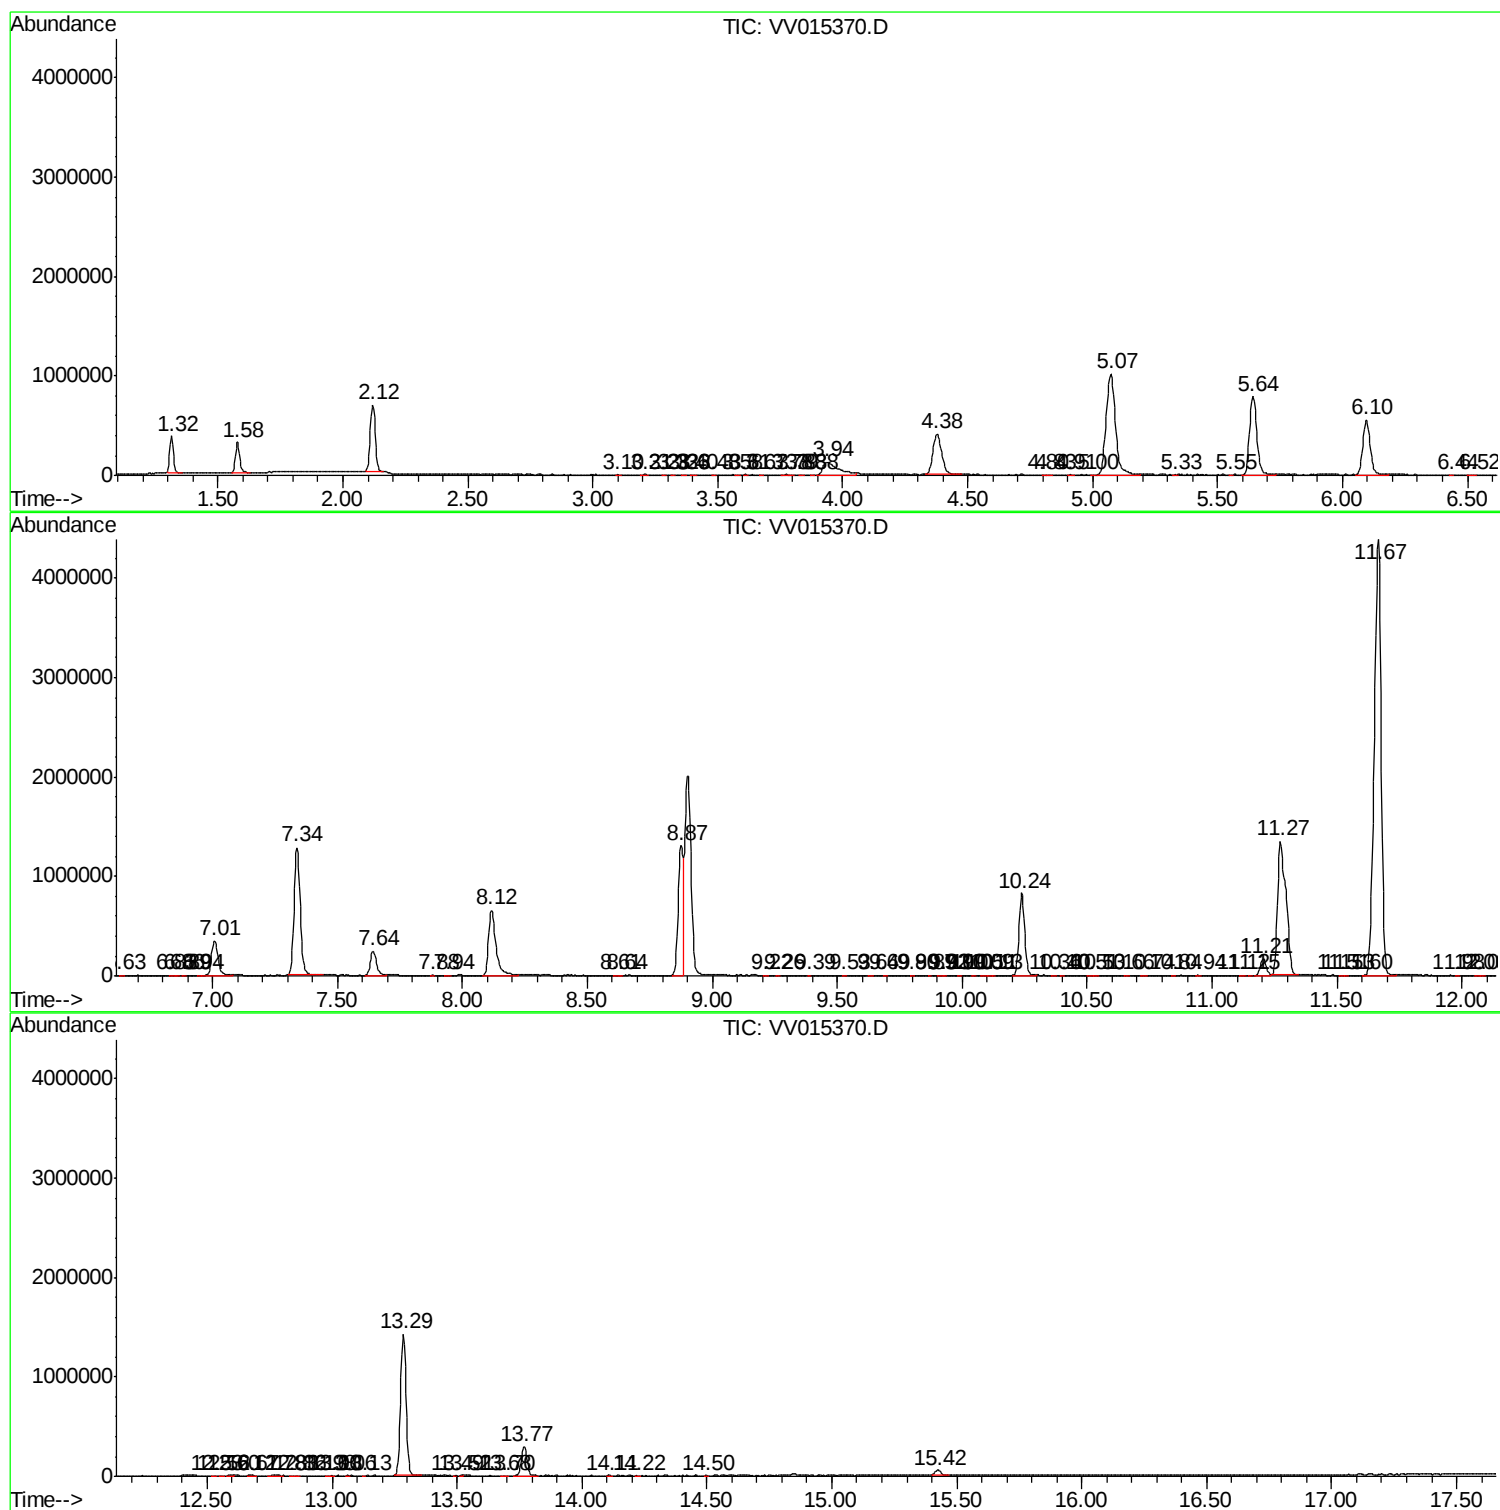

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV040220\
Data File : VV015370.D
Acq On : 02 Apr 2020 13:35
Operator : SY/MD
Sample : L2005-02 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DE2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV040220\
Data File : VV015370.D
Acq On : 02 Apr 2020 13:35
Operator : SY/MD
Sample : L2005-02 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DE2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc