

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015378.D
 Acq On : 02 Apr 2020 16:49
 Operator : SY/MD
 Sample : VIBLK65
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	84	rVB	337326	354225	14.20%	1.746%
2	1.579	146	152	166	rVB	303336	357298	14.32%	1.761%
3	2.119	312	320	343	rVB	666401	1019078	40.85%	5.024%
4	2.997	591	593	596	rBV3	1838	1140	0.05%	0.006%
5	3.081	617	619	621	rBV3	1459	740	0.03%	0.004%
6	3.196	653	655	658	rVB4	1672	882	0.04%	0.004%
7	3.318	691	693	695	rBV3	1430	687	0.03%	0.003%
8	3.421	721	725	727	rBV5	1844	1225	0.05%	0.006%
9	3.560	766	768	770	rBV3	1086	685	0.03%	0.003%
10	3.630	785	790	792	rBV5	2016	2101	0.08%	0.010%
11	3.862	857	862	865	rBV6	1868	1385	0.06%	0.007%
12	3.881	865	868	871	rBV5	1680	844	0.03%	0.004%
13	3.897	871	873	874	rBV2	2253	1052	0.04%	0.005%
14	3.939	874	886	925	rBV	116496	529225	21.21%	2.609%
15	4.376	1009	1022	1046	rVB	400719	983641	39.43%	4.849%
16	4.553	1075	1077	1082	rBV5	2503	1854	0.07%	0.009%
17	4.724	1127	1130	1132	rBV4	2465	1536	0.06%	0.008%
18	4.769	1141	1144	1145	rBV3	1389	643	0.03%	0.003%
19	4.836	1160	1165	1166	rBV5	2515	1635	0.07%	0.008%
20	4.926	1191	1193	1194	rBV2	1091	580	0.02%	0.003%
21	4.958	1200	1203	1206	rBV4	1794	1160	0.05%	0.006%
22	4.974	1206	1208	1210	rBV3	1534	819	0.03%	0.004%
23	5.074	1222	1239	1277	rBV2	995647	2494643	100.00%	12.298%
24	5.640	1402	1415	1444	rBV	798049	1604260	64.31%	7.909%
25	5.820	1468	1471	1473	rBV4	2773	1826	0.07%	0.009%
26	6.093	1544	1556	1587	rVB	549285	1118262	44.83%	5.513%
27	6.376	1642	1644	1648	rBV5	1335	1113	0.04%	0.005%
28	6.434	1657	1662	1664	rBV5	1482	1317	0.05%	0.006%
29	6.473	1671	1674	1675	rBV3	1161	603	0.02%	0.003%
30	6.527	1687	1691	1693	rBV4	1391	1176	0.05%	0.006%
31	6.576	1703	1706	1711	rBV7	1933	1605	0.06%	0.008%
32	6.617	1718	1719	1721	rBV3	1276	573	0.02%	0.003%
33	6.807	1776	1778	1781	rVB3	1652	643	0.03%	0.003%
34	6.826	1782	1784	1788	rVB5	1805	1026	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015378.D
 Acq On : 02 Apr 2020 16:49
 Operator : SY/MD
 Sample : VIBLK65
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

35	6.859	1792	1794	1796	rBV3	1010	544	0.02%	0.003%
36	7.006	1829	1840	1860	rBV	342650	618099	24.78%	3.047%
37	7.338	1931	1943	1965	rBV	1240841	2159611	86.57%	10.647%
38	7.643	2028	2038	2058	rBV	238035	401556	16.10%	1.980%
39	7.929	2124	2127	2129	rBV3	1463	875	0.04%	0.004%
40	8.006	2144	2151	2153	rBV7	2743	2590	0.10%	0.013%
41	8.116	2175	2185	2221	rBV2	629671	1328304	53.25%	6.548%
42	8.331	2250	2252	2262	rVB10	2546	2115	0.08%	0.010%
43	8.418	2276	2279	2281	rBV4	1928	1224	0.05%	0.006%
44	8.604	2335	2337	2342	rBV5	2142	1827	0.07%	0.009%
45	8.633	2342	2346	2349	rBV6	1382	1572	0.06%	0.008%
46	8.675	2356	2359	2363	rVB5	2107	1334	0.05%	0.007%
47	8.698	2363	2366	2371	rBV7	1701	1624	0.07%	0.008%
48	8.875	2409	2421	2443	rBV	1215818	1989131	79.74%	9.806%
49	9.148	2503	2506	2507	rBV2	2040	941	0.04%	0.005%
50	9.296	2550	2552	2556	rVB3	1275	839	0.03%	0.004%
51	9.434	2592	2595	2597	rBV3	1390	987	0.04%	0.005%
52	9.495	2610	2614	2617	rBV4	1459	1061	0.04%	0.005%
53	9.620	2649	2653	2658	rBV7	1885	1778	0.07%	0.009%
54	9.762	2696	2697	2705	rVB7	2214	1654	0.07%	0.008%
55	9.926	2745	2748	2749	rBV3	1480	793	0.03%	0.004%
56	10.010	2767	2774	2776	rBV5	1744	1877	0.08%	0.009%
57	10.045	2783	2785	2789	rVB5	1776	1172	0.05%	0.006%
58	10.064	2789	2791	2793	rBV3	1234	625	0.03%	0.003%
59	10.125	2808	2810	2813	rVB3	1553	659	0.03%	0.003%
60	10.154	2816	2819	2820	rBV3	1385	747	0.03%	0.004%
61	10.193	2827	2831	2832	rBV3	1072	732	0.03%	0.004%
62	10.238	2834	2845	2865	rVB	829447	1287518	51.61%	6.347%
63	10.389	2890	2892	2894	rBV2	999	567	0.02%	0.003%
64	10.530	2934	2936	2940	rVB5	1836	1157	0.05%	0.006%
65	10.563	2940	2946	2947	rBV4	1683	1726	0.07%	0.009%
66	10.598	2954	2957	2962	rBV7	1541	1124	0.05%	0.006%
67	10.675	2978	2981	2982	rBV3	1547	905	0.04%	0.004%
68	10.704	2986	2990	2992	rBV4	1382	1041	0.04%	0.005%
69	10.807	3018	3022	3026	rBV7	1980	1958	0.08%	0.010%
70	10.868	3037	3041	3046	rBV7	2101	2665	0.11%	0.013%
71	10.984	3071	3077	3078	rVV4	1922	1311	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015378.D
 Acq On : 02 Apr 2020 16:49
 Operator : SY/MD
 Sample : VIBLK65
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

72	11.032	3090	3092	3096	rVB4	1619	908	0.04%	0.004%
73	11.141	3122	3126	3127	rBV4	1298	716	0.03%	0.004%
74	11.270	3155	3166	3185	rBV	1254266	1945626	77.99%	9.592%
75	11.440	3215	3219	3220	rBV3	2617	1431	0.06%	0.007%
76	11.501	3236	3238	3239	rBV2	1415	538	0.02%	0.003%
77	11.563	3254	3257	3259	rBV4	1525	1020	0.04%	0.005%
78	11.646	3272	3283	3302	rBV	1283657	1982119	79.46%	9.772%
79	11.878	3349	3355	3359	rBV7	2958	3031	0.12%	0.015%
80	12.083	3416	3419	3422	rBV5	2451	1460	0.06%	0.007%
81	12.164	3441	3444	3445	rBV3	1044	639	0.03%	0.003%
82	12.292	3482	3484	3489	rVB4	1873	1006	0.04%	0.005%
83	12.370	3505	3508	3509	rBV2	1713	1117	0.04%	0.006%
84	12.460	3533	3536	3540	rBV6	1705	1474	0.06%	0.007%
85	12.530	3554	3558	3559	rBV3	1438	923	0.04%	0.005%
86	12.579	3571	3573	3576	rBV4	1206	920	0.04%	0.005%
87	12.643	3591	3593	3596	rBV4	1178	563	0.02%	0.003%
88	12.717	3614	3616	3618	rBV3	1137	693	0.03%	0.003%
89	12.768	3628	3632	3633	rBV3	1306	897	0.04%	0.004%
90	12.807	3641	3644	3648	rVB5	1954	1519	0.06%	0.007%
91	12.829	3648	3651	3657	rBV7	2154	1571	0.06%	0.008%
92	12.884	3666	3668	3670	rBV3	1569	1065	0.04%	0.005%
93	12.993	3699	3702	3703	rBV3	1463	853	0.03%	0.004%
94	13.209	3766	3769	3771	rBV4	1981	1315	0.05%	0.006%
95	13.292	3786	3795	3802	rBV10	8158	13064	0.52%	0.064%
96	13.379	3819	3822	3825	rBV4	1460	910	0.04%	0.004%
97	14.029	4021	4024	4025	rBV2	2164	1259	0.05%	0.006%
98	14.199	4074	4077	4078	rBV4	2165	1066	0.04%	0.005%
99	14.254	4091	4094	4096	rBV4	1891	1192	0.05%	0.006%
100	14.694	4227	4231	4232	rBV3	3018	1917	0.08%	0.009%


Sum of corrected areas: 20284537

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV040220\
Data File : VV015378.D
Acq On : 02 Apr 2020 16:49
Operator : SY/MD
Sample : VIBLK65
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK65

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

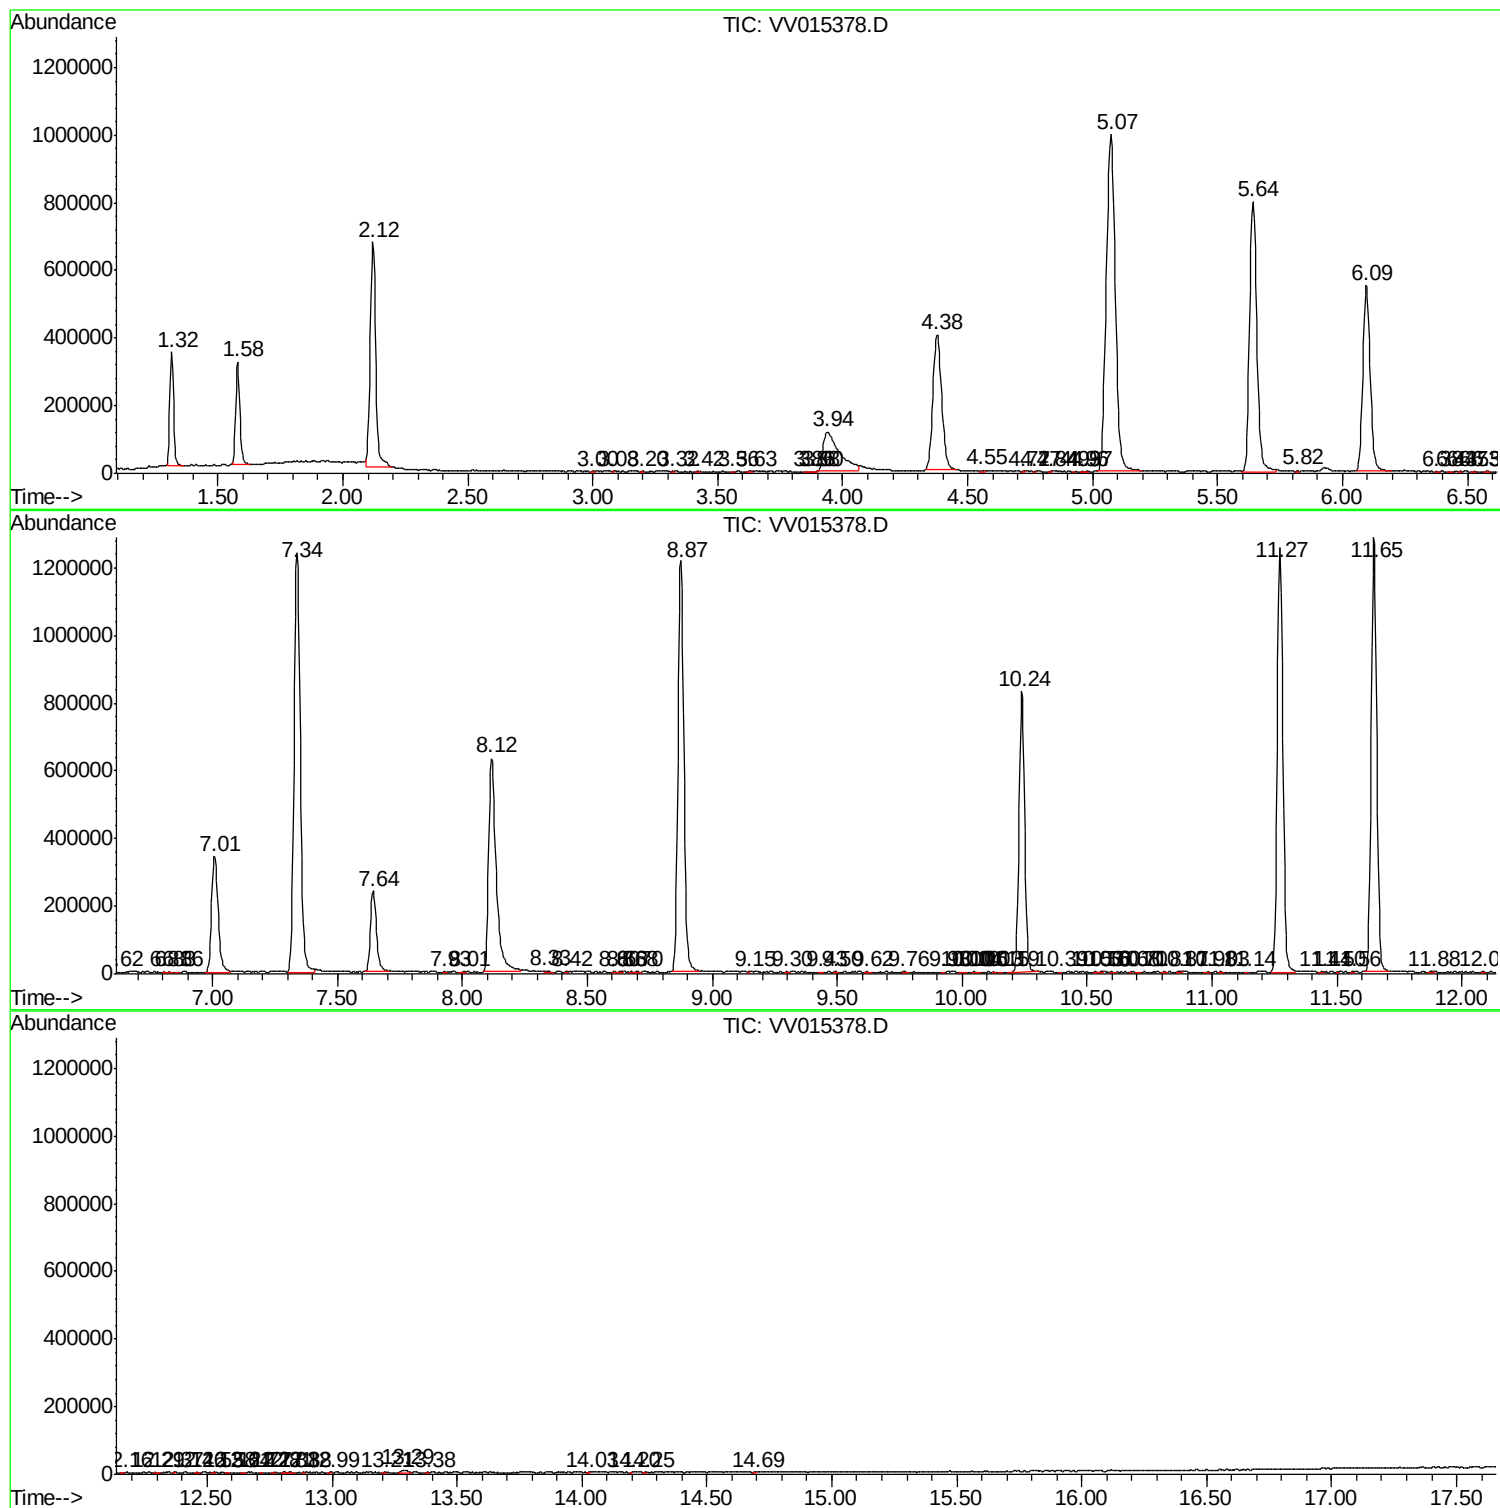

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV040220\
Data File : VV015378.D
Acq On : 02 Apr 2020 16:49
Operator : SY/MD
Sample : VIBLK65
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK65

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV040220\
Data File : VV015378.D
Acq On : 02 Apr 2020 16:49
Operator : SY/MD
Sample : VIBLK65
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK65

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc