

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015379.D
 Acq On : 02 Apr 2020 17:14
 Operator : SY/MD
 Sample : L2003-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	344817	349786	14.71%	1.760%
2	1.579	145	152	169	rVB	285053	342667	14.41%	1.725%
3	2.119	312	320	341	rVB	638537	947594	39.85%	4.769%
4	3.148	637	640	643	rBV3	1458	1164	0.05%	0.006%
5	3.251	670	672	675	rVB4	1782	815	0.03%	0.004%
6	3.270	675	678	679	rBV3	1550	884	0.04%	0.004%
7	3.315	690	692	694	rBV2	1495	577	0.02%	0.003%
8	3.637	791	792	796	rVB3	1611	591	0.02%	0.003%
9	3.656	796	798	800	rBV3	1363	831	0.03%	0.004%
10	3.698	808	811	812	rBV2	1108	751	0.03%	0.004%
11	3.736	821	823	826	rBV4	2294	1508	0.06%	0.008%
12	3.762	829	831	833	rVV3	1589	739	0.03%	0.004%
13	3.775	833	835	837	rVB3	1717	723	0.03%	0.004%
14	3.788	837	839	841	rBV3	1423	736	0.03%	0.004%
15	3.826	848	851	855	rBV4	1104	969	0.04%	0.005%
16	3.939	874	886	916	rBV2	115725	476255	20.03%	2.397%
17	4.376	1008	1022	1050	rVB2	380081	945610	39.77%	4.759%
18	4.807	1154	1156	1159	rBV3	1173	927	0.04%	0.005%
19	4.884	1176	1180	1186	rVB7	3156	3643	0.15%	0.018%
20	4.913	1186	1189	1194	rBV6	2050	2242	0.09%	0.011%
21	4.955	1200	1202	1205	rBV4	2107	1211	0.05%	0.006%
22	5.010	1215	1219	1220	rBV3	1949	1213	0.05%	0.006%
23	5.071	1222	1238	1263	rVV3	947550	2377733	100.00%	11.966%
24	5.640	1402	1415	1444	rBV	838251	1689158	71.04%	8.501%
25	5.932	1494	1506	1515	rBV9	12109	24100	1.01%	0.121%
26	6.093	1544	1556	1582	rBV	522678	1055843	44.41%	5.314%
27	6.383	1644	1646	1650	rVB4	2057	935	0.04%	0.005%
28	6.408	1650	1654	1663	rBV4	2707	3517	0.15%	0.018%
29	6.495	1678	1681	1685	rBV3	1454	1188	0.05%	0.006%
30	6.846	1787	1790	1794	rVB5	1966	1553	0.07%	0.008%
31	6.887	1802	1803	1806	rBV3	1132	614	0.03%	0.003%
32	6.929	1814	1816	1817	rBV2	1426	586	0.02%	0.003%
33	7.006	1827	1840	1861	rVV	320701	578015	24.31%	2.909%
34	7.338	1929	1943	1964	rBV	1192410	2067965	86.97%	10.407%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015379.D
 Acq On : 02 Apr 2020 17:14
 Operator : SY/MD
 Sample : L2003-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

35	7.643	2028	2038	2059	rBV	225378	375351	15.79%	1.889%
36	7.833	2095	2097	2101	rVB4	2053	1145	0.05%	0.006%
37	7.862	2104	2106	2111	rVB6	2484	1444	0.06%	0.007%
38	8.116	2174	2185	2214	rBV3	616193	1281480	53.90%	6.449%
39	8.502	2303	2305	2308	rBV3	2163	1421	0.06%	0.007%
40	8.614	2337	2340	2342	rBV5	1091	618	0.03%	0.003%
41	8.701	2363	2367	2372	rBV8	1868	2001	0.08%	0.010%
42	8.823	2403	2405	2406	rBV2	1143	571	0.02%	0.003%
43	8.874	2409	2421	2449	rVV	1289850	2105988	88.57%	10.599%
44	9.244	2532	2536	2540	rVB7	2708	2492	0.10%	0.013%
45	9.270	2540	2544	2547	rBV5	2922	2447	0.10%	0.012%
46	9.389	2579	2581	2584	rVB4	1807	787	0.03%	0.004%
47	9.431	2591	2594	2597	rBV5	1498	964	0.04%	0.005%
48	9.508	2617	2618	2622	rBV4	2007	1024	0.04%	0.005%
49	9.534	2622	2626	2627	rBV4	1494	824	0.03%	0.004%
50	9.669	2666	2668	2670	rVB3	1618	579	0.02%	0.003%
51	9.804	2705	2710	2711	rBV3	1628	1298	0.05%	0.007%
52	9.839	2718	2721	2723	rBV4	2544	1496	0.06%	0.008%
53	9.903	2737	2741	2744	rVB3	2425	1655	0.07%	0.008%
54	9.964	2758	2760	2762	rVB2	1496	570	0.02%	0.003%
55	9.981	2762	2765	2768	rBV4	1364	827	0.03%	0.004%
56	10.026	2777	2779	2781	rBV3	1339	657	0.03%	0.003%
57	10.058	2781	2789	2795	rBV10	5223	8992	0.38%	0.045%
58	10.238	2832	2845	2863	rBV	786525	1226266	51.57%	6.171%
59	10.370	2883	2886	2887	rBV3	2048	1141	0.05%	0.006%
60	10.585	2950	2953	2955	rBV3	1322	754	0.03%	0.004%
61	10.755	3002	3006	3009	rBV5	2085	1948	0.08%	0.010%
62	10.800	3017	3020	3023	rBV5	856	756	0.03%	0.004%
63	10.833	3028	3030	3034	rVV4	1527	965	0.04%	0.005%
64	11.077	3103	3106	3107	rBV3	2063	1024	0.04%	0.005%
65	11.151	3121	3129	3130	rBV8	1641	1852	0.08%	0.009%
66	11.273	3155	3167	3186	rBV	1303576	2015979	84.79%	10.146%
67	11.514	3239	3242	3244	rBV4	1594	888	0.04%	0.004%
68	11.569	3251	3259	3265	rBV9	7023	11697	0.49%	0.059%
69	11.649	3271	3284	3305	rBV	1183400	1880638	79.09%	9.465%
70	12.032	3401	3403	3405	rVB3	1519	730	0.03%	0.004%
71	12.048	3405	3408	3411	rBV5	1699	1127	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015379.D
 Acq On : 02 Apr 2020 17:14
 Operator : SY/MD
 Sample : L2003-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EL6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

72	12.103	3423	3425	3427	rBV2	1806	1152	0.05%	0.006%
73	12.206	3455	3457	3458	rBV3	1824	780	0.03%	0.004%
74	12.337	3495	3498	3502	rVB5	2295	1757	0.07%	0.009%
75	12.376	3502	3510	3518	rBV5	6145	11137	0.47%	0.056%
76	12.466	3534	3538	3541	rBV3	2436	1973	0.08%	0.010%
77	12.598	3575	3579	3581	rBV4	1570	1289	0.05%	0.006%
78	12.707	3611	3613	3616	rVB4	1778	783	0.03%	0.004%
79	12.842	3652	3655	3656	rBV3	979	622	0.03%	0.003%
80	12.884	3665	3668	3676	rVB8	1585	1553	0.07%	0.008%
81	12.923	3676	3680	3681	rBV4	1654	1341	0.06%	0.007%
82	13.006	3700	3706	3708	rBV5	2256	2283	0.10%	0.011%
83	13.061	3719	3723	3726	rBV5	1553	1342	0.06%	0.007%
84	13.083	3728	3730	3733	rVV3	1204	821	0.03%	0.004%
85	13.244	3776	3780	3783	rBV4	1270	1272	0.05%	0.006%
86	13.337	3807	3809	3811	rBV3	1352	821	0.03%	0.004%
87	13.366	3816	3818	3821	rBV3	1601	823	0.03%	0.004%
88	13.463	3845	3848	3852	rBV3	1813	1671	0.07%	0.008%
89	13.533	3865	3870	3873	rBV7	2634	2332	0.10%	0.012%
90	13.595	3886	3889	3892	rVB6	1805	1074	0.05%	0.005%
91	13.617	3892	3896	3900	rBV7	2415	1990	0.08%	0.010%
92	13.636	3900	3902	3904	rBV3	1846	930	0.04%	0.005%
93	13.717	3922	3927	3929	rBV4	2170	1802	0.08%	0.009%
94	13.810	3953	3956	3958	rBV4	1537	889	0.04%	0.004%
95	13.829	3959	3962	3964	rVV4	2011	871	0.04%	0.004%
96	13.849	3964	3968	3972	rBV6	1805	1886	0.08%	0.009%
97	13.897	3980	3983	3986	rBV5	1733	1377	0.06%	0.007%
98	13.984	4007	4010	4011	rBV3	1230	742	0.03%	0.004%
99	14.099	4044	4046	4048	rBV3	1154	753	0.03%	0.004%
100	14.453	4154	4156	4158	rBV3	1575	952	0.04%	0.005%


Sum of corrected areas: 19870057

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV040220\
Data File : VV015379.D
Acq On : 02 Apr 2020 17:14
Operator : SY/MD
Sample : L2003-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

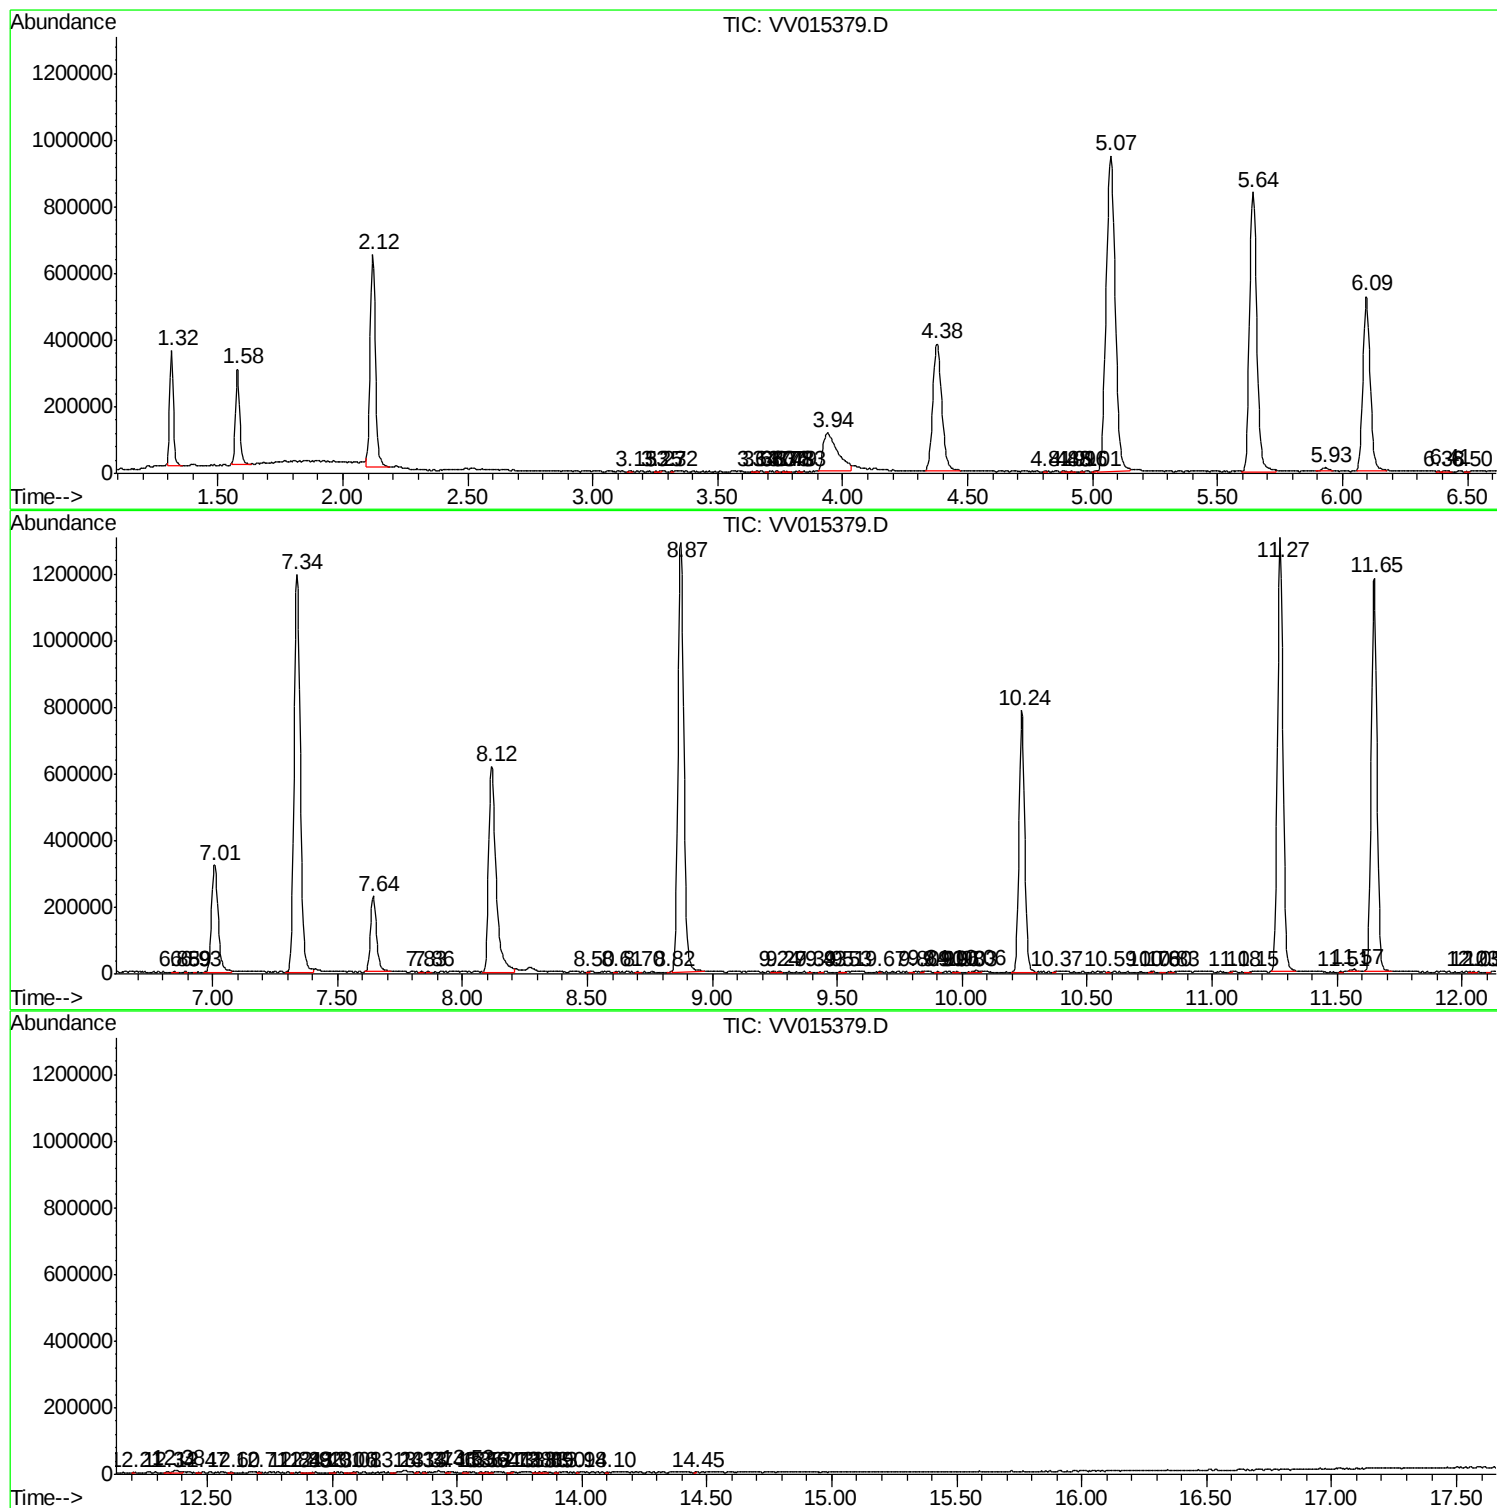

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV040220\
Data File : VV015379.D
Acq On : 02 Apr 2020 17:14
Operator : SY/MD
Sample : L2003-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EL6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV040220\
Data File : VV015379.D
Acq On : 02 Apr 2020 17:14
Operator : SY/MD
Sample : L2003-06
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0EL6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc