

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015388.D
 Acq On : 02 Apr 2020 22:04
 Operator : SY/MD
 Sample : VIBLK66
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK66

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	81	rVB	367370	361188	14.58%	1.775%
2	1.576	145	151	165	rVB	296536	349238	14.10%	1.716%
3	2.116	312	319	343	rVB	649349	968229	39.09%	4.759%
4	3.020	596	600	602	rBV6	2029	1786	0.07%	0.009%
5	3.216	659	661	663	rBV2	2130	1141	0.05%	0.006%
6	3.242	667	669	672	rBV4	1188	803	0.03%	0.004%
7	3.290	682	684	686	rBV3	1240	835	0.03%	0.004%
8	3.393	714	716	719	rVV4	1809	1163	0.05%	0.006%
9	3.454	732	735	737	rBV3	1258	721	0.03%	0.004%
10	3.496	744	748	751	rVB5	2024	1439	0.06%	0.007%
11	3.621	784	787	791	rBV5	1765	1509	0.06%	0.007%
12	3.682	804	806	809	rBV3	1636	893	0.04%	0.004%
13	3.750	824	827	830	rBV3	1788	1150	0.05%	0.006%
14	3.811	841	846	847	rBV5	1564	1193	0.05%	0.006%
15	3.833	850	853	855	rBV3	1972	1088	0.04%	0.005%
16	3.869	861	864	866	rBV3	1623	1027	0.04%	0.005%
17	3.936	872	885	917	rBV2	126617	546596	22.07%	2.686%
18	4.377	1008	1022	1049	rVB2	407032	1000612	40.40%	4.918%
19	4.566	1079	1081	1084	rBV4	2508	1542	0.06%	0.008%
20	4.785	1142	1149	1152	rBV9	2066	3029	0.12%	0.015%
21	4.836	1163	1165	1167	rBV3	1199	886	0.04%	0.004%
22	4.878	1174	1178	1184	rBV8	1898	2365	0.10%	0.012%
23	5.071	1220	1238	1266	rBV2	998784	2476951	100.00%	12.174%
24	5.557	1385	1389	1394	rBV6	1763	1721	0.07%	0.008%
25	5.640	1402	1415	1445	rBV	797668	1591458	64.25%	7.822%
26	5.875	1486	1488	1491	rBV3	1242	682	0.03%	0.003%
27	6.093	1540	1556	1586	rVV	549324	1135314	45.84%	5.580%
28	6.470	1670	1673	1677	rBV5	2554	2220	0.09%	0.011%
29	6.585	1707	1709	1712	rBV4	1028	624	0.03%	0.003%
30	6.708	1744	1747	1749	rBV3	1781	1235	0.05%	0.006%
31	6.756	1756	1762	1764	rBV7	2629	2398	0.10%	0.012%
32	6.804	1775	1777	1779	rBV3	1439	641	0.03%	0.003%
33	6.852	1789	1792	1795	rBV5	2431	1688	0.07%	0.008%
34	6.894	1802	1805	1809	rBV6	2231	2163	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015388.D
 Acq On : 02 Apr 2020 22:04
 Operator : SY/MD
 Sample : VIBLK66
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK66

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

35	7.007	1828	1840	1866	rBV	332118	601009	24.26%	2.954%
36	7.193	1896	1898	1900	rBV3	1901	858	0.03%	0.004%
37	7.338	1931	1943	1962	rBV	1237641	2120631	85.61%	10.423%
38	7.643	2025	2038	2057	rBV	228213	400619	16.17%	1.969%
39	8.000	2146	2149	2156	rVB9	2468	2940	0.12%	0.014%
40	8.026	2156	2157	2161	rBV4	1394	758	0.03%	0.004%
41	8.116	2174	2185	2224	rBV2	656544	1351640	54.57%	6.643%
42	8.579	2326	2329	2331	rVB3	1789	1010	0.04%	0.005%
43	8.698	2364	2366	2367	rBV2	1343	655	0.03%	0.003%
44	8.875	2409	2421	2445	rVV	1211607	1947603	78.63%	9.572%
45	9.116	2491	2496	2498	rBV5	2020	1782	0.07%	0.009%
46	9.151	2503	2507	2509	rBV5	1951	1589	0.06%	0.008%
47	9.206	2519	2524	2527	rVB7	1832	1864	0.08%	0.009%
48	9.228	2529	2531	2533	rVV3	1780	908	0.04%	0.004%
49	9.241	2533	2535	2539	rVB4	2075	1210	0.05%	0.006%
50	9.296	2550	2552	2555	rBV5	1193	901	0.04%	0.004%
51	9.315	2555	2558	2559	rBV3	1723	861	0.03%	0.004%
52	9.437	2593	2596	2600	rBV5	2540	1958	0.08%	0.010%
53	9.457	2600	2602	2607	rVV5	1770	1477	0.06%	0.007%
54	9.486	2607	2611	2613	rVV5	1197	716	0.03%	0.004%
55	9.498	2613	2615	2617	rVV3	1307	580	0.02%	0.003%
56	9.695	2673	2676	2683	rVB7	2038	2179	0.09%	0.011%
57	9.765	2696	2698	2700	rBV3	1411	597	0.02%	0.003%
58	9.830	2716	2718	2721	rBV4	1399	772	0.03%	0.004%
59	9.878	2731	2733	2740	rVB8	2631	2464	0.10%	0.012%
60	9.923	2740	2747	2750	rBV9	1273	1702	0.07%	0.008%
61	9.958	2753	2758	2760	rBV4	2034	2021	0.08%	0.010%
62	10.045	2782	2785	2789	rVB6	1211	712	0.03%	0.003%
63	10.097	2798	2801	2802	rBV3	1107	731	0.03%	0.004%
64	10.125	2808	2810	2812	rBV2	1363	802	0.03%	0.004%
65	10.196	2827	2832	2833	rBV5	2011	2011	0.08%	0.010%
66	10.238	2833	2845	2866	rVV	818019	1266708	51.14%	6.226%
67	10.396	2888	2894	2895	rBV5	2381	2359	0.10%	0.012%
68	10.560	2939	2945	2948	rBV6	3533	3393	0.14%	0.017%
69	10.650	2971	2973	2976	rVV4	2230	1369	0.06%	0.007%
70	10.679	2980	2982	2989	rVB7	2161	2164	0.09%	0.011%
71	10.752	3003	3005	3009	rVB4	1541	935	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015388.D
 Acq On : 02 Apr 2020 22:04
 Operator : SY/MD
 Sample : VIBLK66
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK66

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

72	10.778	3009	3013	3015	rBV5	1695	1397	0.06%	0.007%
73	10.839	3028	3032	3036	rBV6	2273	1924	0.08%	0.009%
74	10.878	3037	3044	3046	rBV6	2845	2728	0.11%	0.013%
75	11.006	3082	3084	3090	rVB7	1617	1311	0.05%	0.006%
76	11.042	3090	3095	3096	rBV5	1029	872	0.04%	0.004%
77	11.090	3107	3110	3113	rBV4	1999	1449	0.06%	0.007%
78	11.106	3113	3115	3117	rVV3	1387	659	0.03%	0.003%
79	11.148	3125	3128	3130	rBV4	1805	1465	0.06%	0.007%
80	11.270	3155	3166	3182	rBV	1216076	1876494	75.76%	9.223%
81	11.498	3233	3237	3242	rVV7	1400	1199	0.05%	0.006%
82	11.521	3242	3244	3246	rBV2	1706	761	0.03%	0.004%
83	11.579	3260	3262	3264	rBV3	1559	913	0.04%	0.004%
84	11.646	3268	3283	3299	rBV	1228180	1942312	78.42%	9.546%
85	12.016	3395	3398	3399	rBV3	1661	839	0.03%	0.004%
86	12.164	3442	3444	3447	rVB4	1461	742	0.03%	0.004%
87	12.215	3458	3460	3463	rBV4	1001	658	0.03%	0.003%
88	12.434	3524	3528	3530	rBV4	1307	1111	0.04%	0.005%
89	12.492	3545	3546	3551	rVB4	2181	1148	0.05%	0.006%
90	12.540	3560	3561	3565	rBV4	1352	842	0.03%	0.004%
91	13.067	3721	3725	3728	rBV6	1855	1528	0.06%	0.008%
92	13.244	3778	3780	3782	rBV3	1452	808	0.03%	0.004%
93	13.389	3823	3825	3827	rBV3	1621	901	0.04%	0.004%
94	13.531	3861	3869	3885	rVB	141951	229030	9.25%	1.126%
95	13.903	3983	3985	3988	rBV3	1090	708	0.03%	0.003%
96	14.032	4021	4025	4027	rBV4	1725	1185	0.05%	0.006%
97	14.325	4114	4116	4120	rBV5	2519	1674	0.07%	0.008%
98	14.540	4179	4183	4185	rBV4	2312	1800	0.07%	0.009%
99	14.592	4195	4199	4201	rBV4	2460	1867	0.08%	0.009%
100	14.662	4212	4221	4236	rVB	41950	69867	2.82%	0.343%


Sum of corrected areas: 20346208

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV040220\
Data File : VV015388.D
Acq On : 02 Apr 2020 22:04
Operator : SY/MD
Sample : VIBLK66
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VIBLK66

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

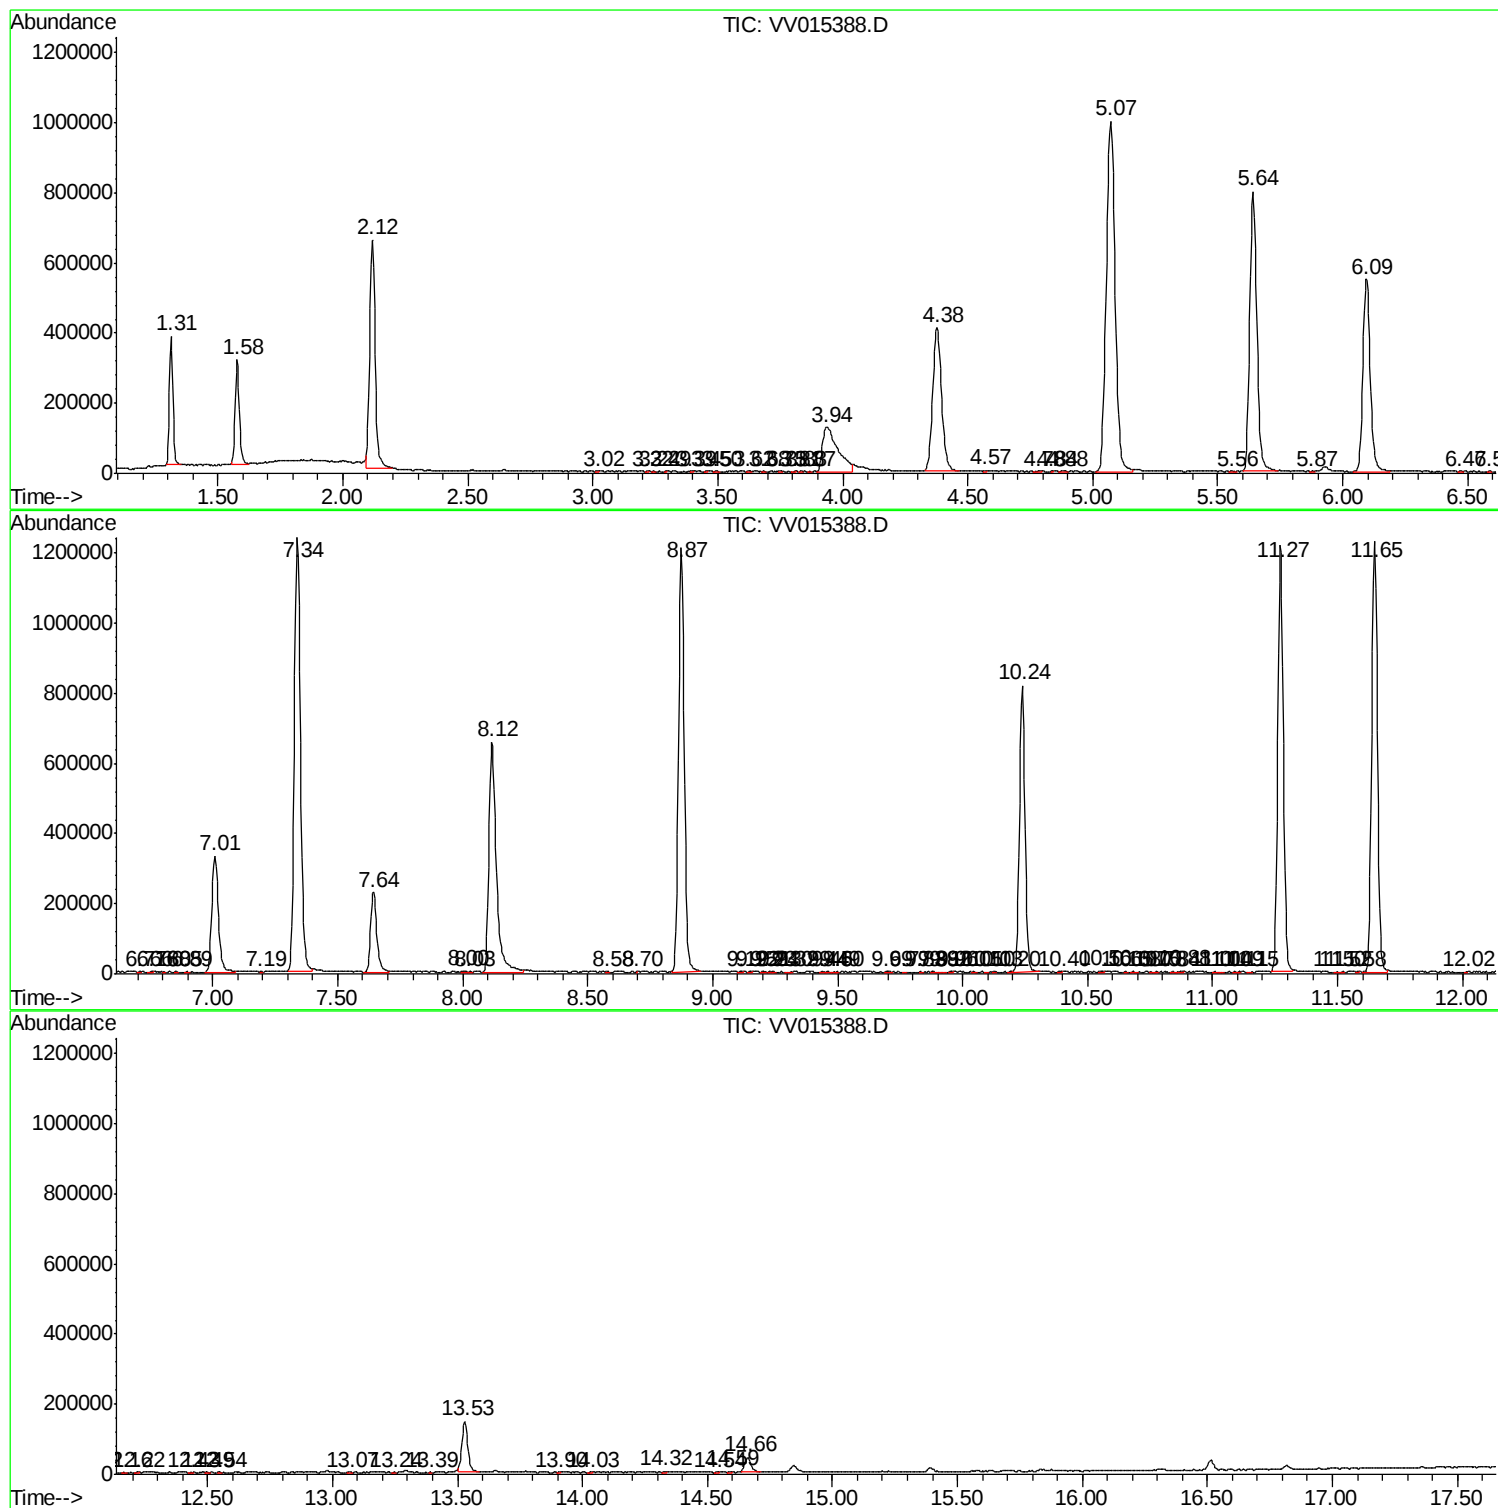

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV040220\
Data File : VV015388.D
Acq On : 02 Apr 2020 22:04
Operator : SY/MD
Sample : VIBLK66
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK66

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV040220\
Data File : VV015388.D
Acq On : 02 Apr 2020 22:04
Operator : SY/MD
Sample : VIBLK66
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK66

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc