

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015392.D
 Acq On : 02 Apr 2020 23:42
 Operator : SY/MD
 Sample : VIBLK67
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK67

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	63	70	87	rVB	356201	372944	15.89%	1.958%
2	1.576	145	151	166	rVB	288585	349157	14.88%	1.834%
3	2.116	312	319	332	rVB	645761	904856	38.56%	4.752%
4	2.936	572	574	578	rVB4	2672	1618	0.07%	0.008%
5	2.997	590	593	594	rBV3	1835	836	0.04%	0.004%
6	3.193	652	654	656	rBV3	1703	684	0.03%	0.004%
7	3.264	674	676	678	rVB3	2025	837	0.04%	0.004%
8	3.277	678	680	682	rBV3	1217	553	0.02%	0.003%
9	3.373	707	710	714	rBV5	1779	1408	0.06%	0.007%
10	3.428	724	727	729	rBV3	1456	1207	0.05%	0.006%
11	3.479	741	743	745	rBV3	942	666	0.03%	0.003%
12	3.631	788	790	792	rBV3	1343	488	0.02%	0.003%
13	3.714	814	816	819	rBV4	1352	806	0.03%	0.004%
14	3.759	825	830	832	rBV5	1327	1152	0.05%	0.006%
15	3.804	842	844	850	rBV5	1781	1627	0.07%	0.009%
16	3.936	874	885	926	rBV2	120660	530041	22.59%	2.783%
17	4.376	1006	1022	1050	rBV	382251	943876	40.23%	4.957%
18	4.766	1138	1143	1145	rBV3	2644	2005	0.09%	0.011%
19	5.071	1218	1238	1268	rBV2	943663	2346430	100.00%	12.322%
20	5.393	1335	1338	1340	rBV4	2203	1109	0.05%	0.006%
21	5.579	1394	1396	1398	rBV2	1450	639	0.03%	0.003%
22	5.640	1402	1415	1437	rBV	786246	1560581	66.51%	8.195%
23	6.026	1533	1535	1538	rBV3	1656	1235	0.05%	0.006%
24	6.093	1544	1556	1578	rBV	515801	1034425	44.09%	5.432%
25	6.302	1619	1621	1625	rVB5	1578	1032	0.04%	0.005%
26	6.344	1632	1634	1636	rBV3	1385	756	0.03%	0.004%
27	6.470	1671	1673	1677	rVB4	1783	1122	0.05%	0.006%
28	6.492	1678	1680	1682	rBV3	1091	658	0.03%	0.003%
29	6.544	1691	1696	1699	rBV7	2227	2148	0.09%	0.011%
30	6.560	1699	1701	1703	rBV3	1271	620	0.03%	0.003%
31	6.872	1796	1798	1799	rBV2	1052	511	0.02%	0.003%
32	7.010	1829	1841	1865	rBV	295435	542293	23.11%	2.848%
33	7.338	1931	1943	1978	rBV	1157857	1994379	85.00%	10.473%
34	7.643	2028	2038	2057	rBV	207843	353147	15.05%	1.854%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015392.D
 Acq On : 02 Apr 2020 23:42
 Operator : SY/MD
 Sample : VIBLK67
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK67

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

35	7.884	2111	2113	2117	rBV4	1414	1097	0.05%	0.006%
36	8.116	2175	2185	2216	rBV2	602800	1242909	52.97%	6.527%
37	8.537	2314	2316	2317	rBV2	2296	889	0.04%	0.005%
38	8.579	2327	2329	2330	rBV2	1160	390	0.02%	0.002%
39	8.627	2343	2344	2345	rBV	1245	399	0.02%	0.002%
40	8.688	2360	2363	2366	rBV5	1422	935	0.04%	0.005%
41	8.875	2409	2421	2443	rBV	1173571	1916647	81.68%	10.065%
42	9.199	2520	2522	2525	rBV3	1034	453	0.02%	0.002%
43	9.219	2525	2528	2530	rBV4	1206	657	0.03%	0.003%
44	9.244	2535	2536	2541	rVB4	1195	762	0.03%	0.004%
45	9.267	2541	2543	2545	rBV3	1326	763	0.03%	0.004%
46	9.405	2584	2586	2588	rBV3	958	432	0.02%	0.002%
47	9.434	2592	2595	2599	rVB6	1326	1073	0.05%	0.006%
48	9.521	2619	2622	2627	rBV6	2284	2305	0.10%	0.012%
49	9.563	2632	2635	2636	rBV2	2587	1271	0.05%	0.007%
50	9.643	2657	2660	2661	rBV3	942	366	0.02%	0.002%
51	9.675	2667	2670	2674	rBV3	1888	1529	0.07%	0.008%
52	9.746	2689	2692	2696	rBV5	1882	1771	0.08%	0.009%
53	9.897	2735	2739	2740	rBV2	1757	955	0.04%	0.005%
54	9.913	2740	2744	2747	rVV5	1635	1151	0.05%	0.006%
55	9.929	2747	2749	2751	rVV3	1014	457	0.02%	0.002%
56	9.994	2765	2769	2771	rBV5	702	618	0.03%	0.003%
57	10.023	2771	2778	2781	rBV7	1740	2054	0.09%	0.011%
58	10.100	2800	2802	2803	rBV2	767	313	0.01%	0.002%
59	10.238	2832	2845	2863	rBV	762367	1194995	50.93%	6.275%
60	10.515	2930	2931	2934	rBV2	857	530	0.02%	0.003%
61	10.563	2941	2946	2949	rBV7	1856	1934	0.08%	0.010%
62	10.595	2954	2956	2958	rBV3	1112	572	0.02%	0.003%
63	10.666	2976	2978	2981	rBV3	1698	978	0.04%	0.005%
64	10.743	2997	3002	3003	rBV3	1299	1178	0.05%	0.006%
65	10.772	3009	3011	3013	rBV3	1148	586	0.02%	0.003%
66	10.839	3029	3032	3033	rBV3	1032	478	0.02%	0.003%
67	10.904	3050	3052	3054	rBV3	976	409	0.02%	0.002%
68	11.006	3080	3084	3085	rBV3	1133	633	0.03%	0.003%
69	11.055	3097	3099	3100	rBV2	1103	399	0.02%	0.002%
70	11.167	3132	3134	3135	rBV2	1589	731	0.03%	0.004%
71	11.206	3144	3146	3149	rVB4	1959	956	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040220\
 Data File : VV015392.D
 Acq On : 02 Apr 2020 23:42
 Operator : SY/MD
 Sample : VIBLK67
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK67

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
 Title : VOC Analysis

72	11.273	3152	3167	3188	rBV	1203981	1852328	78.94%	9.727%
73	11.444	3218	3220	3223	rBV2	1573	955	0.04%	0.005%
74	11.540	3248	3250	3253	rBV4	1508	925	0.04%	0.005%
75	11.572	3258	3260	3264	rVB5	2013	1494	0.06%	0.008%
76	11.650	3269	3284	3302	rBV	1142432	1799676	76.70%	9.451%
77	11.884	3354	3357	3358	rBV3	1238	722	0.03%	0.004%
78	12.154	3438	3441	3443	rBV3	1797	970	0.04%	0.005%
79	12.222	3460	3462	3463	rBV2	535	270	0.01%	0.001%
80	12.231	3463	3465	3466	rVV2	519	185	0.01%	0.001%
81	12.318	3487	3492	3493	rBV5	2107	1866	0.08%	0.010%
82	12.421	3521	3524	3529	rBV7	1790	1497	0.06%	0.008%
83	12.482	3540	3543	3544	rBV2	691	521	0.02%	0.003%
84	12.566	3568	3569	3571	rVB2	1057	336	0.01%	0.002%
85	12.646	3592	3594	3599	rVB5	1687	994	0.04%	0.005%
86	12.817	3645	3647	3649	rBV4	1104	600	0.03%	0.003%
87	12.923	3678	3680	3682	rBV2	1138	472	0.02%	0.002%
88	12.965	3690	3693	3696	rBV5	1627	1207	0.05%	0.006%
89	13.029	3711	3713	3715	rBV3	992	366	0.02%	0.002%
90	13.045	3715	3718	3724	rVV6	1824	1502	0.06%	0.008%
91	13.276	3783	3790	3792	rBV7	2790	3704	0.16%	0.019%
92	13.392	3823	3826	3830	rBV4	1882	1199	0.05%	0.006%
93	13.530	3862	3869	3880	rBV	11186	17093	0.73%	0.090%
94	13.881	3975	3978	3979	rBV3	1512	758	0.03%	0.004%
95	13.958	4000	4002	4008	rVB7	1988	1285	0.05%	0.007%
96	13.990	4009	4012	4018	rBV7	2070	2446	0.10%	0.013%
97	14.170	4065	4068	4071	rBV4	2355	1483	0.06%	0.008%
98	14.482	4162	4165	4167	rBV4	2534	2015	0.09%	0.011%
99	15.360	4435	4438	4441	rVB	10597	5718	0.24%	0.030%


Sum of corrected areas: 19043008

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV040220\
Data File : VV015392.D
Acq On : 02 Apr 2020 23:42
Operator : SY/MD
Sample : VIBLK67
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK67

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

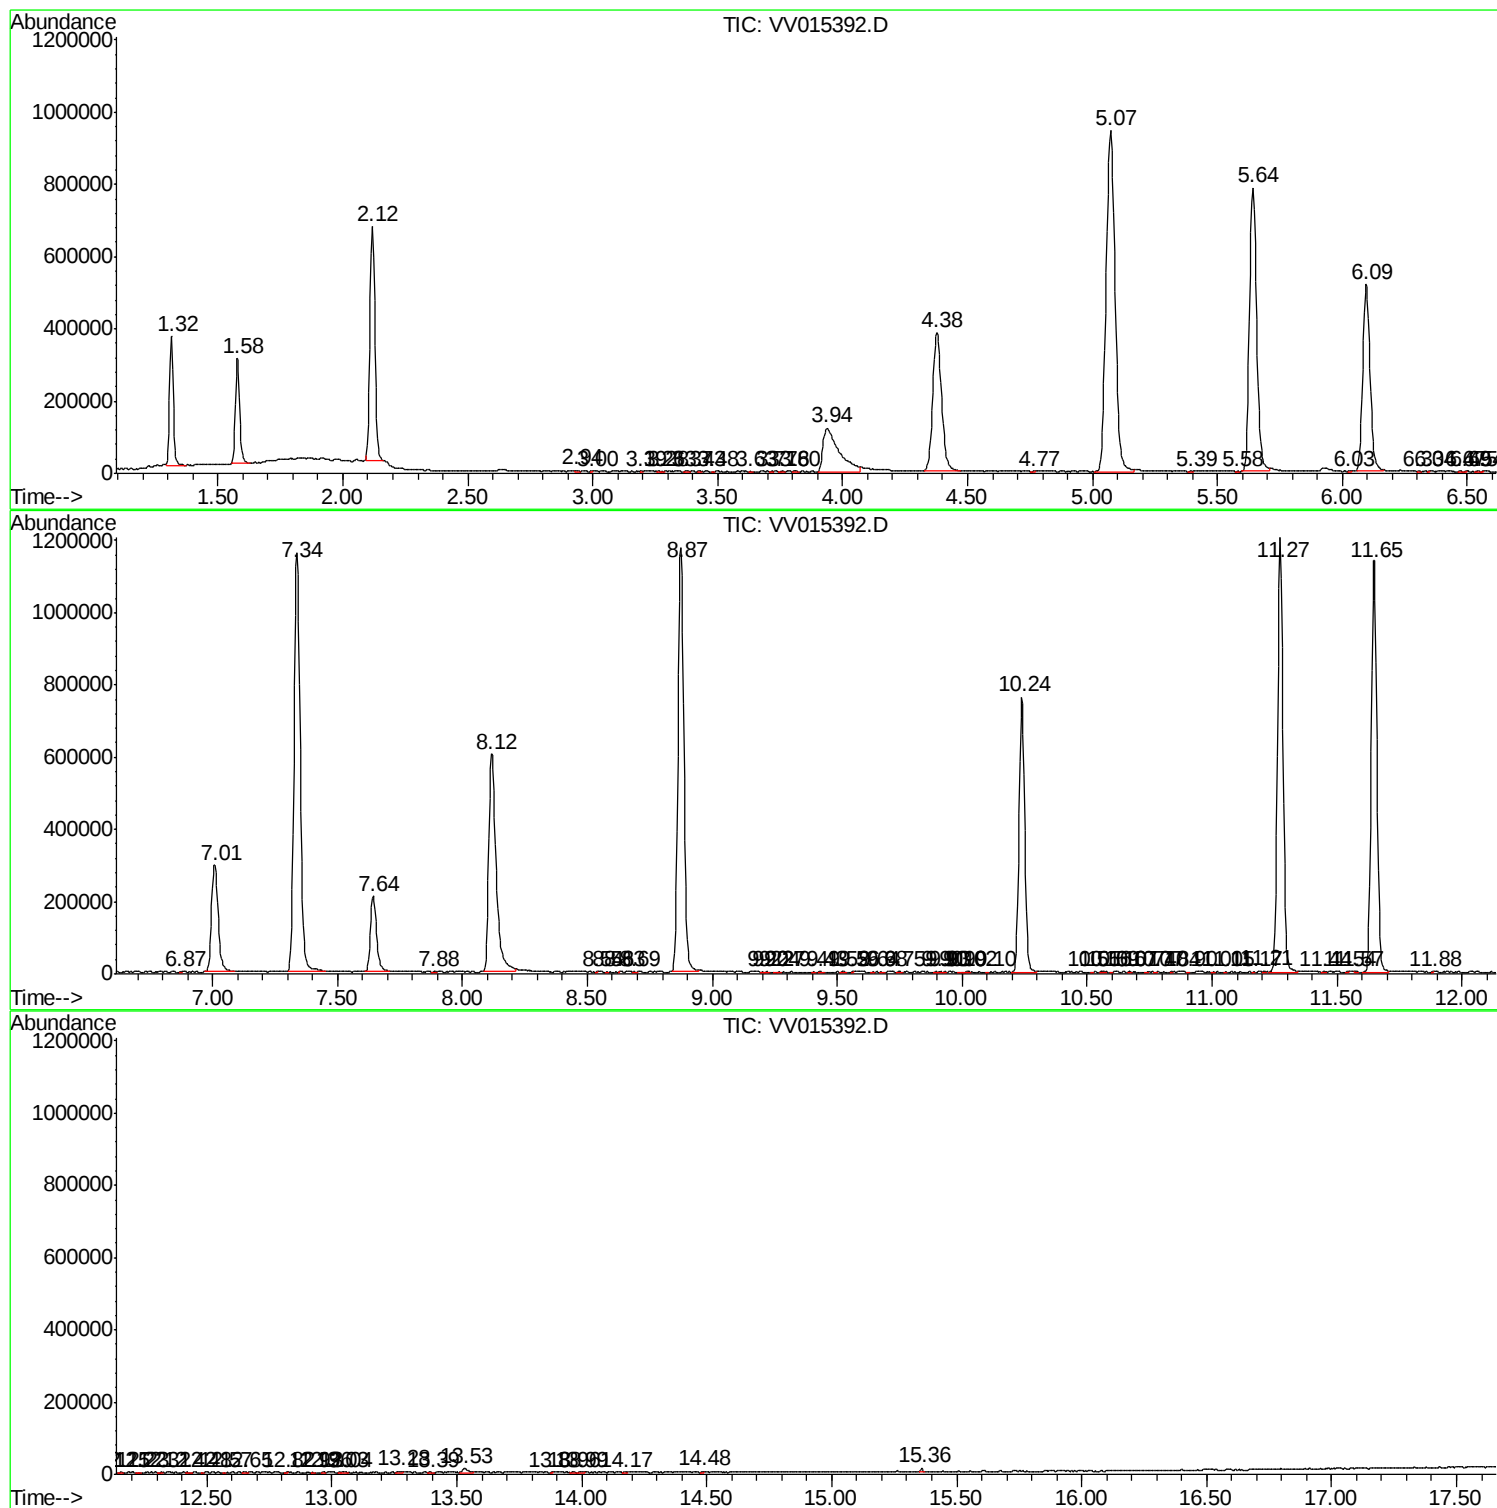

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV040220\
Data File : VV015392.D
Acq On : 02 Apr 2020 23:42
Operator : SY/MD
Sample : VIBLK67
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK67

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV040220\
Data File : VV015392.D
Acq On : 02 Apr 2020 23:42
Operator : SY/MD
Sample : VIBLK67
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK67

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM040120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc